


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM112318\
Data File : BM017755.D
Acq On : 23 Nov 2018 11:17
Operator : MJ/SJ
Sample : J6036-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0923

Quant Time: Nov 26 03:46:17 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 23 21:57:24 2018
Response via : Initial Calibration

Manual Integrations
APPROVED

MOHAMMAD
11/26/2018 3:05:06 PM

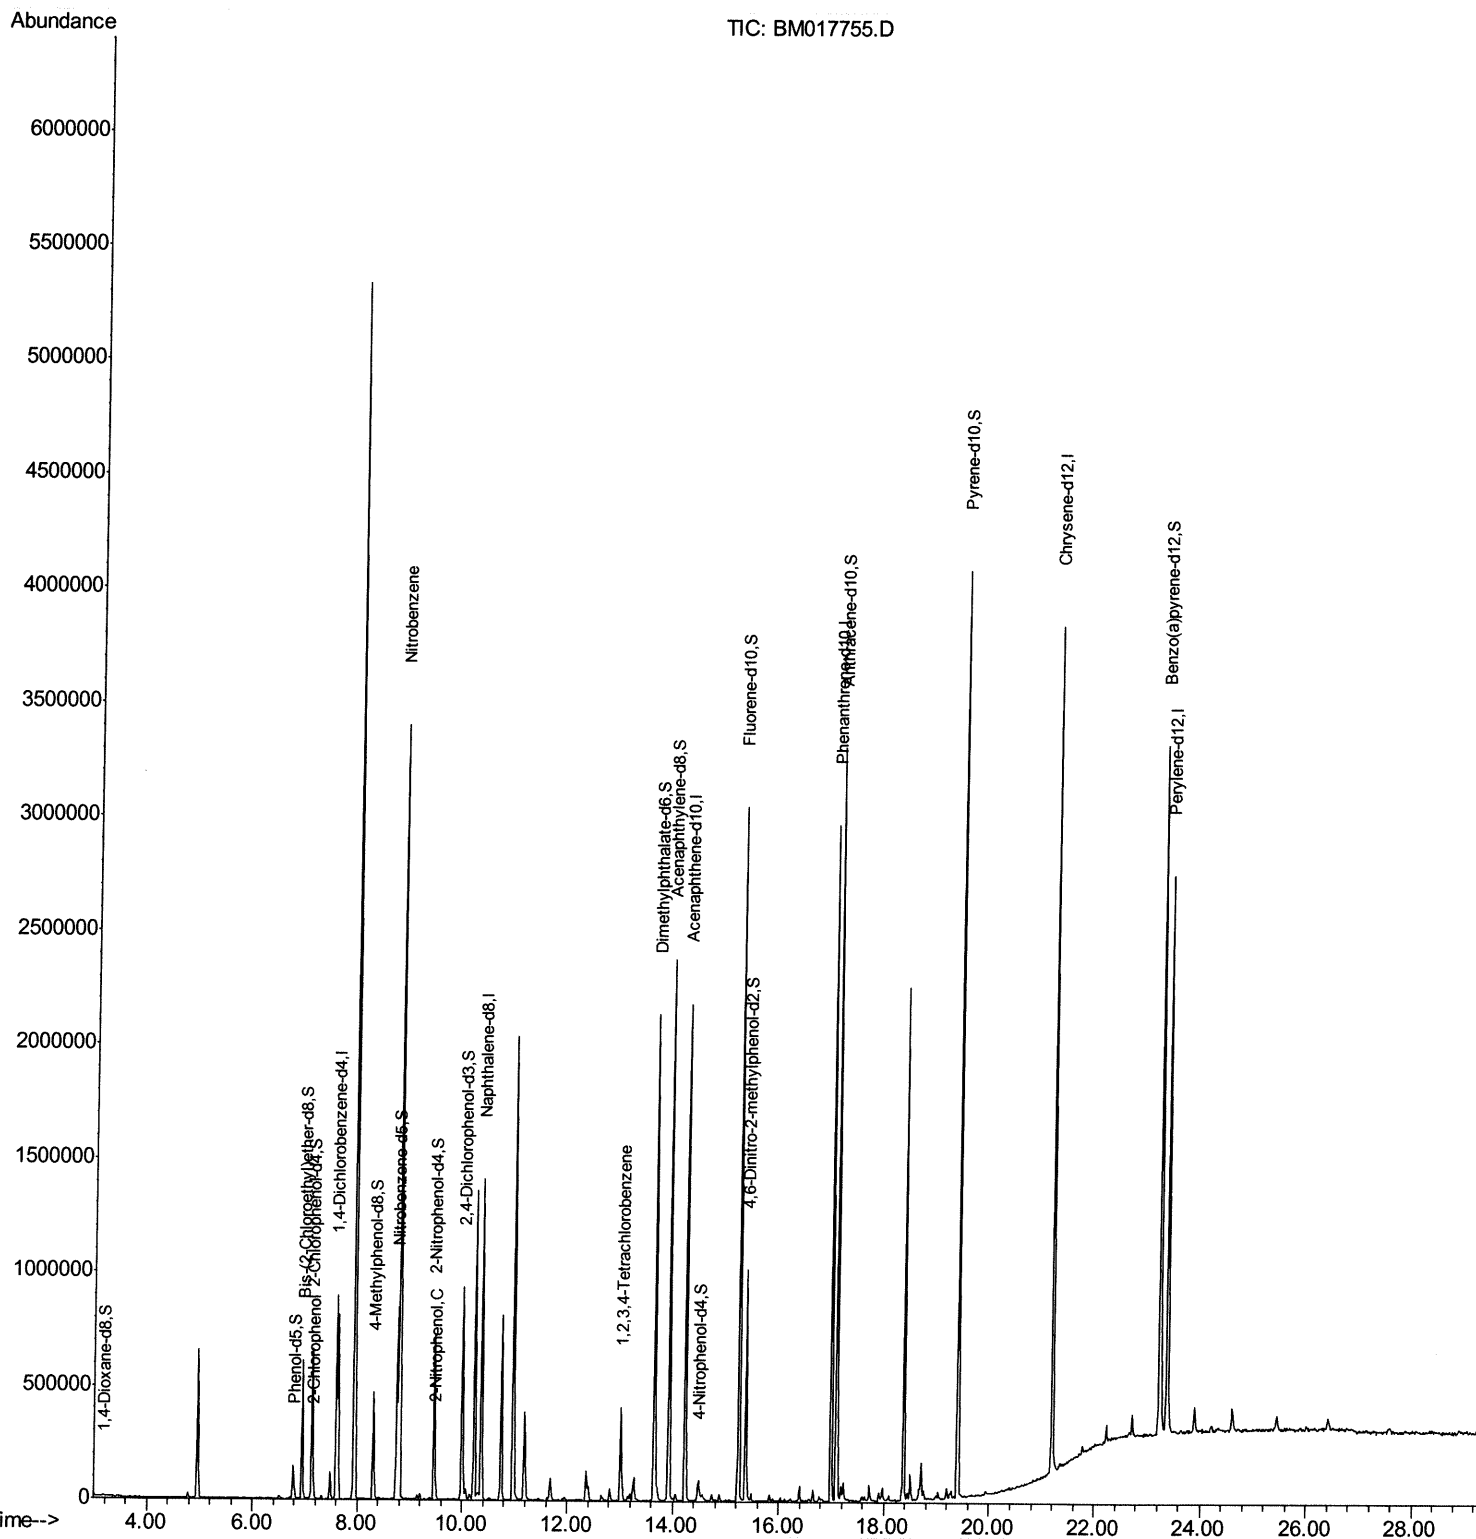




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM112318\
 Data File : BM017755.D
 Acq On : 23 Nov 2018 11:17
 Operator : MJ/SJ
 Sample : J6036-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0923

Manual Integrations
 APPROVED

MOHAMMAD
 11/26/2018 3:05:06 PM

Quant Time: Nov 26 03:46:17 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 23 21:57:24 2018
 Response via : Initial Calibration

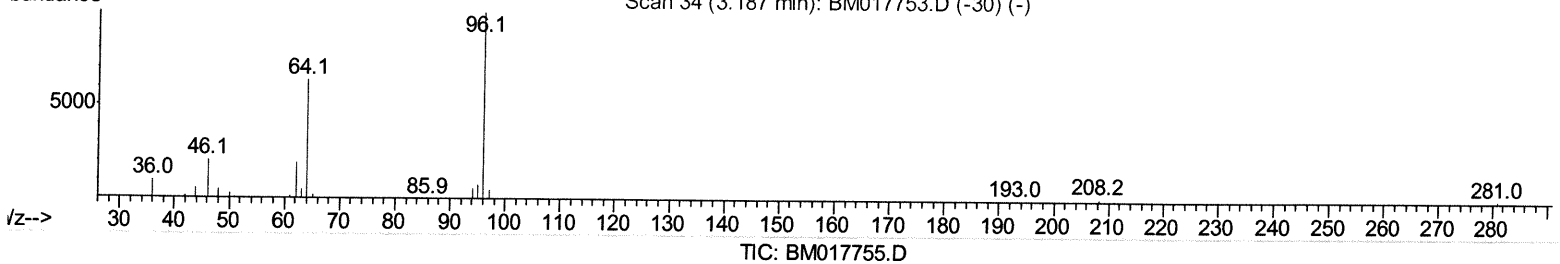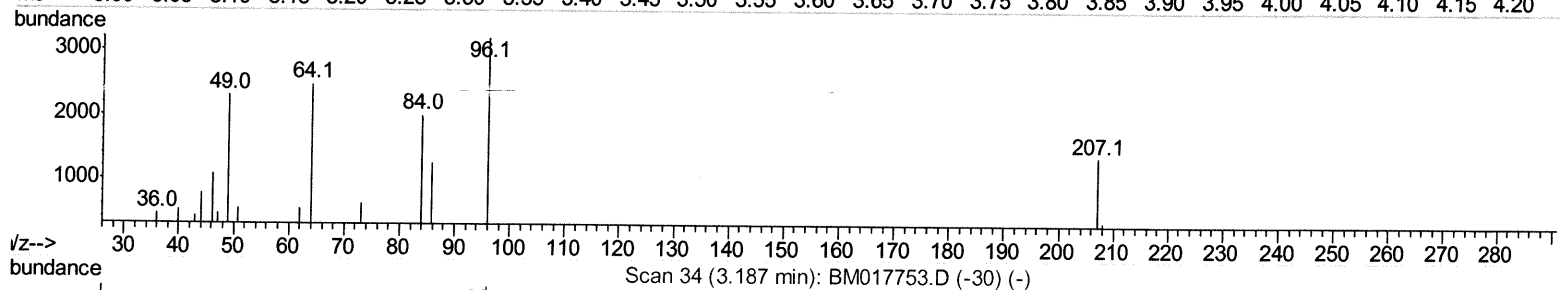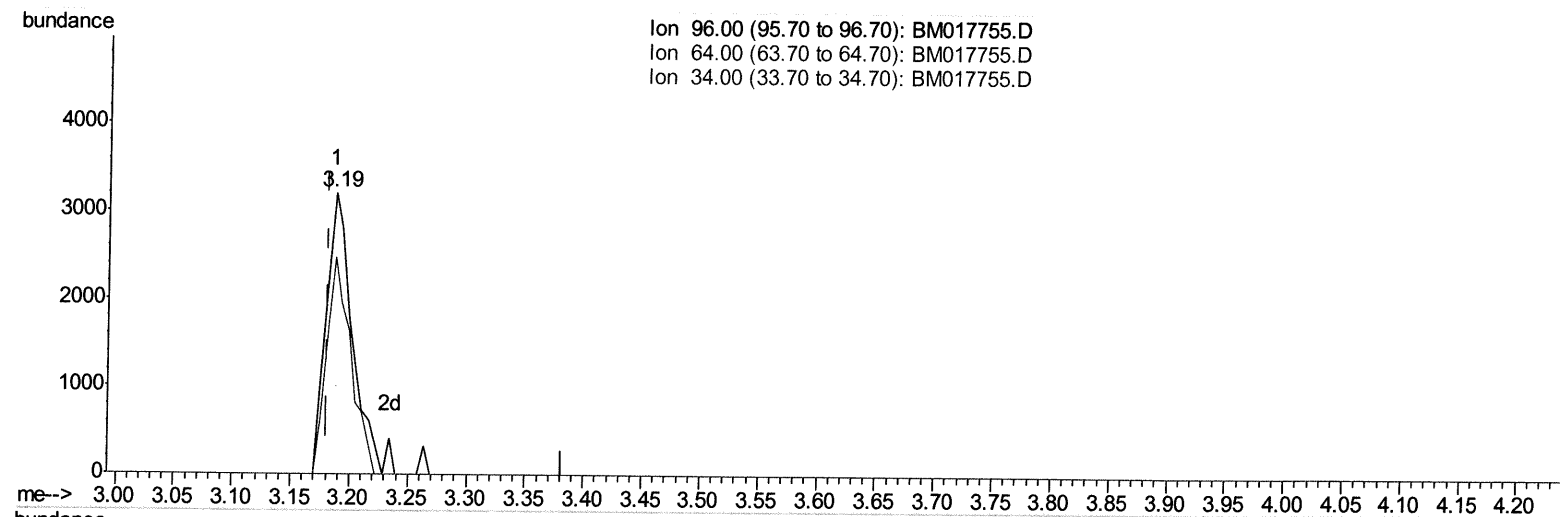

(3) 1,4-Dioxane-d8 (S)

3.187min (+0.006) 1.02ng/uL m

response 5117

Jul 11/28/18

Ion	Exp%	Act%
96.00	100	100
64.00	68.40	77.28
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM112318\
 Data File : BM017755.D
 Acq On : 23 Nov 2018 11:17
 Operator : MJ/SJ
 Sample : J6036-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0923

Manual Integrations
 APPROVED

MOHAMMAD
 11/26/2018 3:05:06 PM

Quant Time: Nov 26 03:46:17 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 23 21:57:24 2018
 Response via : Initial Calibration

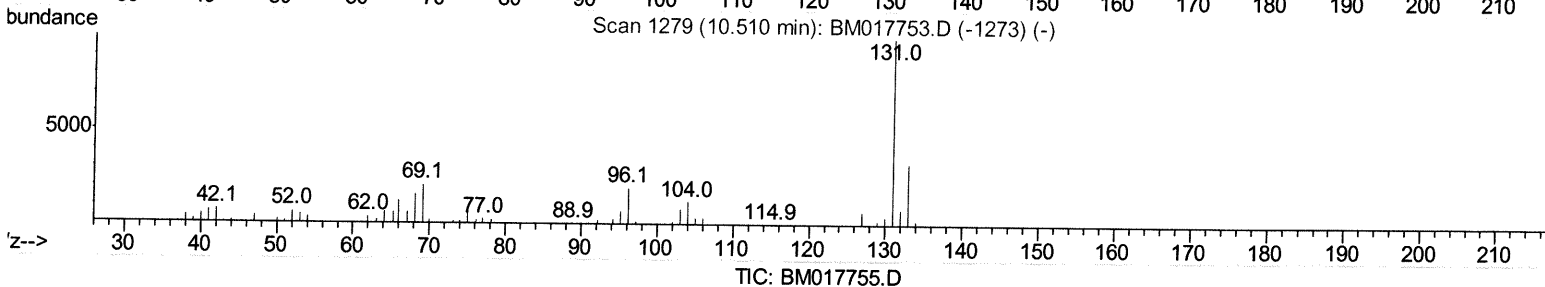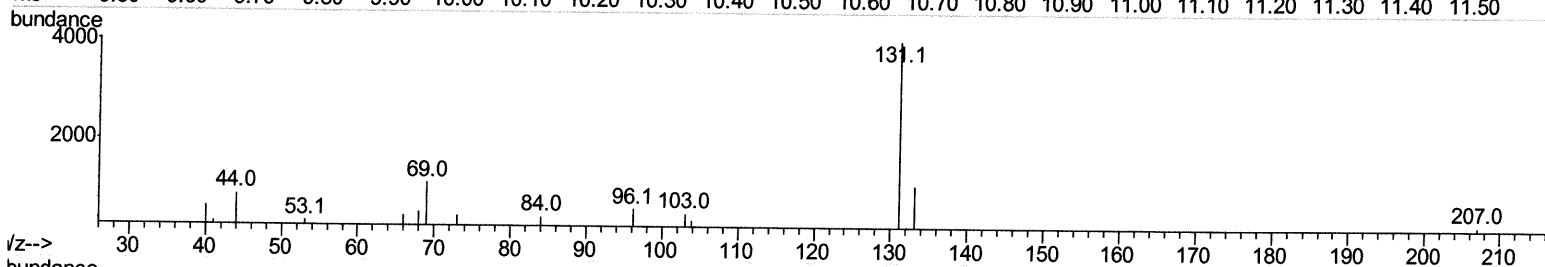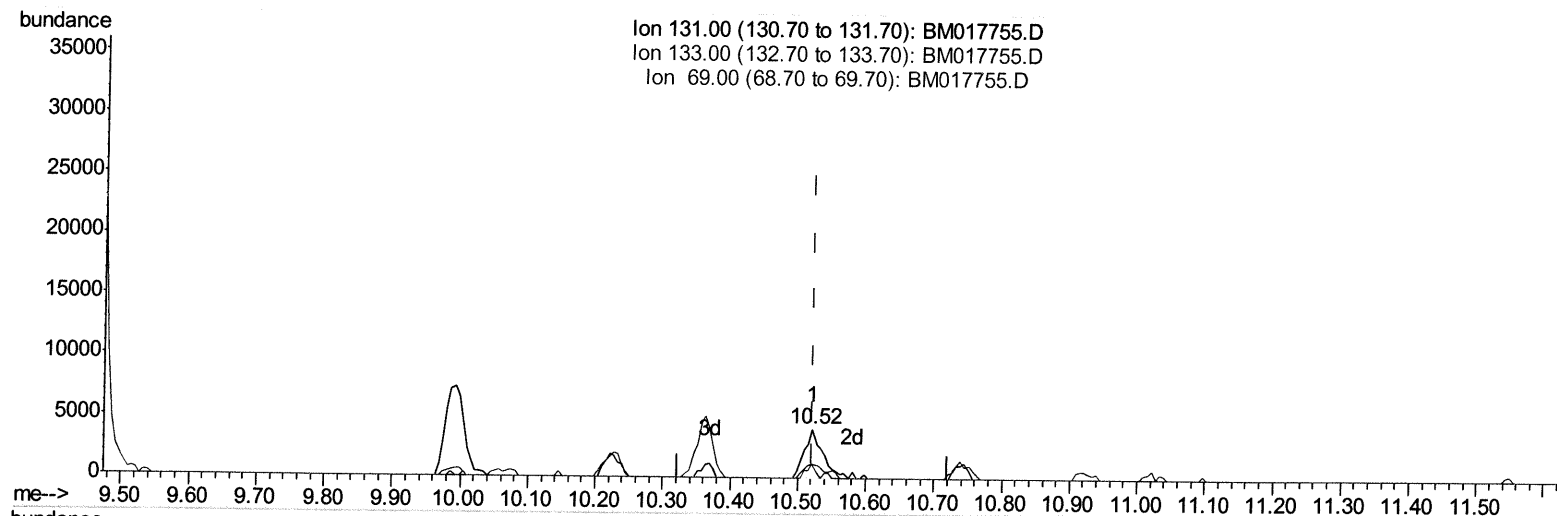

(29) 4-Chloroaniline-d4 (S)

10.522min (-0.000) 0.48ng/ul m

response 7723

Je 11/28/18

Ion	Exp%	Act%
131.00	100	100
133.00	32.40	28.36
69.00	18.90	29.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM112318\
 Data File : BM017755.D
 Acq On : 23 Nov 2018 11:17
 Operator : MJ/SJ
 Sample : J6036-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 C0923

Manual Integrations
 APPROVED

MOHAMMAD
 11/26/2018 3:05:06 PM

Quant Time: Nov 26 03:46:17 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 23 21:57:24 2018
 Response via : Initial Calibration

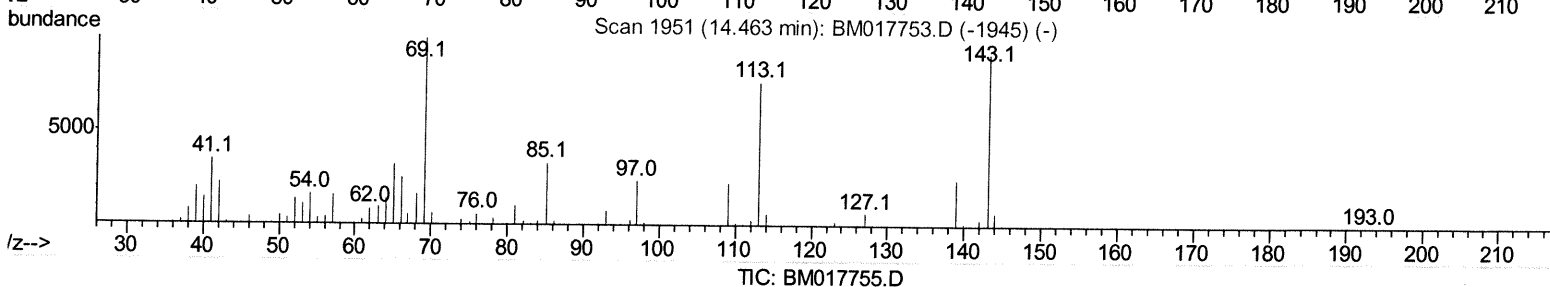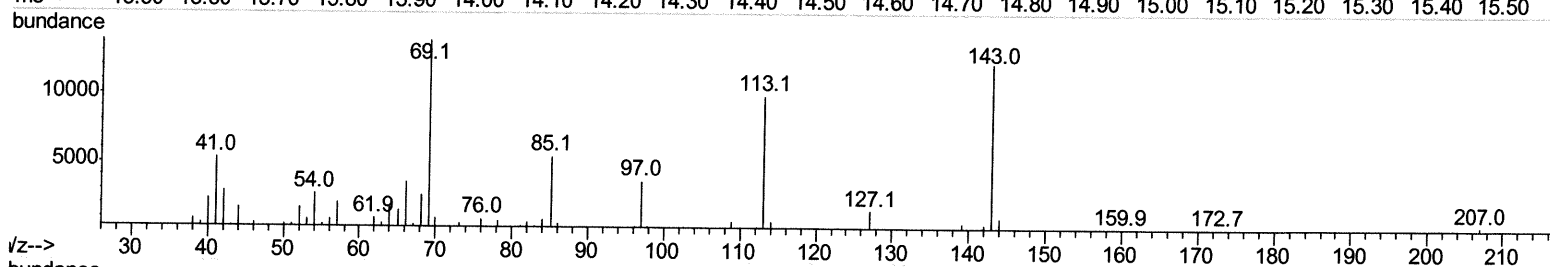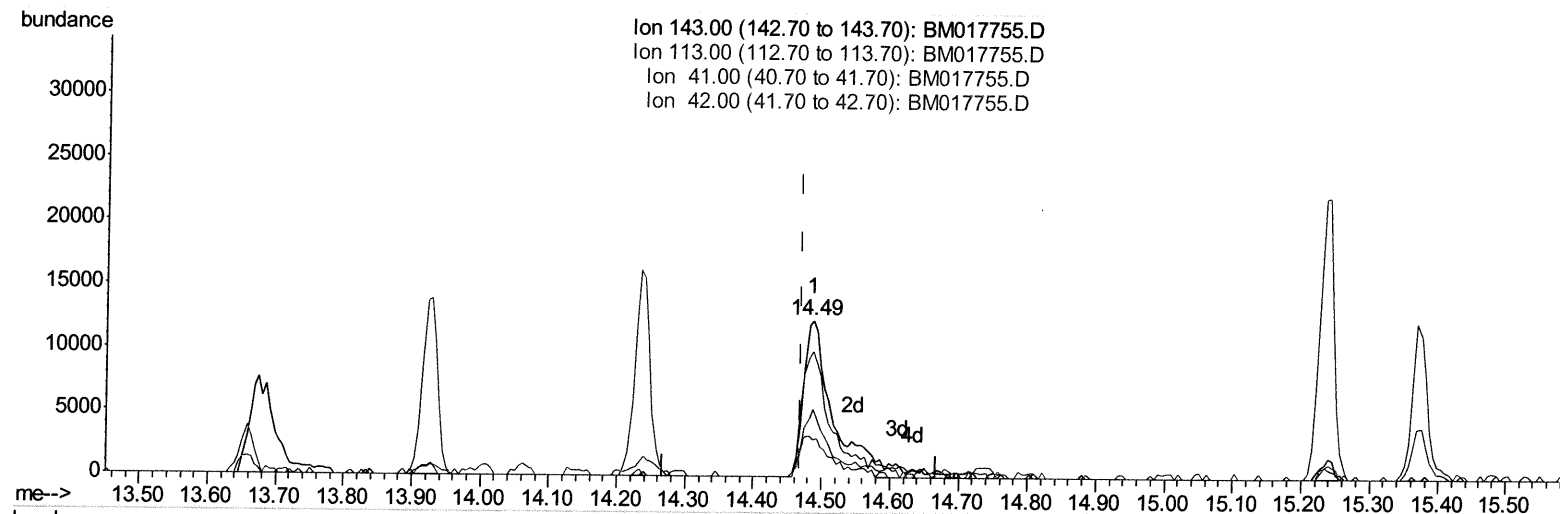

(51) 4-Nitrophenol-d4 (S)

14.486min (+0.017) 3.29ng/ul m

response 35755

Ju a / 28/18

Ion	Exp%	Act%
143.00	100	100
113.00	79.10	80.59
41.00	40.10	43.16
42.00	26.80	23.70




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM112318\
 Data File : BM017755.D
 Acq On : 23 Nov 2018 11:17
 Operator : MJ/SJ
 Sample : J6036-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0923

Manual Integrations
 APPROVED

MOHAMMAD
 11/26/2018 3:05:06 PM

Quant Time: Nov 28 16:05:56 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 28 15:59:26 2018
 Response via : Initial Calibration

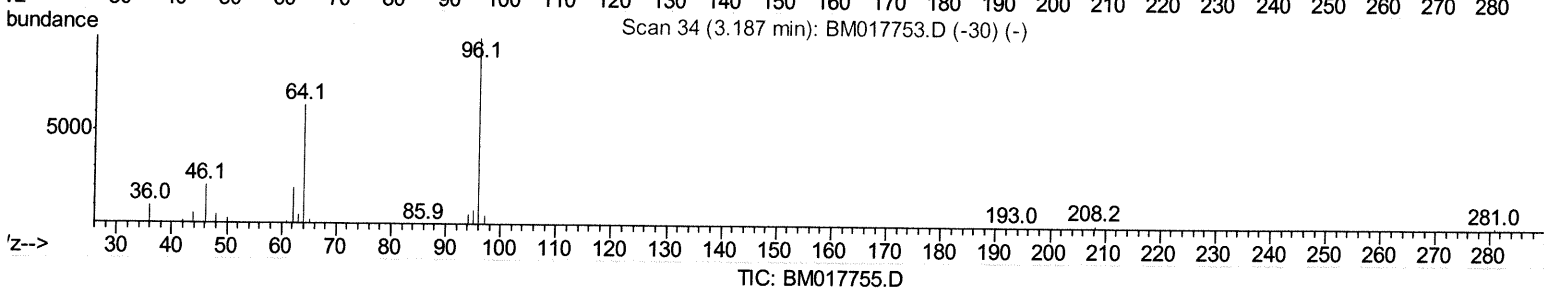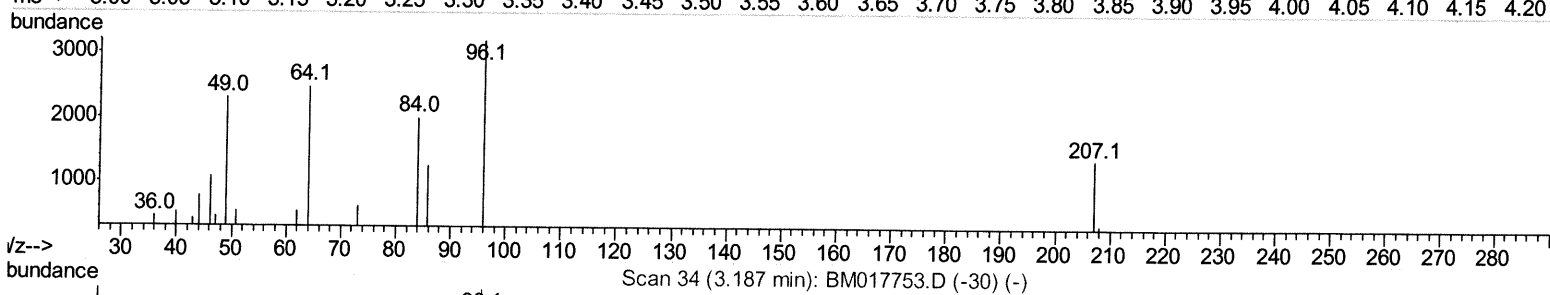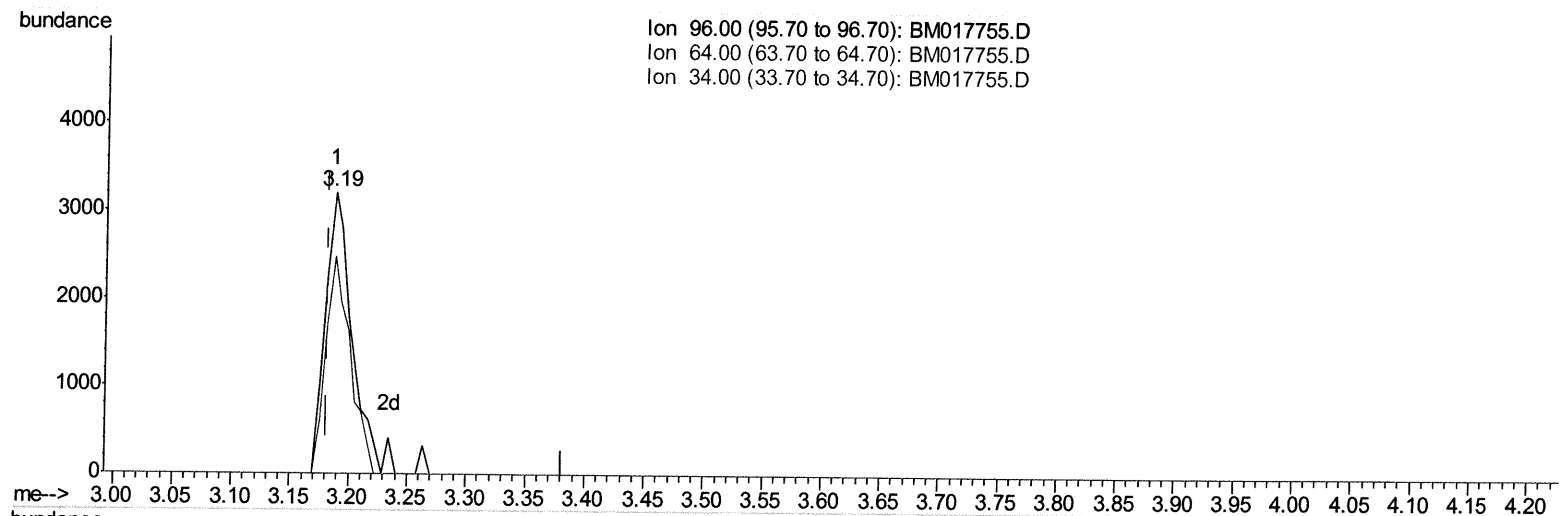

(3) 1,4-Dioxane-d8 (S)

3.187min (+0.006) 1.00ng/uL

response 4972

Ion	Exp%	Act%
96.00	100	100
64.00	68.40	77.28
34.00	0.00	0.00
0.00	0.00	0.00


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM112318\
 Data File : BM017755.D
 Acq On : 23 Nov 2018 11:17
 Operator : MJ/SJ
 Sample : J6036-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0923

Manual Integrations
 APPROVED

MOHAMMAD
 11/26/2018 3:05:06 PM

Quant Time: Nov 28 16:05:56 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 28 15:59:26 2018
 Response via : Initial Calibration

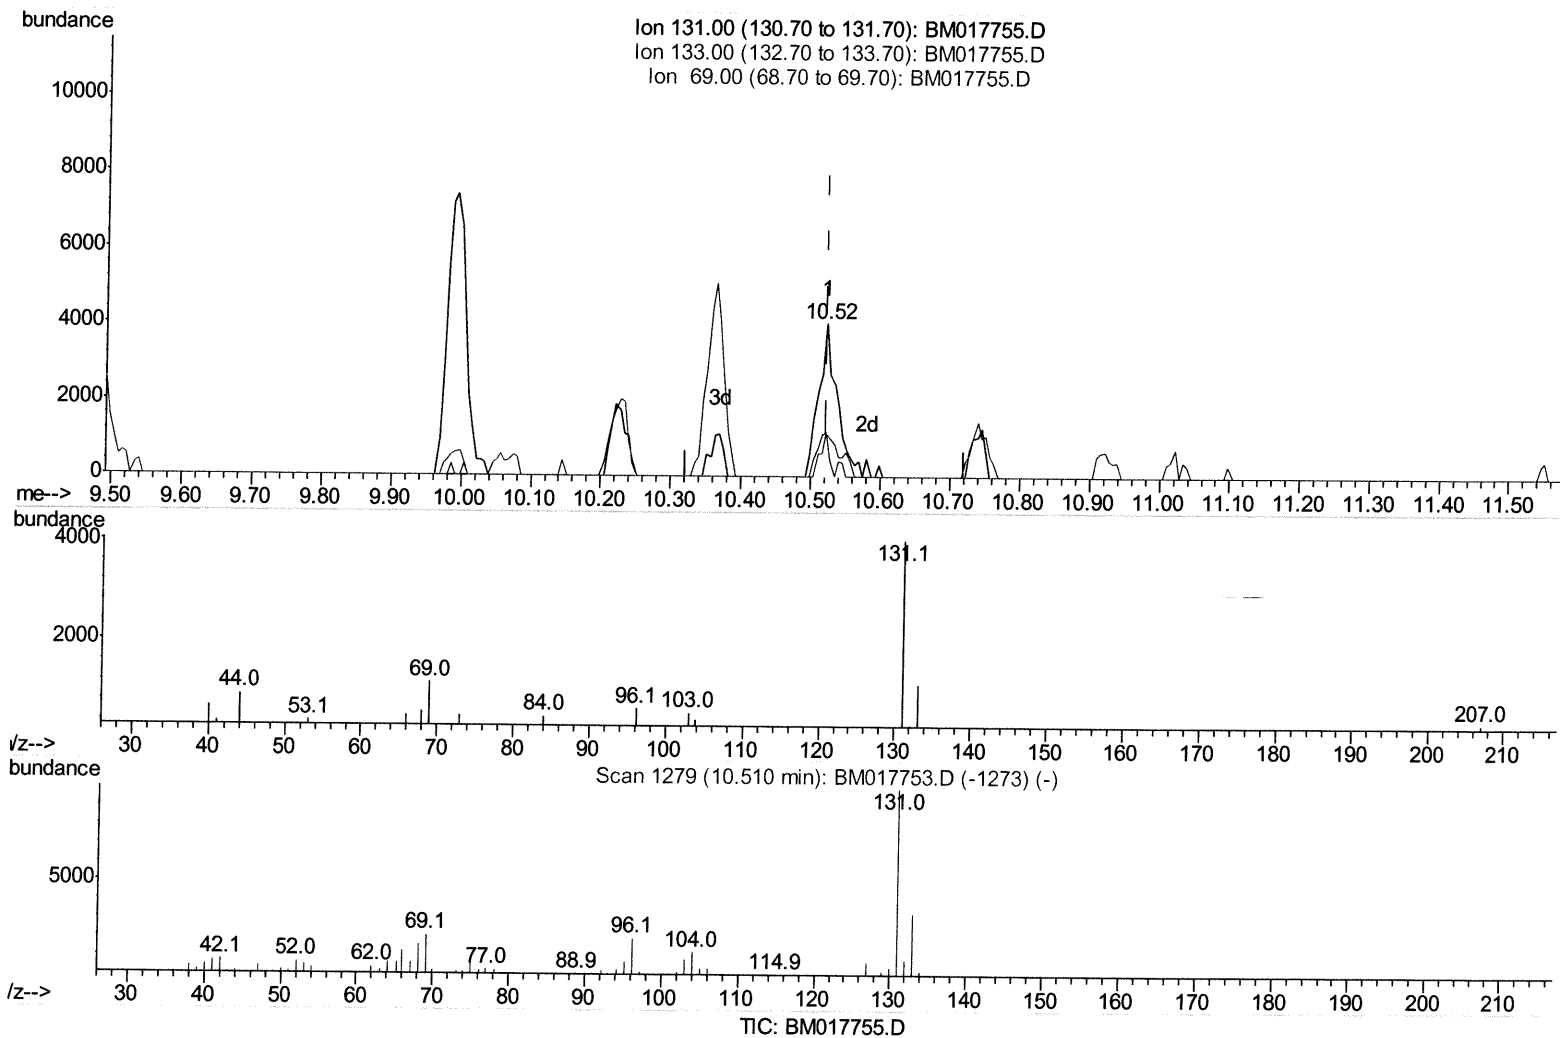

(29) 4-Chloroaniline-d4 (S)

10.522min (-0.000) 0.46ng/ul

response 7443

Ion	Exp%	Act%
131.00	100	100
133.00	32.40	28.36
69.00	18.90	29.00#
0.00	0.00	0.00


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM112318\
Data File : BM017755.D
Acq On : 23 Nov 2018 11:17
Operator : MJ/SJ
Sample : J6036-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
C0923

Manual Integrations
APPROVED

MOHAMMAD
11/26/2018 3:05:06 PM

Quant Time: Nov 28 16:05:56 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 28 15:59:26 2018
Response via : Initial Calibration

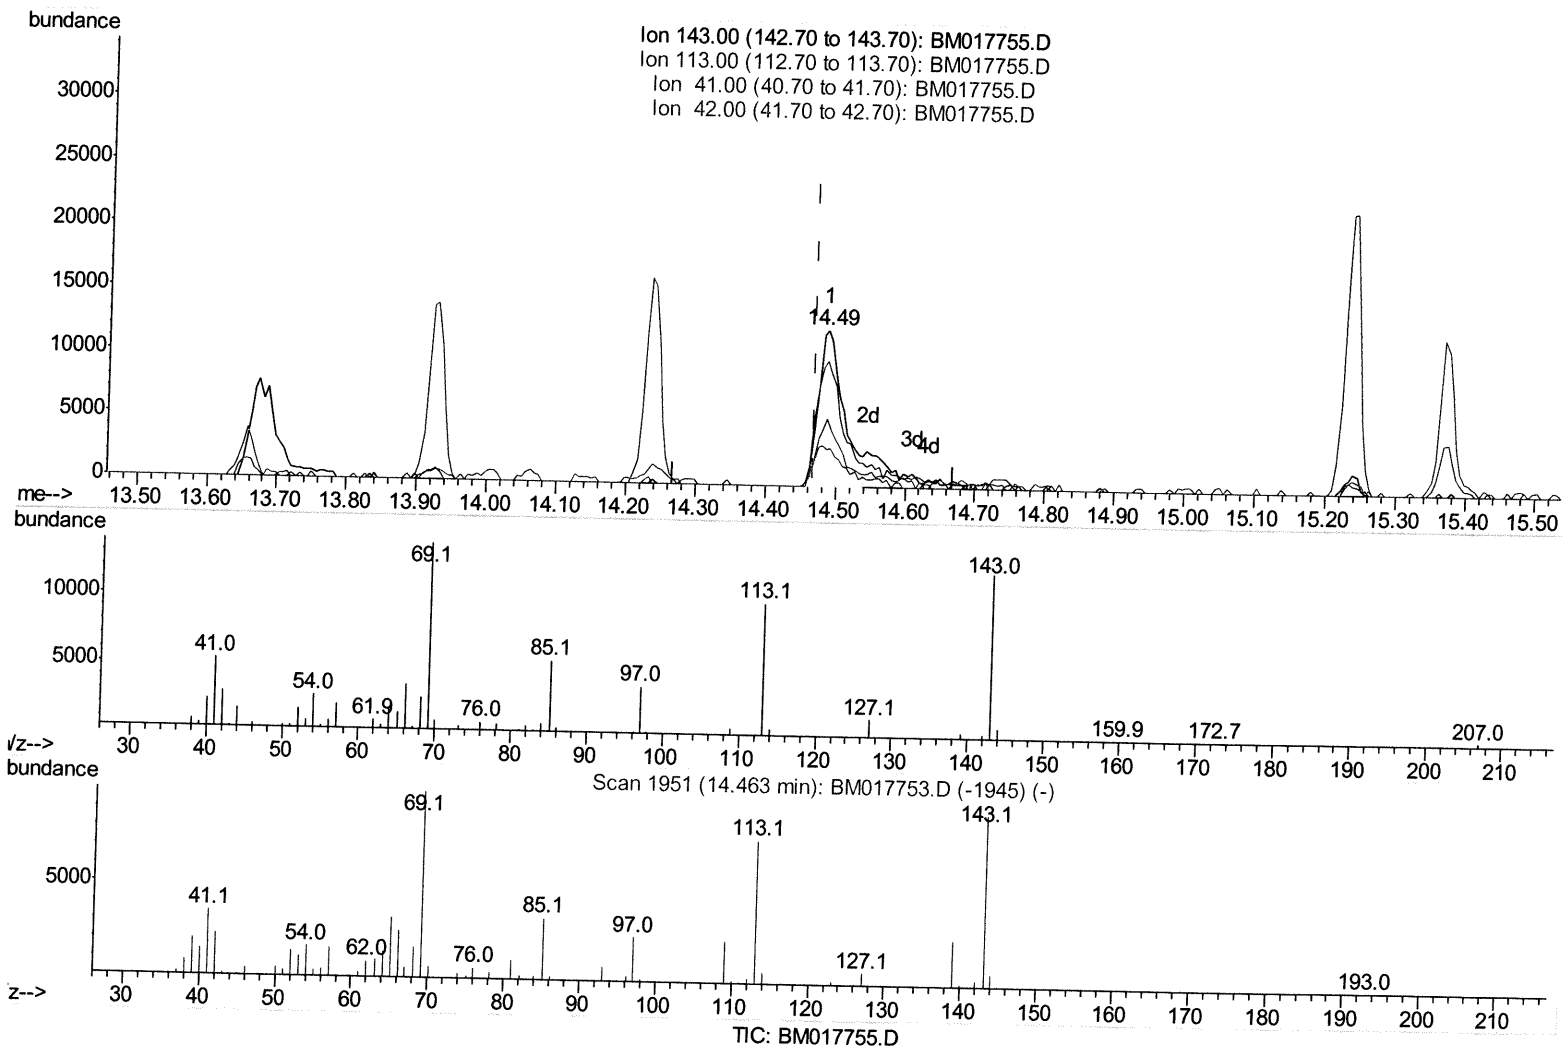

(51) 4-Nitrophenol-d4 (S)

14.486min (+0.017) 2.80ng/ul

response 30419

Ion	Exp%	Act%
143.00	100	100
113.00	79.10	80.59
41.00	40.10	43.16
42.00	26.80	23.70

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM112318\
 Data File : BM017755.D
 Acq On : 23 Nov 2018 11:17
 Operator : MJ/SJ
 Sample : J6036-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0923

Manual Integrations
 APPROVED

MOHAMMAD
 11/26/2018 3:05:06 PM

Quant Time: Nov 26 03:46:17 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 23 21:57:24 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	228501	20.00	ng/ul	0.00
18) Naphthalene-d8	10.36	136	1116107	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.24	164	689249	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.99	188	1601576	20.00	ng/ul	0.00
77) Chrysene-d12	21.20	240	1780866	20.00	ng/ul	0.00
85) Perylene-d12	23.38	264	1760267	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.19	96	5117m>	1.02	ng/uL	> 0.00	> Jc 11/28/18
5) Phenol-d5	6.78	99	90196	4.32	ng/ul	0.00	
7) Bis-(2-Chloroethyl)ether-d	6.94	67	267802	21.28	ng/ul	0.00	
9) 2-Chlorophenol-d4	7.13	132	291422	17.85	ng/ul	0.00	
13) 4-Methylphenol-d8	8.30	113	189446	11.11	ng/ul	0.00	
19) Nitrobenzene-d5	8.75	128	189789	22.14	ng/ul	0.00	
22) 2-Nitrophenol-d4	9.46	143	216854	22.08	ng/ul	0.00	
26) 2,4-Dichlorophenol-d3	9.99	165	359310	19.22	ng/ul	0.00	
29) 4-Chloroaniline-d4	10.52	131	7723m>	0.48	ng/ul	> 0.00	> Jc 11/28/18
43) Dimethylphthalate-d6	13.66	166	1357594	22.70	ng/ul	0.00	
46) Acenaphthylene-d8	13.93	160	1611202	22.26	ng/ul	0.00	
51) 4-Nitrophenol-d4	14.49	143	35755m>	3.29	ng/ul	> 0.02	> Jc 11/28/18
57) Fluorene-d10	15.24	176	1163603	22.53	ng/ul	0.00	
62) 4,6-Dinitro-2-methylphenol	15.37	200	217457	18.99	ng/ul	0.00	
70) Anthracene-d10	17.09	188	1809223	22.69	ng/ul	0.00	
78) Pyrene-d10	19.39	212	2046470	23.75	ng/ul	0.00	
89) Benzo(a)pyrene-d12	23.24	264	2167549	22.70	ng/ul	-0.01	

Target Compounds

					Ovalue	
10) 2-Chlorophenol	7.16	128	36352	2.228	ng/ul	96
20) Nitrobenzene	8.79	77	1834760	85.269	ng/ul	97
23) 2-Nitrophenol	9.49	139	16512	1.615	ng/ul	97
72) 1,2,3,4-Tetrachlorobenzene	13.02	216	127403	5.613	ng/uL	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed