


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM112320\
Data File : BM027914.D
Acq On : 23 Nov 2020 15:35
Operator : JU/CG
Sample : L4711-11DL 5X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0B55DL

Manual Integrations
APPROVED

mohammad
11/25/2020 12:44:33 PM

Quant Time: Nov 23 16:10:43 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM112020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 23 11:35:49 2020
Response via : Initial Calibration

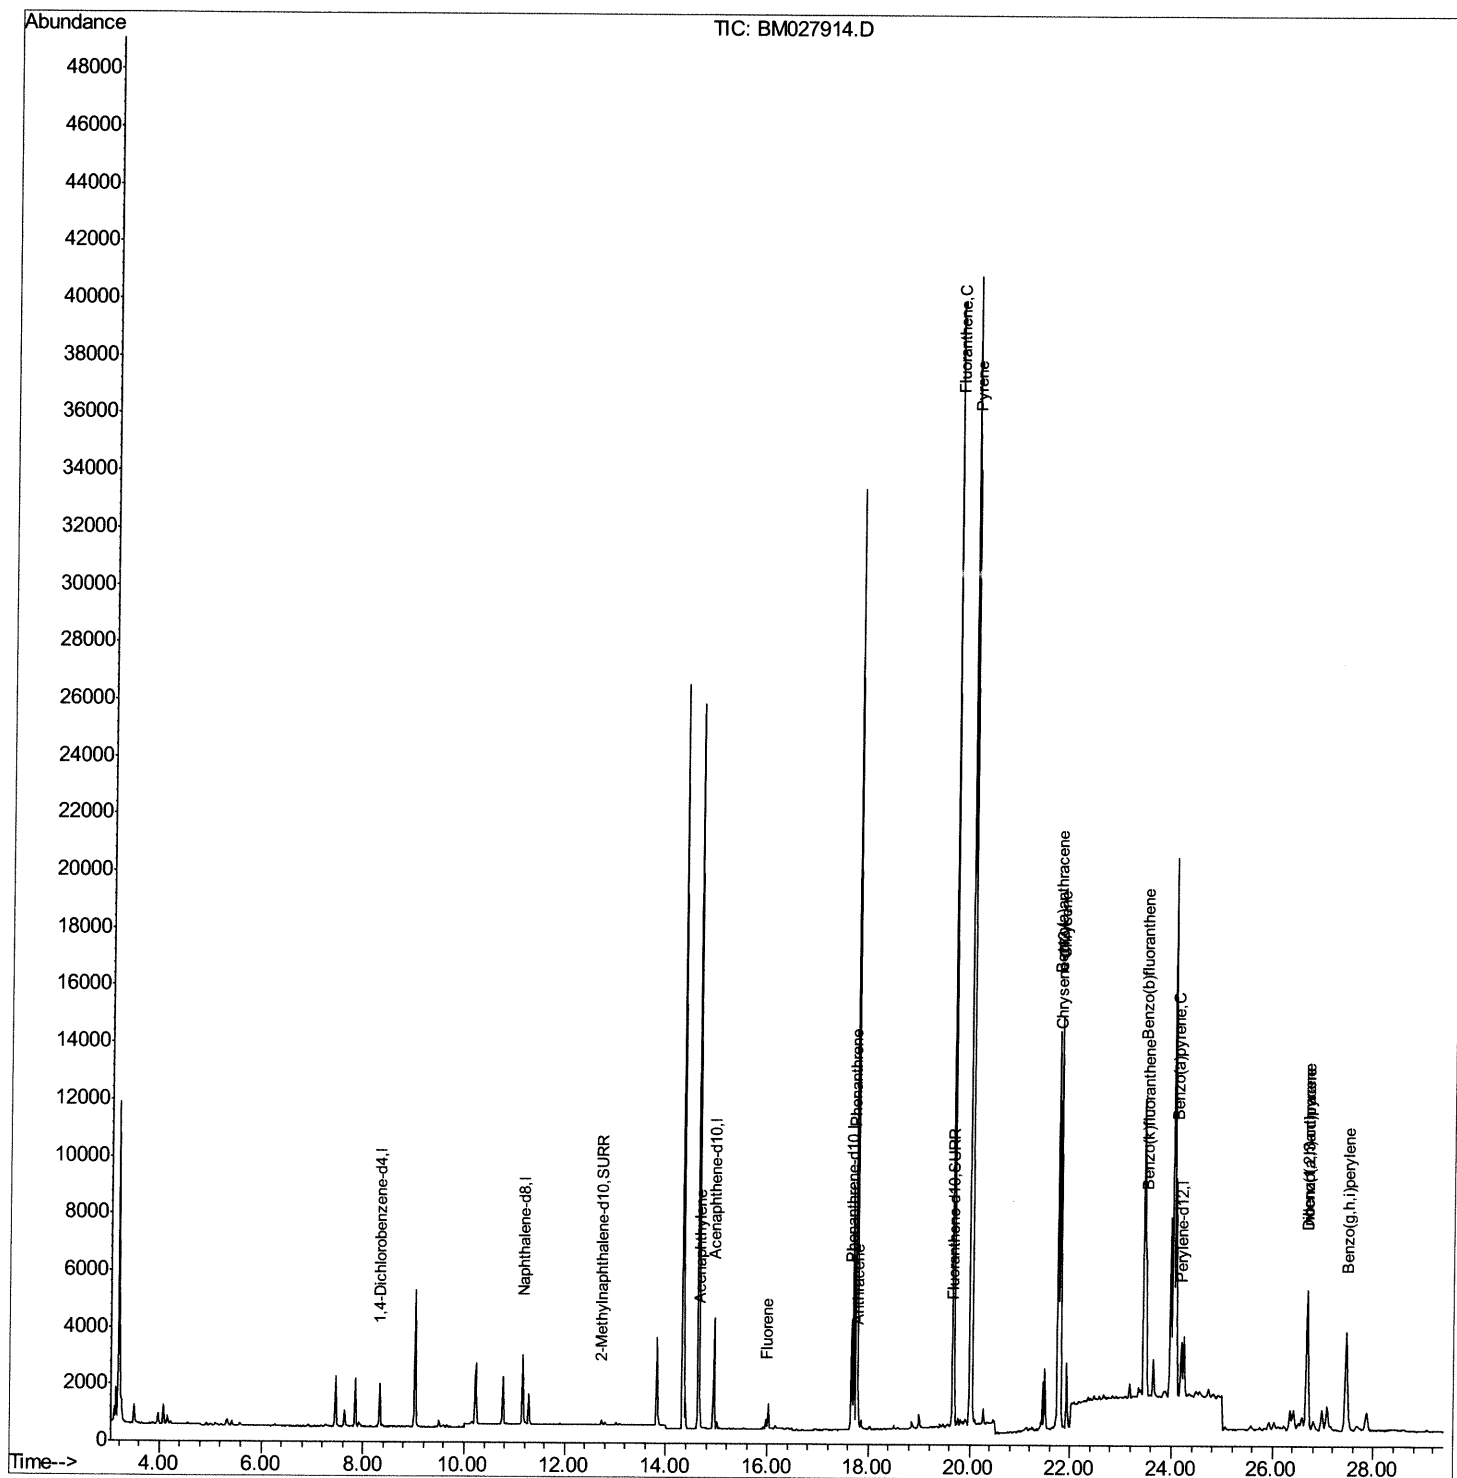

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM112320\
 Data File : BM027914.D
 Acq On : 23 Nov 2020 15:35
 Operator : JU/CG
 Sample : L4711-11DL 5X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0B55DL

Manual Integrations
 APPROVED

mohammad
 11/25/2020 12:44:33 PM

Quant Time: Nov 23 16:09:26 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM112020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 23 11:35:49 2020
 Response via : Initial Calibration

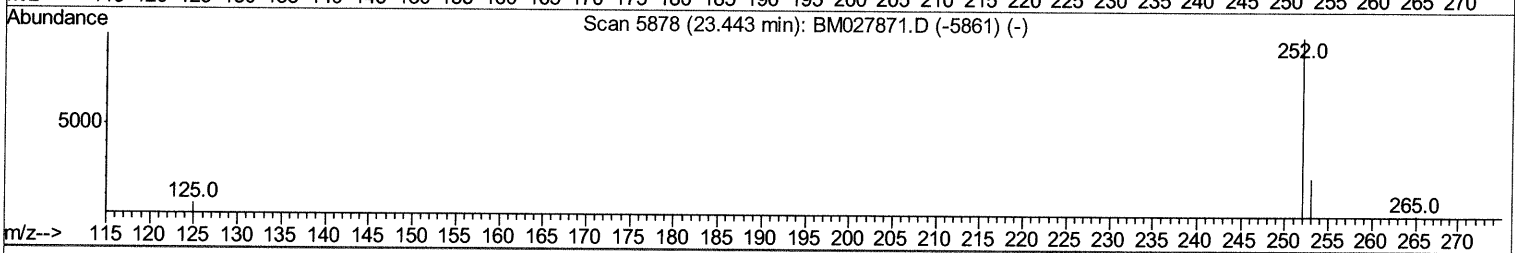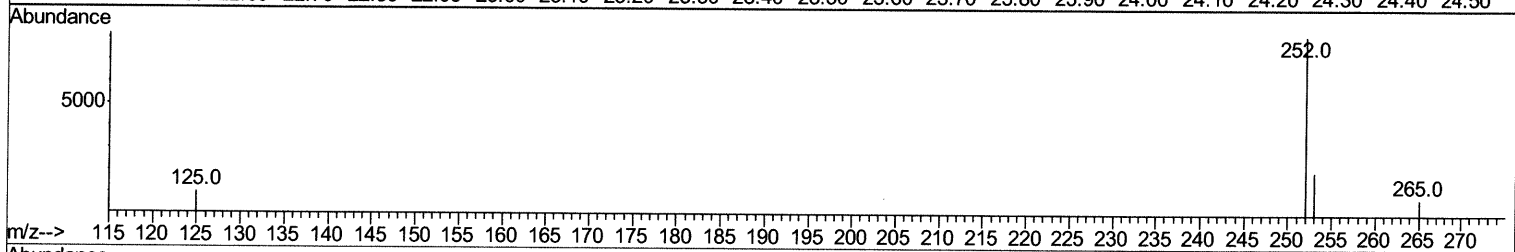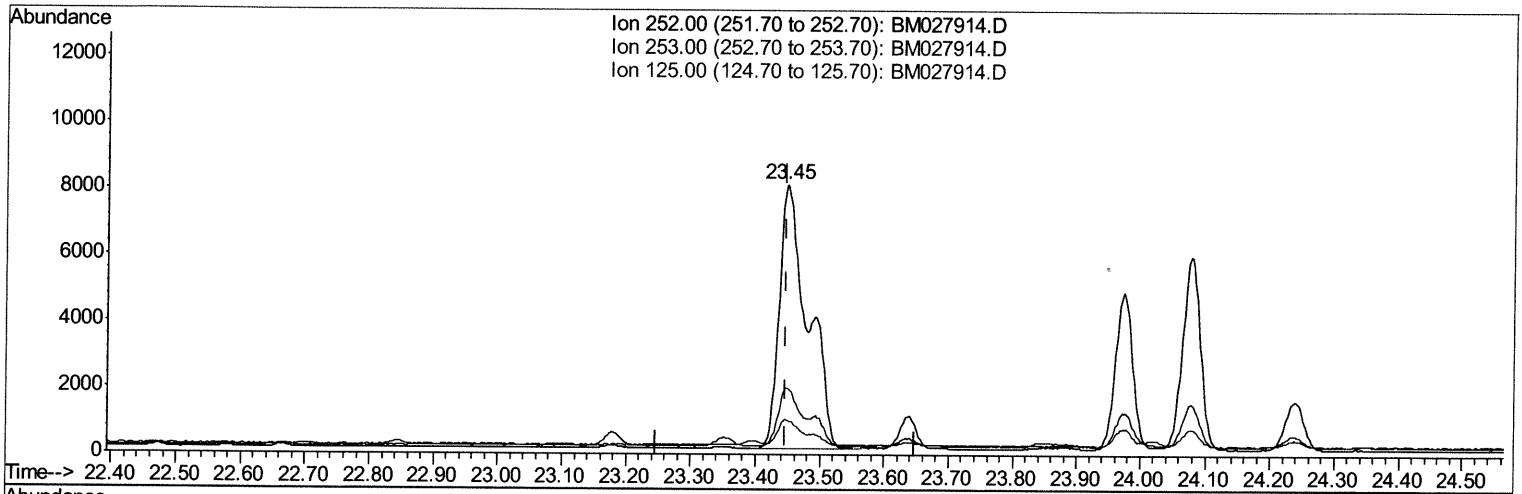

(21) Benzo(b)fluoranthene
 23.447min (0.000) 2.17ng/ul
 response 24428

Ion	Exp%	Act%
252.00	100	100
253.00	29.80	24.66
125.00	14.20	12.79
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM112320\
 Data File : BM027914.D
 Acq On : 23 Nov 2020 15:35
 Operator : JU/CG
 Sample : L4711-11DL 5X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0B55DL

Manual Integrations
 APPROVED

mohammad
 11/25/2020 12:44:33 PM

Quant Time: Nov 23 16:09:26 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM112020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 23 11:35:49 2020
 Response via : Initial Calibration

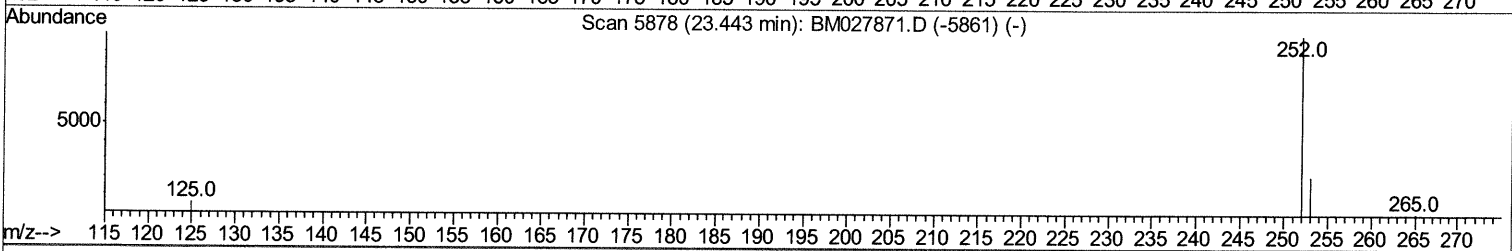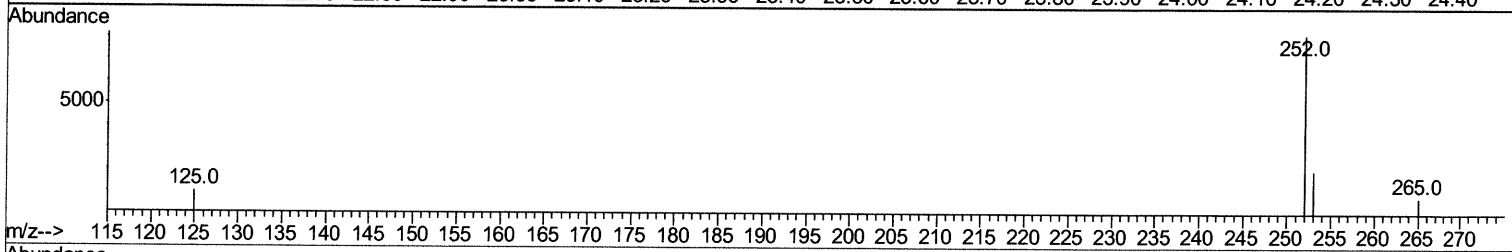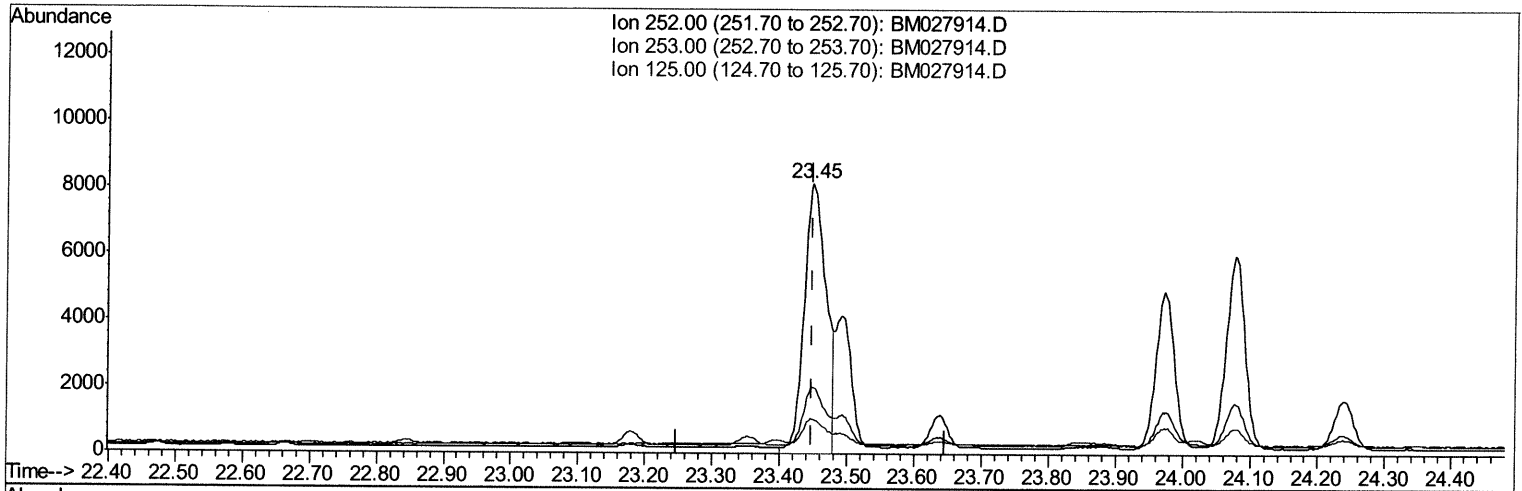

TIC: BM027914.D

(21) Benzo(b)fluoranthene

23.447min (0.000) 1.66ng/ul m 11/25/2020 JU

response 18678

Ion	Exp%	Act%
252.00	100	100
253.00	29.80	24.66
125.00	14.20	12.79
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM112320\
 Data File : BM027914.D
 Acq On : 23 Nov 2020 15:35
 Operator : JU/CG
 Sample : L4711-11DL 5X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0B55DL

Manual Integrations
 APPROVED

mohammad
 11/25/2020 12:44:33 PM

Quant Time: Nov 23 16:09:26 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM112020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 23 11:35:49 2020
 Response via : Initial Calibration

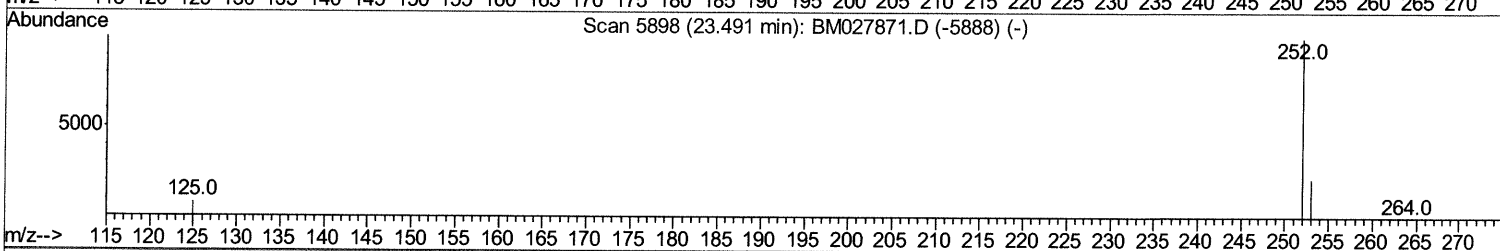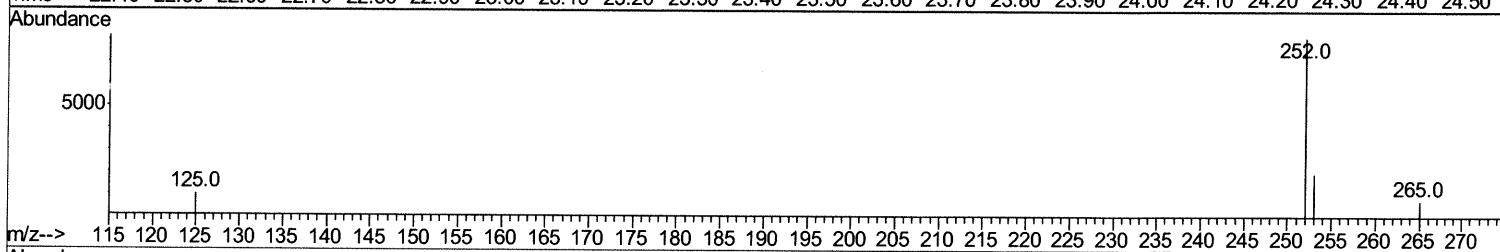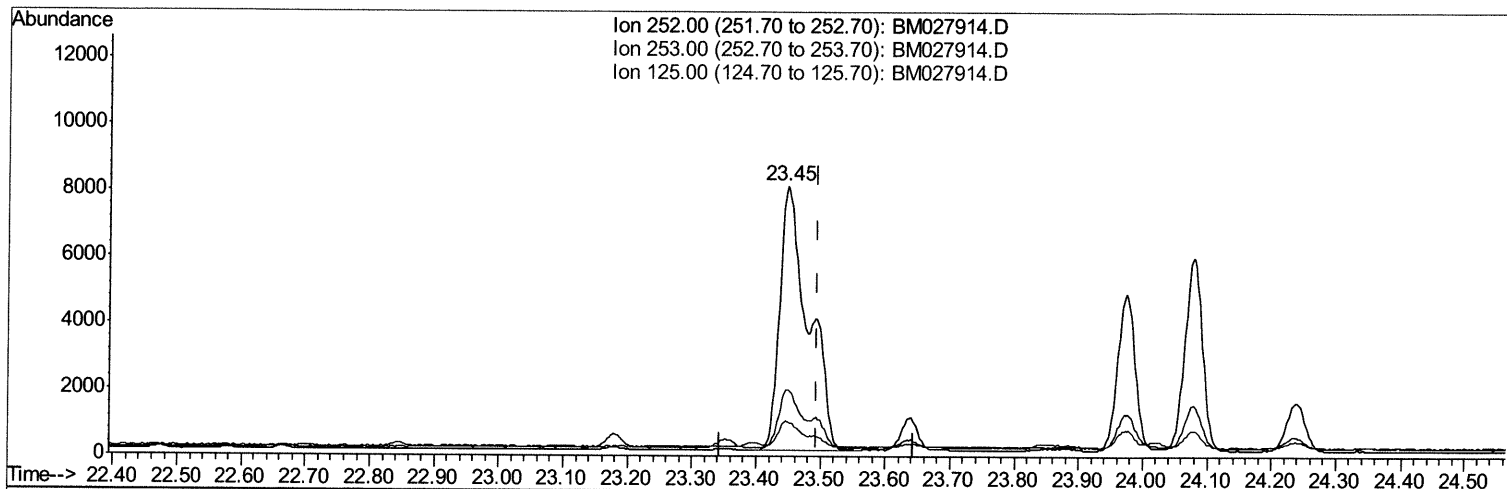

TIC: BM027914.D

(22) Benzo(k)fluoranthene

23.447min (-0.046) 2.22ng/ul

response 24428

Ion	Exp%	Act%
252.00	100	100
253.00	29.00	24.66
125.00	14.70	12.79
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM112320\
 Data File : BM027914.D
 Acq On : 23 Nov 2020 15:35
 Operator : JU/CG
 Sample : L4711-11DL 5X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0B55DL

Manual Integrations
 APPROVED

mohammad
 11/25/2020 12:44:33 PM

Quant Time: Nov 23 16:09:26 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM112020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 23 11:35:49 2020
 Response via : Initial Calibration

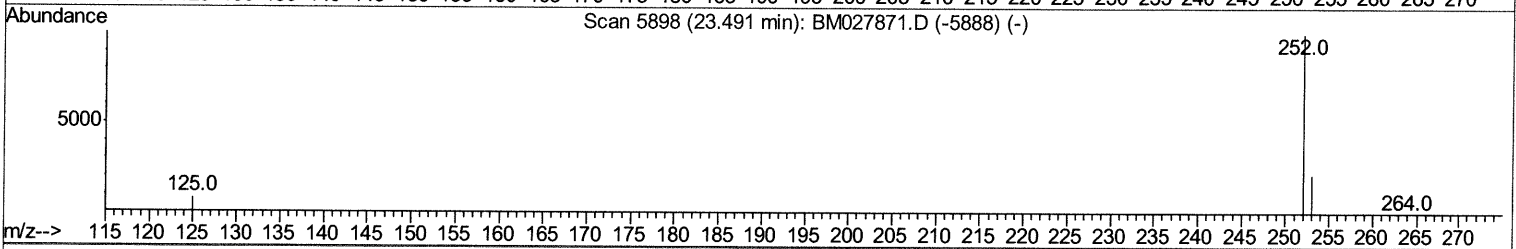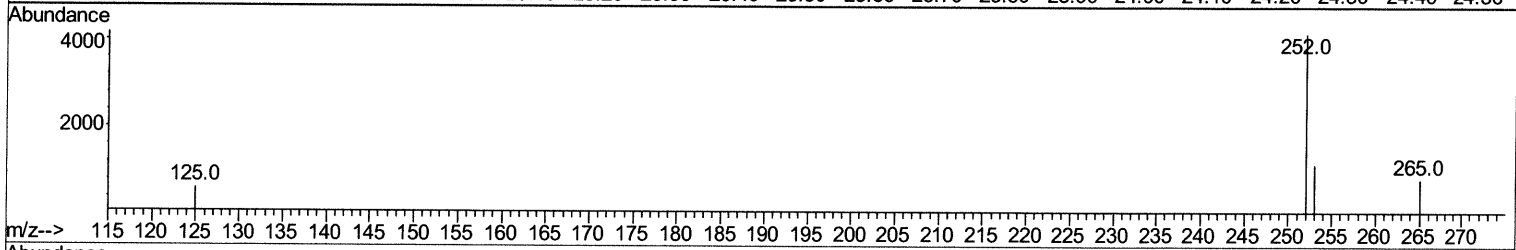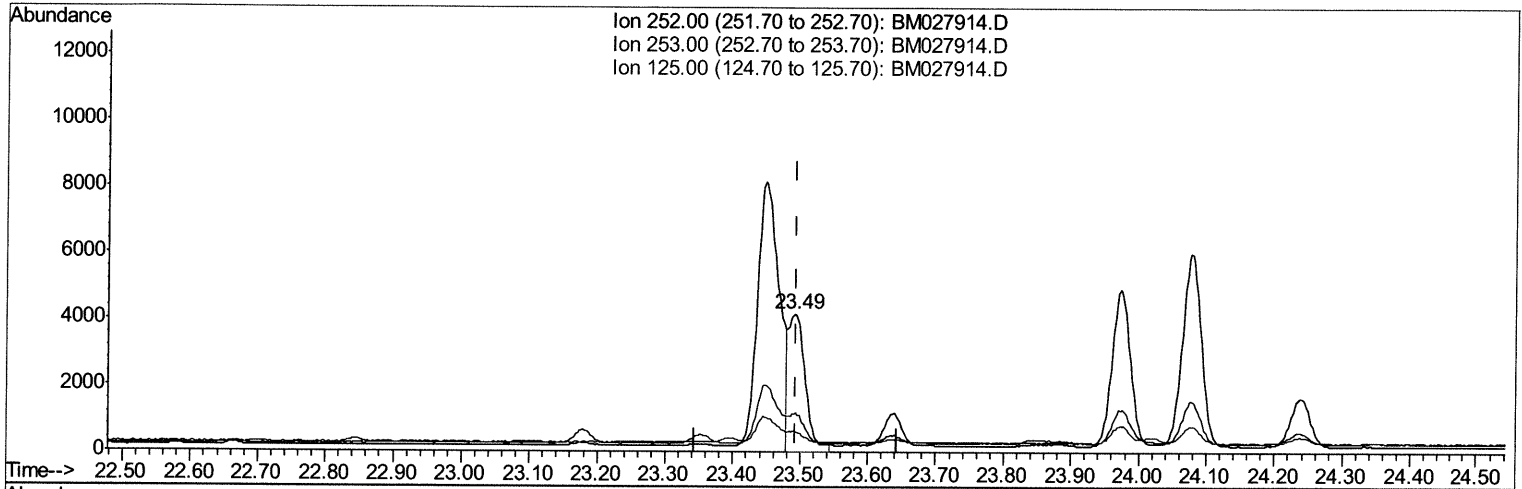

TIC: BM027914.D

(22) Benzo(k)fluoranthene

23.494min (0.000) 0.67ng/ul m 11/25/20 JU

response 7355

Ion	Exp%	Act%
252.00	100	100
253.00	29.00	28.07
125.00	14.70	14.71
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM112320\
 Data File : BM027914.D
 Acq On : 23 Nov 2020 15:35
 Operator : JU/CG
 Sample : L4711-11DL 5X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0B55DL

Manual Integrations
 APPROVED

mohammad
 11/25/2020 12:44:33 PM

Quant Time: Nov 23 16:10:43 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM112020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 23 11:35:49 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.33	152	776	0.40	ng/ul	0.00
2) Naphthalene-d8	11.17	136	3265	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.94	164	2055	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.66	188	4505	0.40	ng/ul	0.00
16) Chrysene-d12	21.76	240	3062	0.40	ng/ul	0.00
20) Perylene-d12	24.18	264	2677	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.73	152	222	0.04	ng/ul	0.00
14) Fluoranthene-d10	19.65	212	470	0.04	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
7) Acenaphthylene	14.67	152	258	0.026	ng/ul#	59
9) Fluorene	15.98	166	228	0.026	ng/ul#	89
12) Phenanthrene	17.70	178	8653	0.608	ng/ul	98
13) Anthracene	17.79	178	1269	0.092	ng/ul#	91
15) Fluoranthene	19.68	202	33645	2.132	ng/ul	100
17) Pyrene	20.04	202	27837	1.790	ng/ul	99
18) Benzo(a)anthracene	21.75	228	11621	0.941	ng/ul	99
19) Chrysene	21.80	228	14388	1.196	ng/ul	99
21) Benzo(b)fluoranthene	23.45	252	18678m	1.660	ng/ul	5
22) Benzo(k)fluoranthene	23.49	252	7355m	0.668	ng/ul	5
23) Benzo(a)pyrene	24.08	252	11146	1.133	ng/ul#	90
24) Indeno(1,2,3-cd)pyrene	26.68	276	8554	0.803	ng/ul#	96
25) Dibenzo(a,h)anthracene	26.68	278	1900	0.214	ng/ul#	78
26) Benzo(g,h,i)perylene	27.46	276	7728	0.865	ng/ul	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed