


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM112320\
Data File : BM027931.D
Acq On : 24 Nov 2020 01:52
Operator : JU/CG
Sample : L4711-20DL 5X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0B05DL

Manual Integrations
APPROVED

mohammad
11/25/2020 12:45:38 PM

Quant Time: Nov 24 03:15:22 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM112020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 24 00:42:23 2020
Response via : Initial Calibration

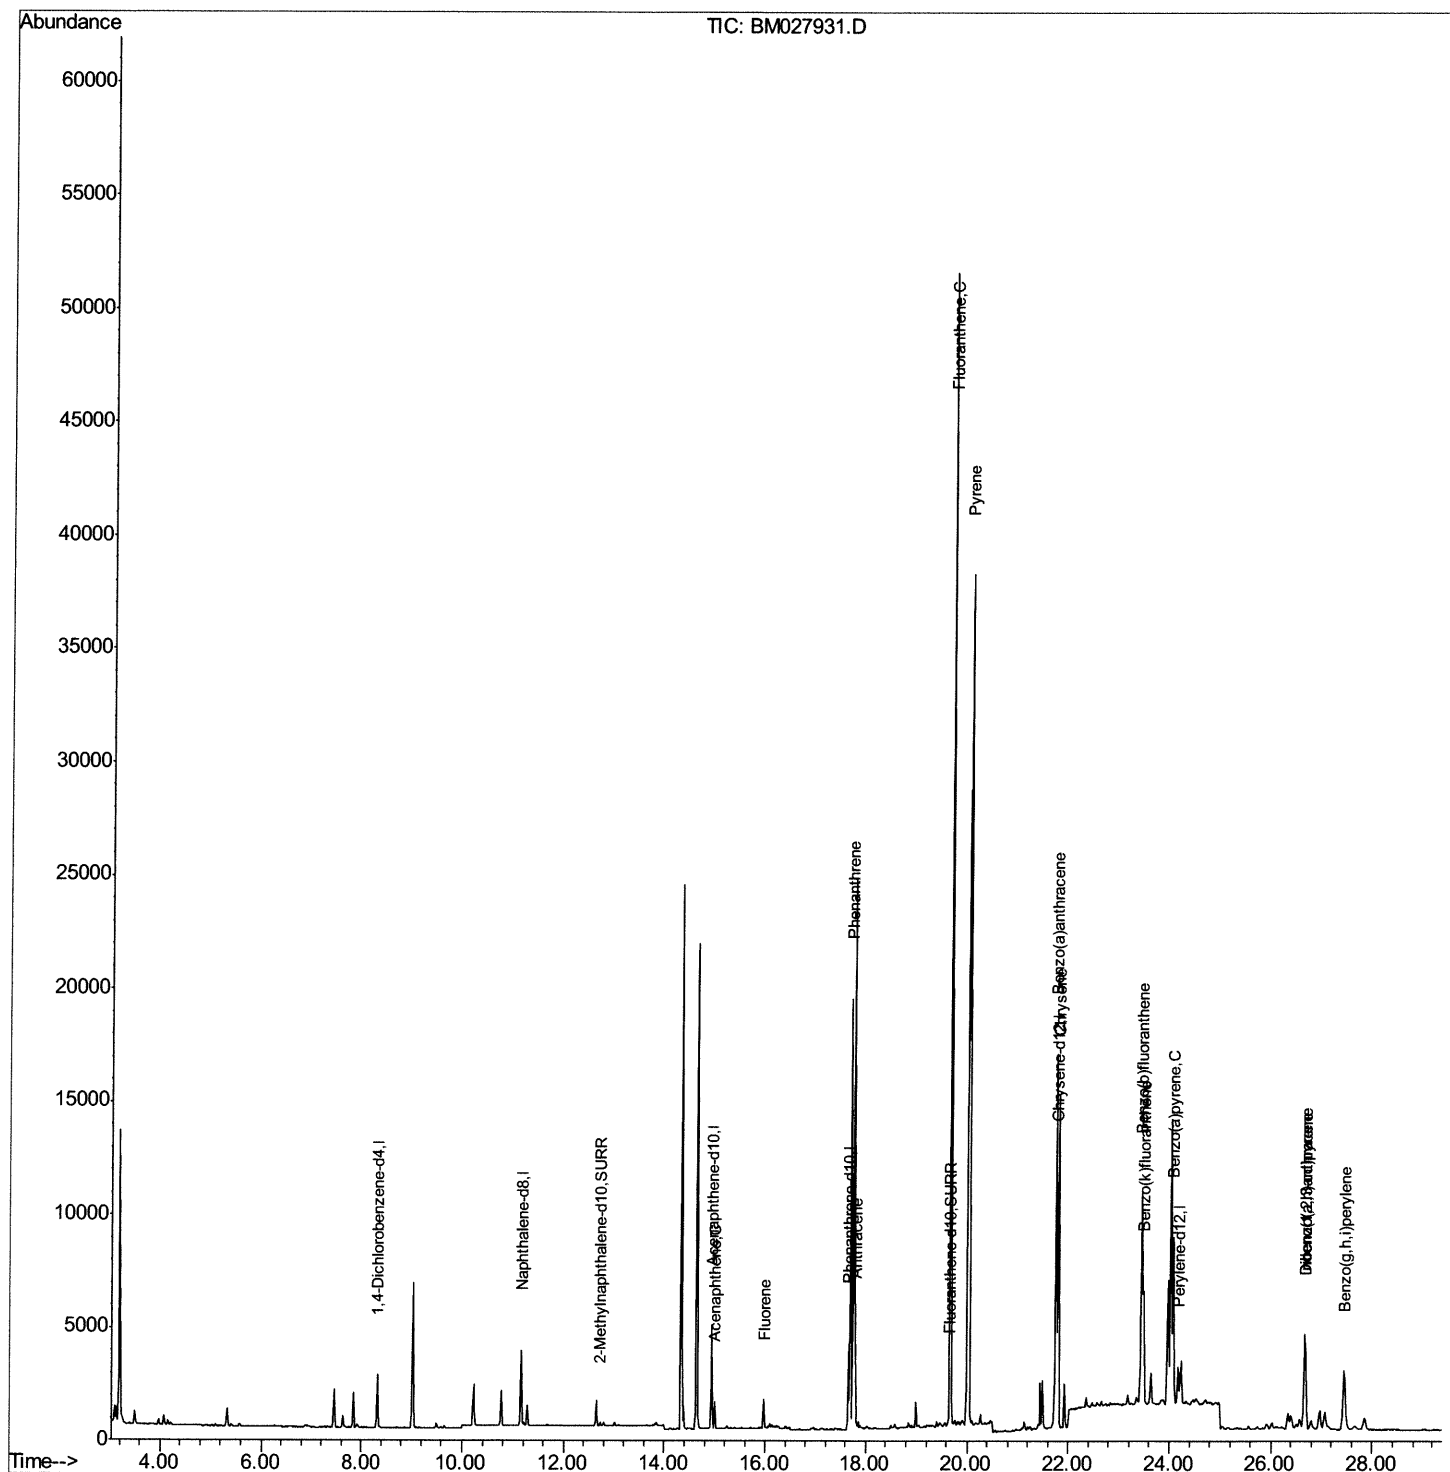

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM112320\
Data File : BM027931.D
Acq On : 24 Nov 2020 01:52
Operator : JU/CG
Sample : L4711-20DL 5X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0B05DL

Manual Integrations
APPROVED

mohammad
11/25/2020 12:45:38 PM

Quant Time: Nov 24 03:03:04 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM112020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 24 00:42:23 2020
Response via : Initial Calibration

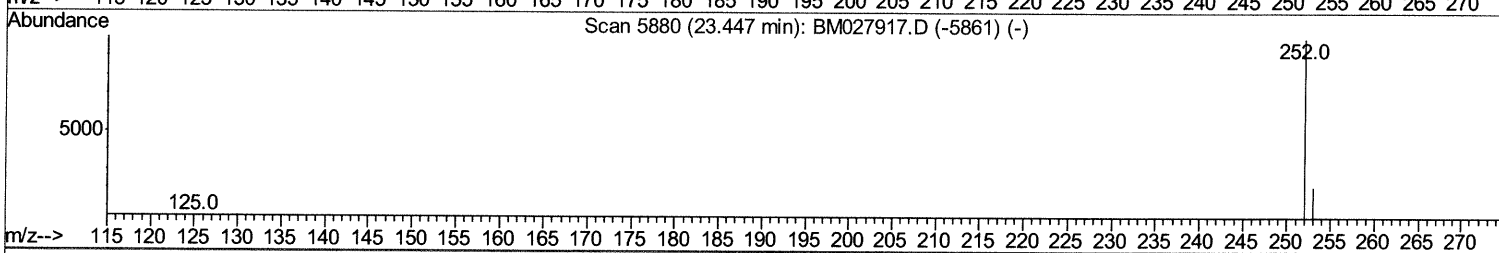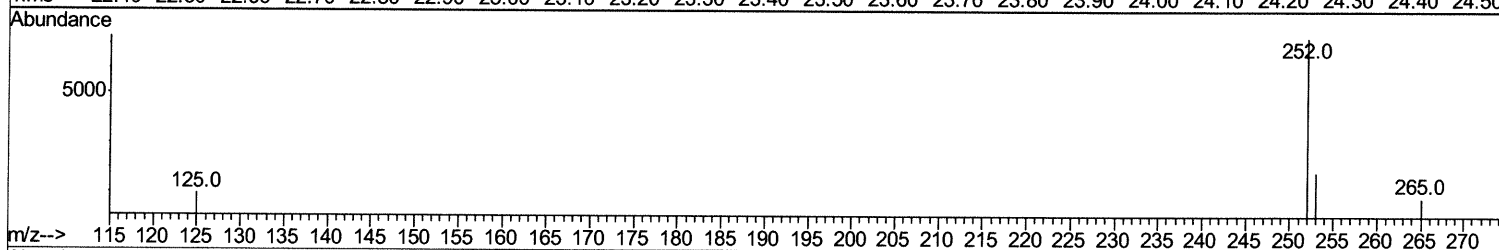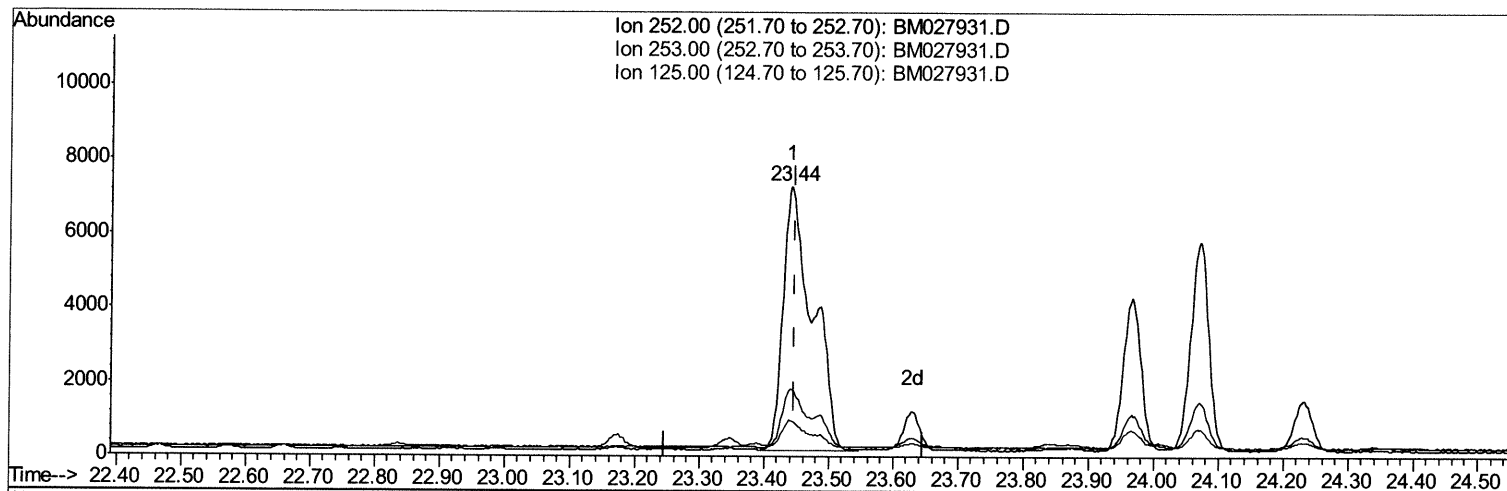

TIC: BM027931.D

(21) Benzo(b)fluoranthene

23.440min (-0.007) 2.33ng/ul

response 22424

Ion	Exp%	Act%
252.00	100	100
253.00	29.80	25.23
125.00	14.20	13.03
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM112320\
 Data File : BM027931.D
 Acq On : 24 Nov 2020 01:52
 Operator : JU/CG
 Sample : L4711-20DL 5X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0B05DL

Manual Integrations
 APPROVED

mohammad
 11/25/2020 12:45:38 PM

Quant Time: Nov 24 03:03:04 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM112020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 24 00:42:23 2020
 Response via : Initial Calibration

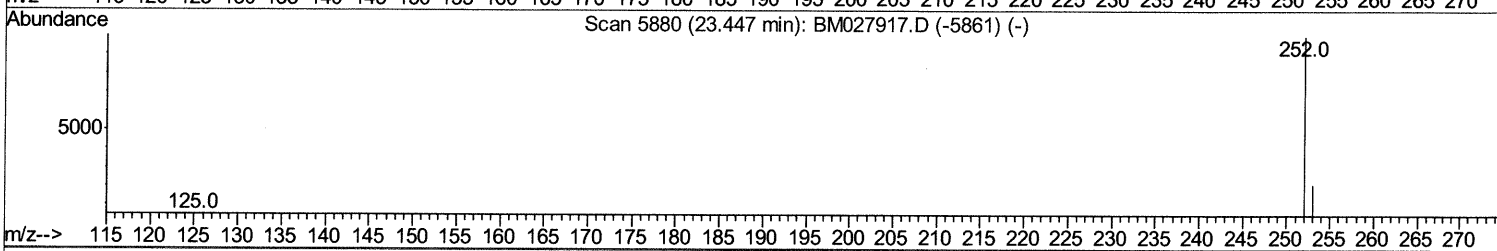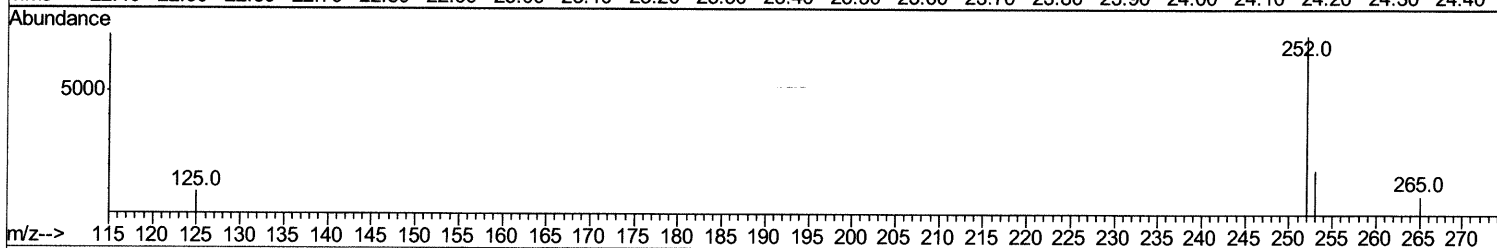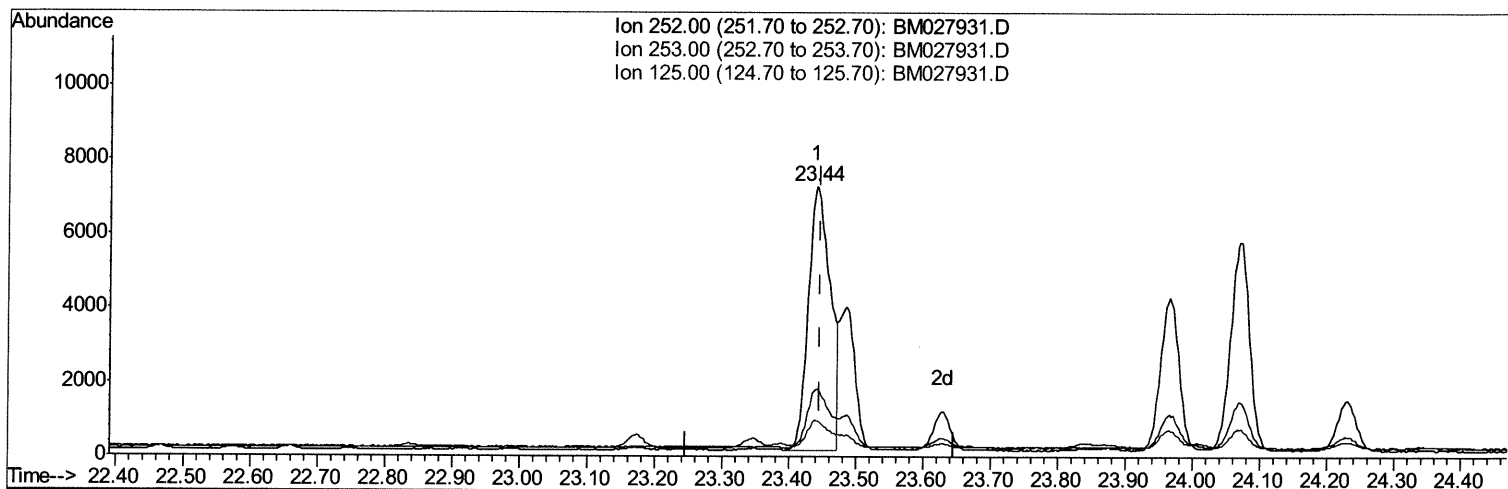

TIC: BM027931.D

(21) Benzo(b)fluoranthene

23.440min (-0.007) 1.68ng/ul m 11/25/20 JU

response 16130

Ion	Exp%	Act%
252.00	100	100
253.00	29.80	25.23
125.00	14.20	13.03
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM112320\
 Data File : BM027931.D
 Acq On : 24 Nov 2020 01:52
 Operator : JU/CG
 Sample : L4711-20DL 5X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0B05DL

Manual Integrations
 APPROVED

mohammad
 11/25/2020 12:45:38 PM

Quant Time: Nov 24 03:03:04 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM112020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 24 00:42:23 2020
 Response via : Initial Calibration

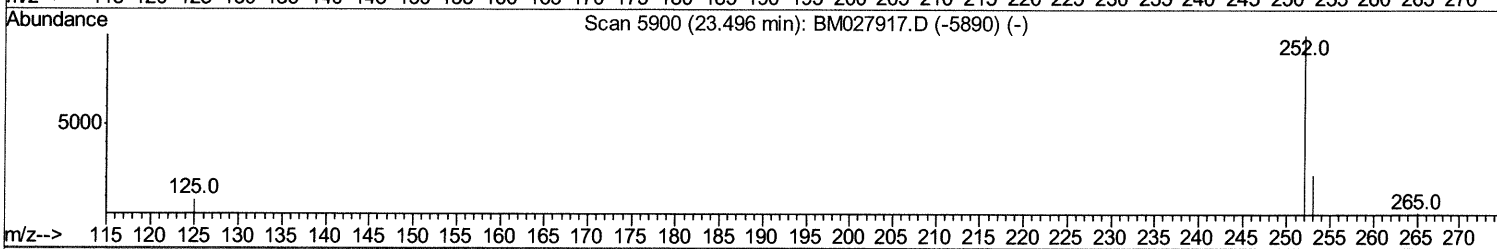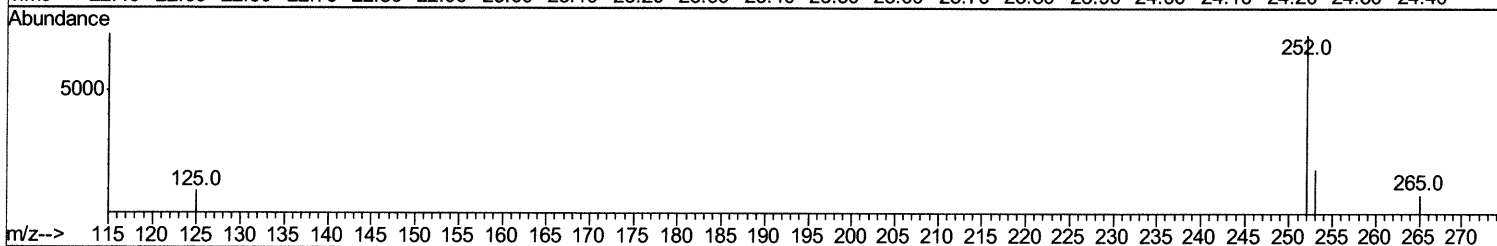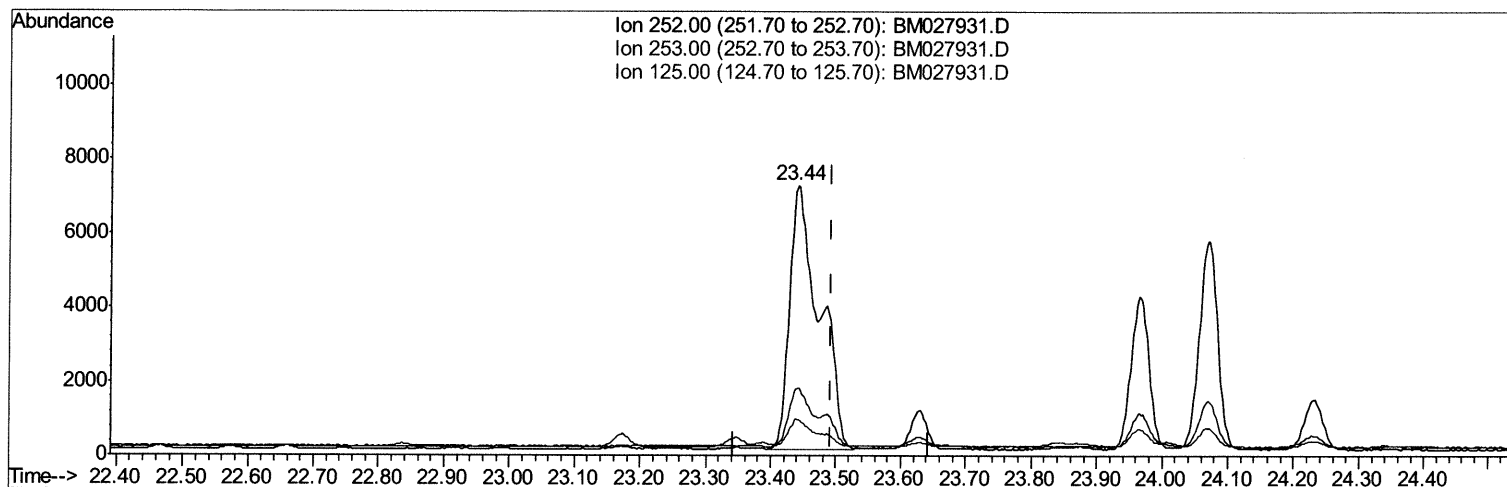

TIC: BM027931.D

(22) Benzo(k)fluoranthene
 23.440min (-0.053) 2.38ng/ul
 response 22404

Ion	Exp%	Act%
252.00	100	100
253.00	29.00	25.23
125.00	14.70	13.03
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM112320\
Data File : BM027931.D
Acq On : 24 Nov 2020 01:52
Operator : JU/CG
Sample : L4711-20DL 5X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0B05DL

Manual Integrations
APPROVED

mohammad
11/25/2020 12:45:38 PM

Quant Time: Nov 24 03:03:04 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM112020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 24 00:42:23 2020
Response via : Initial Calibration

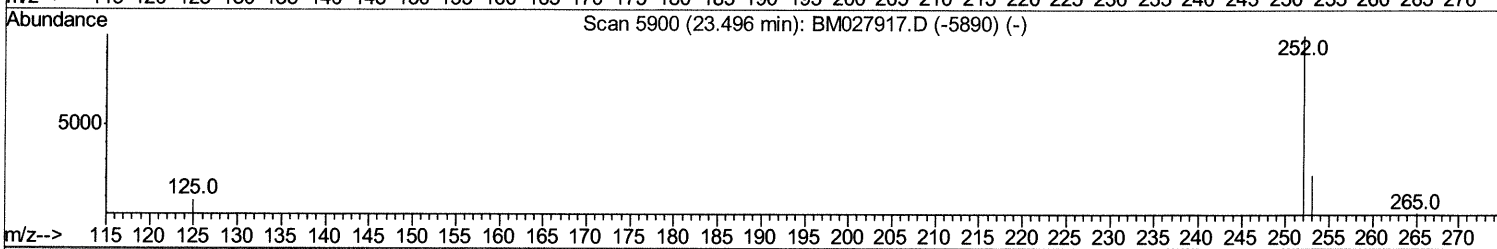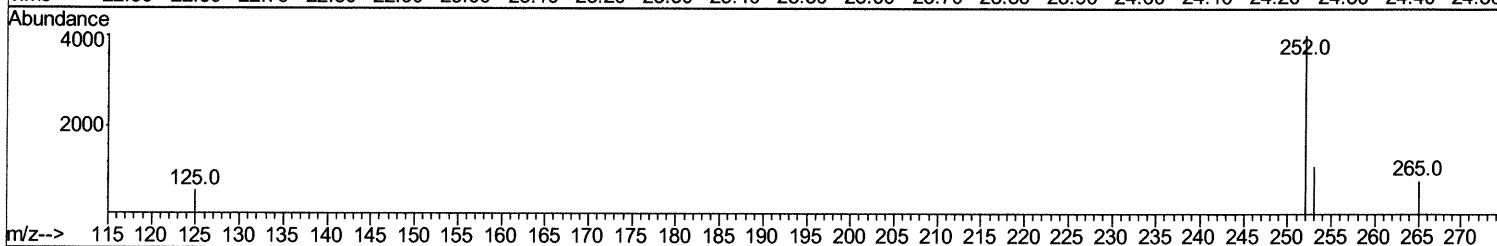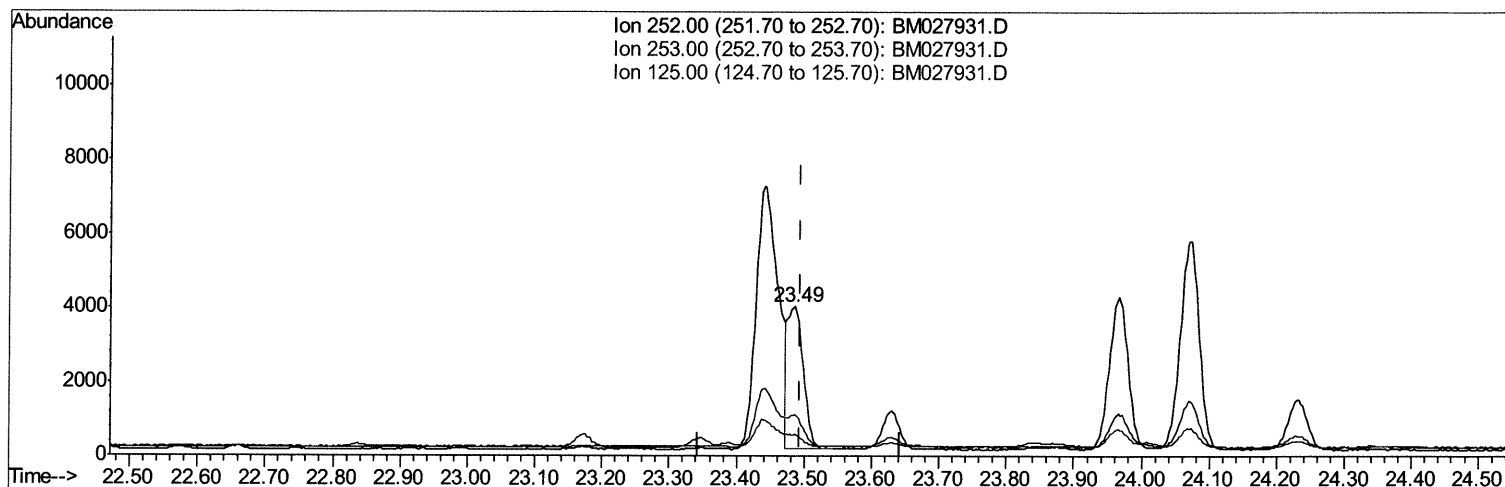

TIC: BM027931.D

(22) Benzo(k)fluoranthene

23.486min (-0.007) 0.66ng/ul m 11/25/20 JU

response 6235

Ion	Exp%	Act%
252.00	100	100
253.00	29.00	27.71
125.00	14.70	14.42
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM112320\
 Data File : BM027931.D
 Acq On : 24 Nov 2020 01:52
 Operator : JU/CG
 Sample : L4711-20DL 5X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0B05DL

Manual Integrations
 APPROVED

mohammad
 11/25/2020 12:45:38 PM

Quant Time: Nov 24 03:15:22 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM112020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 24 00:42:23 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.33	152	1169	0.40	ng/ul	0.00
2) Naphthalene-d8	11.16	136	4538	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.94	164	2493	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.66	188	4448	0.40	ng/ul	0.00
16) Chrysene-d12	21.76	240	2478	0.40	ng/ul	0.00
20) Perylene-d12	24.18	264	2291	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.73	152	186	0.02	ng/ul	0.00
14) Fluoranthene-d10	19.65	212	300	0.03	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
8) Acenaphthene	15.00	153	683	0.075	ng/ul	94
9) Fluorene	15.98	166	828	0.078	ng/ul#	96
12) Phenanthrene	17.70	178	19564	1.392	ng/ul	97
13) Anthracene	17.79	178	4028	0.297	ng/ul	98
15) Fluoranthene	19.68	202	41028	2.633	ng/ul	100
17) Pyrene	20.03	202	32118	2.552	ng/ul	99
18) Benzo(a)anthracene	21.74	228	14148	1.415	ng/ul	100
19) Chrysene	21.80	228	14788	1.519	ng/ul	98
21) Benzo(b)fluoranthene	23.44	252	16130m3	1.675	ng/ul3	11/25/2020
22) Benzo(k)fluoranthene	23.49	252	6235m3	0.661	ng/ul3	
23) Benzo(a)pyrene	24.07	252	10926	1.298	ng/ul#	89
24) Indeno(1,2,3-cd)pyrene	26.67	276	7164	0.786	ng/ul#	96
25) Dibenzo(a,h)anthracene	26.68	278	1871	0.247	ng/ul#	83
26) Benzo(a,h,i)perylene	27.44	276	6018	0.787	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed