




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM112320\
Data File : BM027945.D
Acq On : 24 Nov 2020 16:31
Operator : JU/CG
Sample : L4749-14
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0B13

Manual Integrations
APPROVED

mohammad
11/25/2020 12:46:12 PM

Quant Time: Nov 24 17:25:41 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM112020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 24 15:00:24 2020
Response via : Initial Calibration

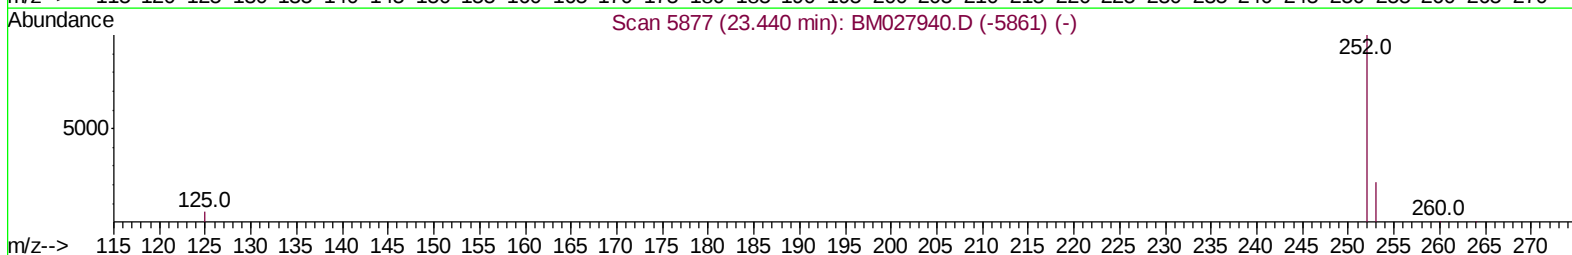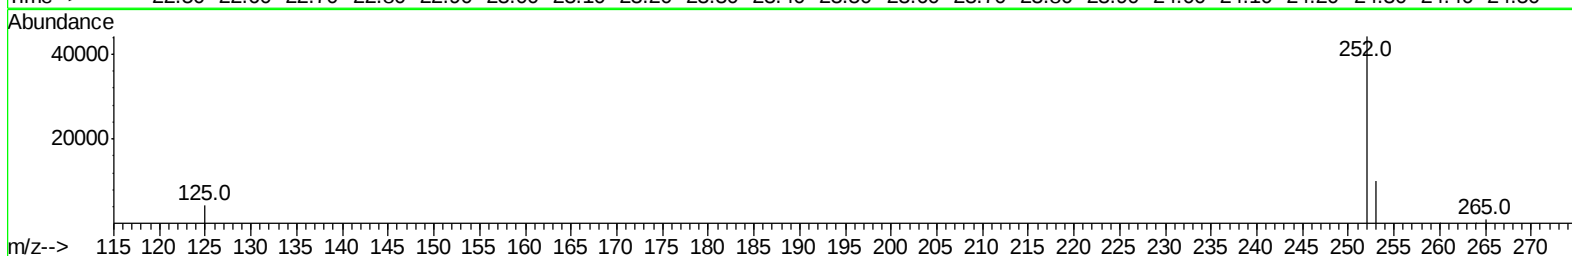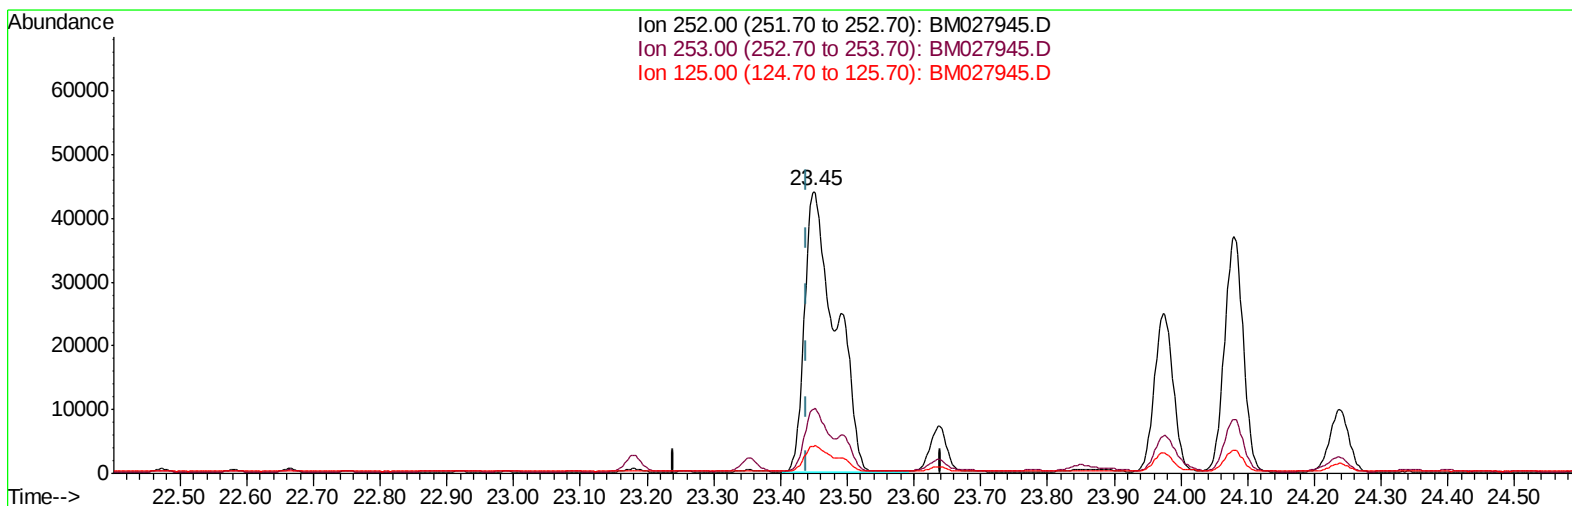

TIC: BM027945.D

(21) Benzo(b)fluoranthene

23.450min (+0.010) 16.89ng/ul

response 142239

Ion	Exp%	Act%
252.00	100	100
253.00	29.80	22.83
125.00	14.20	9.71
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM112320\
Data File : BM027945.D
Acq On : 24 Nov 2020 16:31
Operator : JU/CG
Sample : L4749-14
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0B13

Manual Integrations
APPROVED

mohammad
11/25/2020 12:46:12 PM

Quant Time: Nov 24 17:25:41 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM112020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 24 15:00:24 2020
Response via : Initial Calibration

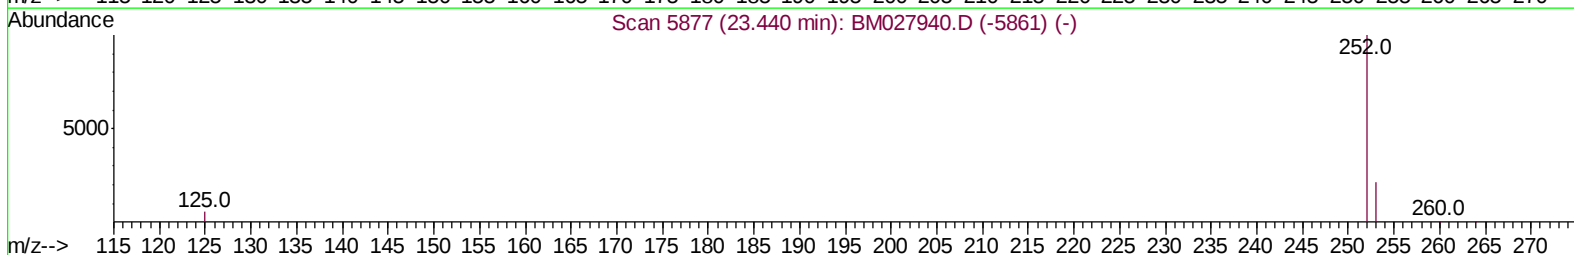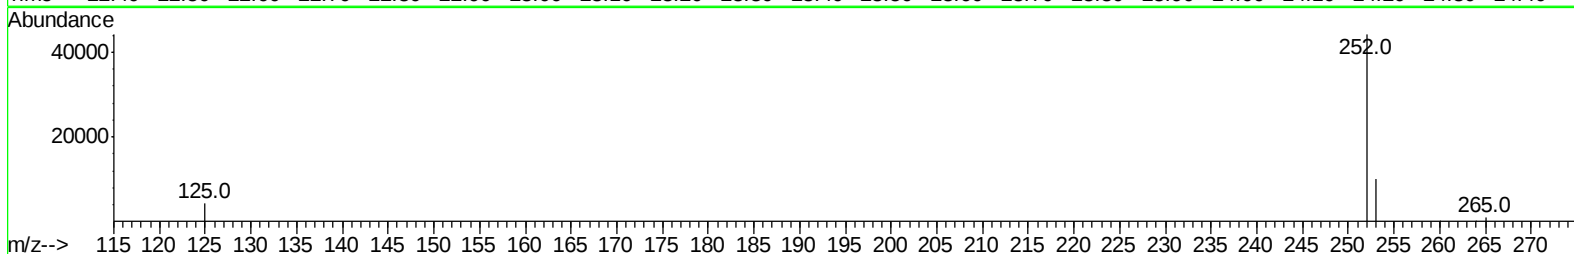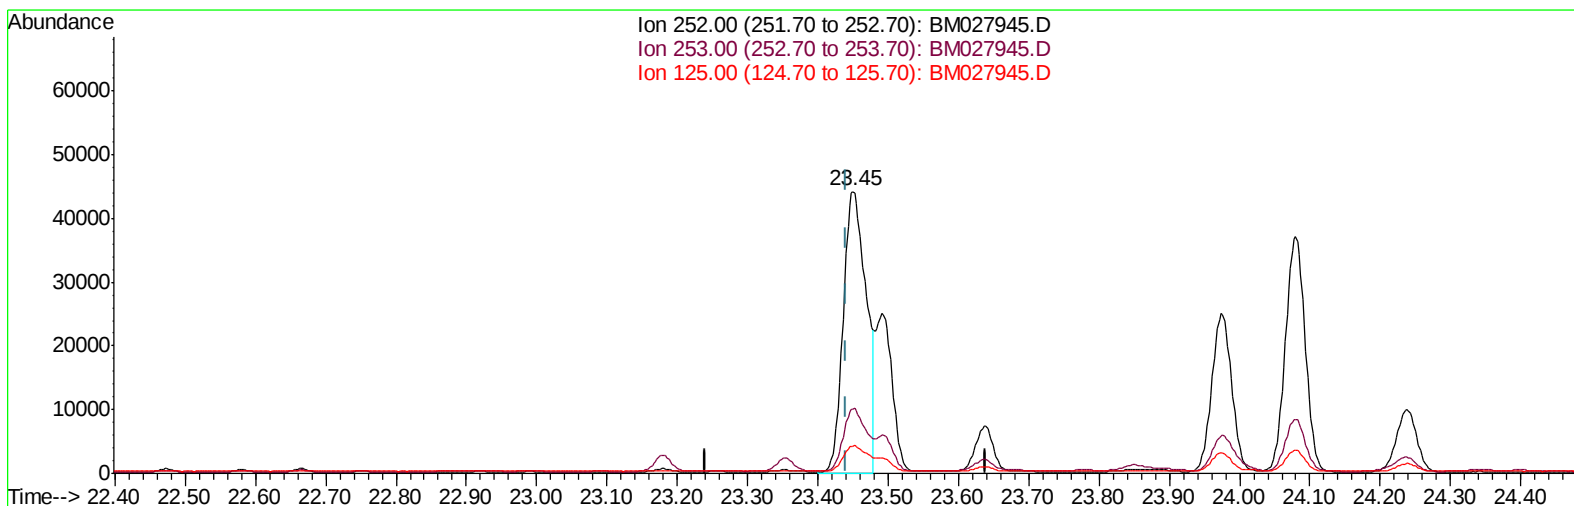

TIC: BM027945.D

(21) Benzo(b)fluoranthene

23.450min (+0.010) 12.17ng/ul m

response 102533

Ion	Exp%	Act%
252.00	100	100
253.00	29.80	22.83
125.00	14.20	9.71
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM112320\
 Data File : BM027945.D
 Acq On : 24 Nov 2020 16:31
 Operator : JU/CG
 Sample : L4749-14
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0B13

Manual Integrations
 APPROVED

mohammad
 11/25/2020 12:46:12 PM

Quant Time: Nov 24 17:25:41 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM112020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 24 15:00:24 2020
 Response via : Initial Calibration

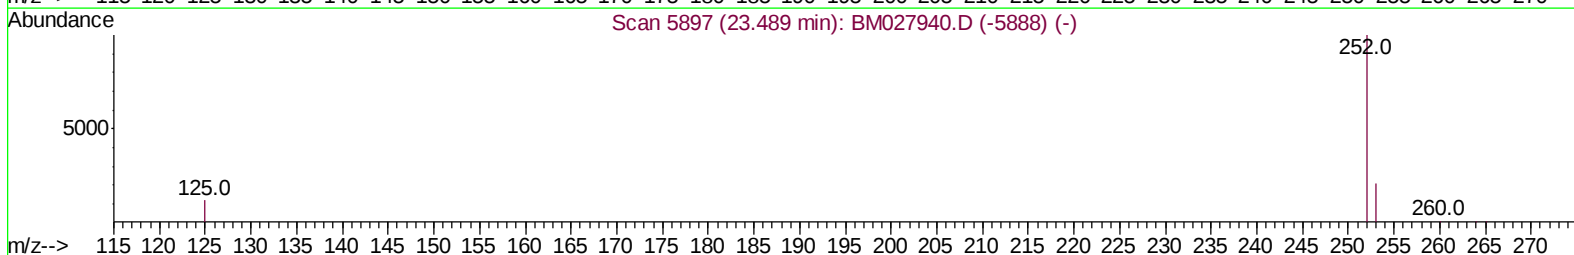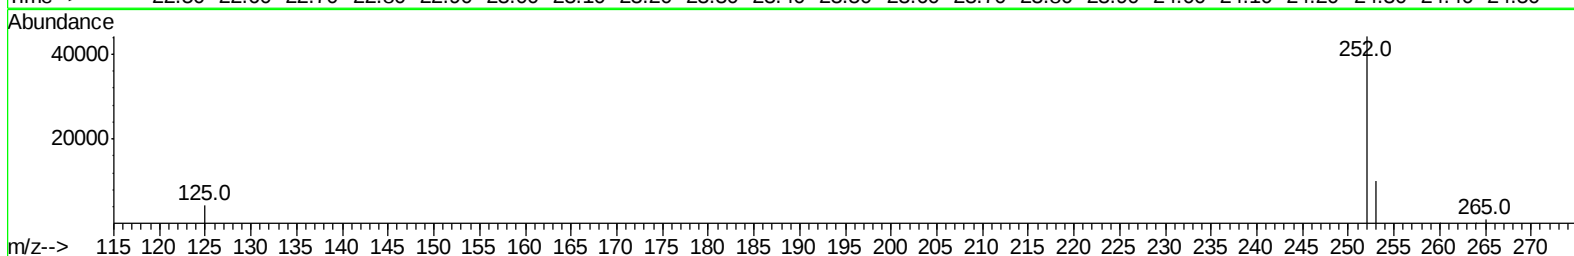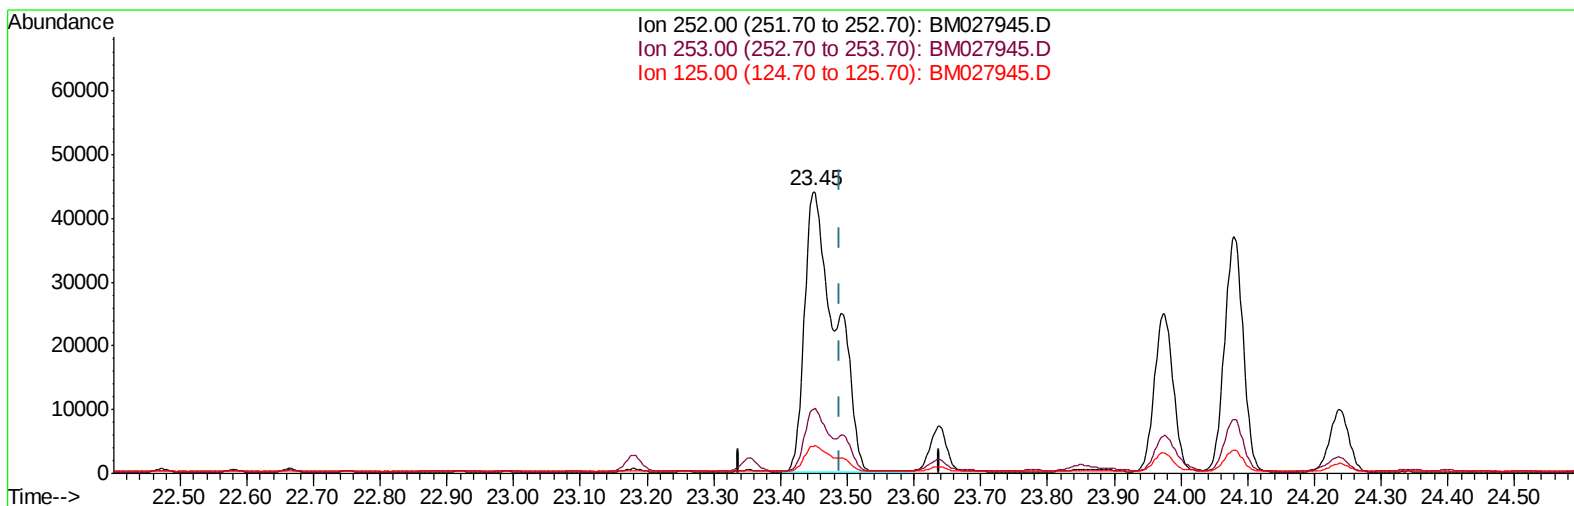

TIC: BM027945.D

(22) Benzo(k)fluoranthene

23.450min (-0.039) 17.25ng/ul

response 142239

Ion	Exp%	Act%
252.00	100	100
253.00	29.00	22.83#
125.00	14.70	9.71#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM112320\
 Data File : BM027945.D
 Acq On : 24 Nov 2020 16:31
 Operator : JU/CG
 Sample : L4749-14
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0B13

Manual Integrations
 APPROVED

mohammad
 11/25/2020 12:46:12 PM

Quant Time: Nov 24 17:25:41 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM112020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 24 15:00:24 2020
 Response via : Initial Calibration

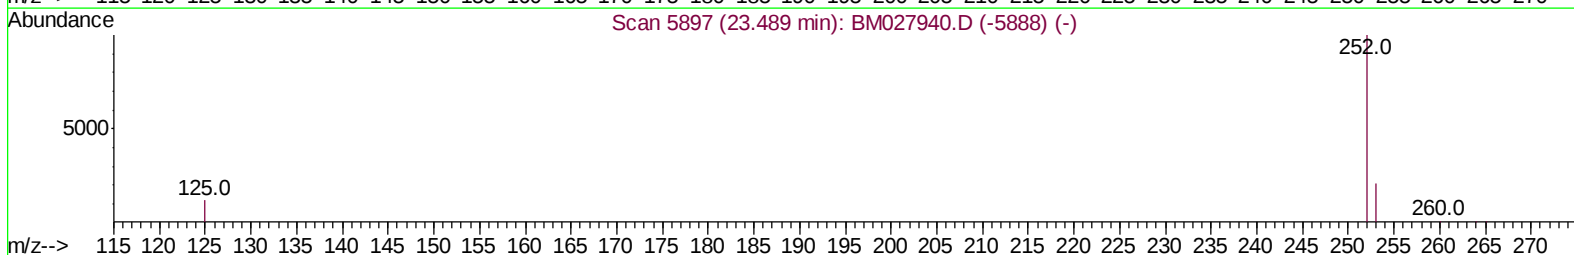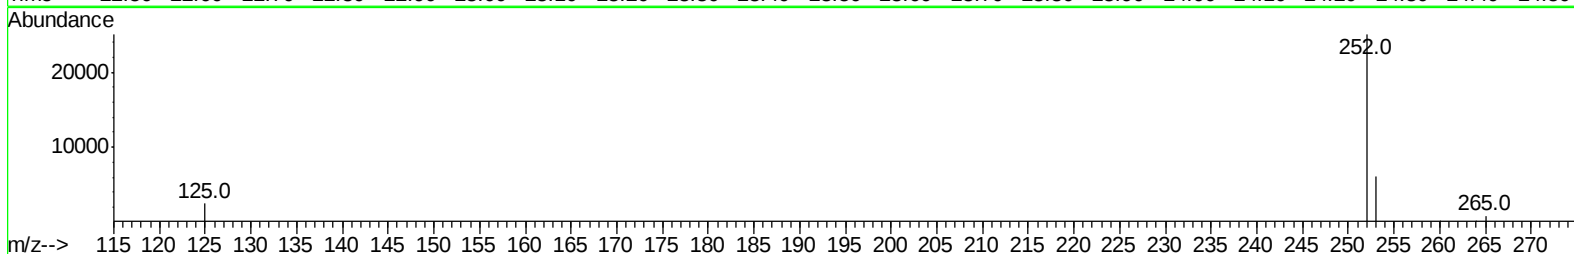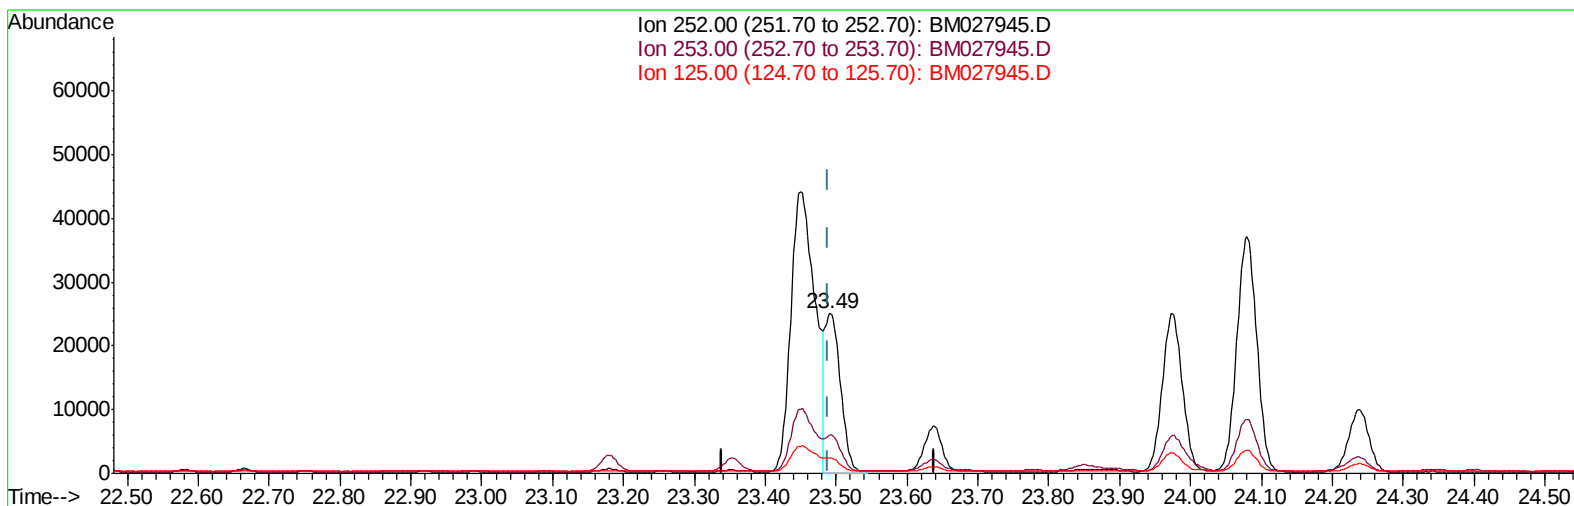

TIC: BM027945.D

(22) Benzo(k)fluoranthene

23.491min (+0.002) 4.68ng/ul m

response 38575

Ion	Exp%	Act%
252.00	100	100
253.00	29.00	23.94
125.00	14.70	9.72#
0.00	0.00	0.00