

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112423\
 Data File : BM042986.D
 Acq On : 24 Nov 2023 19:43
 Operator : MA/JU
 Sample : PB157096BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK096

Quant Time: Nov 24 23:23:49 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 24 15:22:31 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.817	152	791	0.400	ng/ul	#-0.06
4) Naphthalene-d8	10.616	136	2653	0.400	ng/ul	#-0.03
9) Acenaphthene-d10	14.459	164	1543	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.309	188	270660	0.400	ng/ul	# 0.07
17) Chrysene-d12	21.441	240	1630	0.400	ng/ul	0.02
23) Perylene-d12	0.000	264	0	0.000	ng/ul	-23.78
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.164	96	6083	5.012	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.261	152	937	0.264	ng/ul	0.01
18) Fluoranthene-d10	19.252	212	2231	0.376	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.454	166	563	0.092	ng/ul#	22
20) Pyrene	19.610	202	577	0.059	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112423\
Data File : BM042986.D
Acq On : 24 Nov 2023 19:43
Operator : MA/JU
Sample : PB157096BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK096

Quant Time: Nov 24 23:23:49 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 24 15:22:31 2023
Response via : Initial Calibration




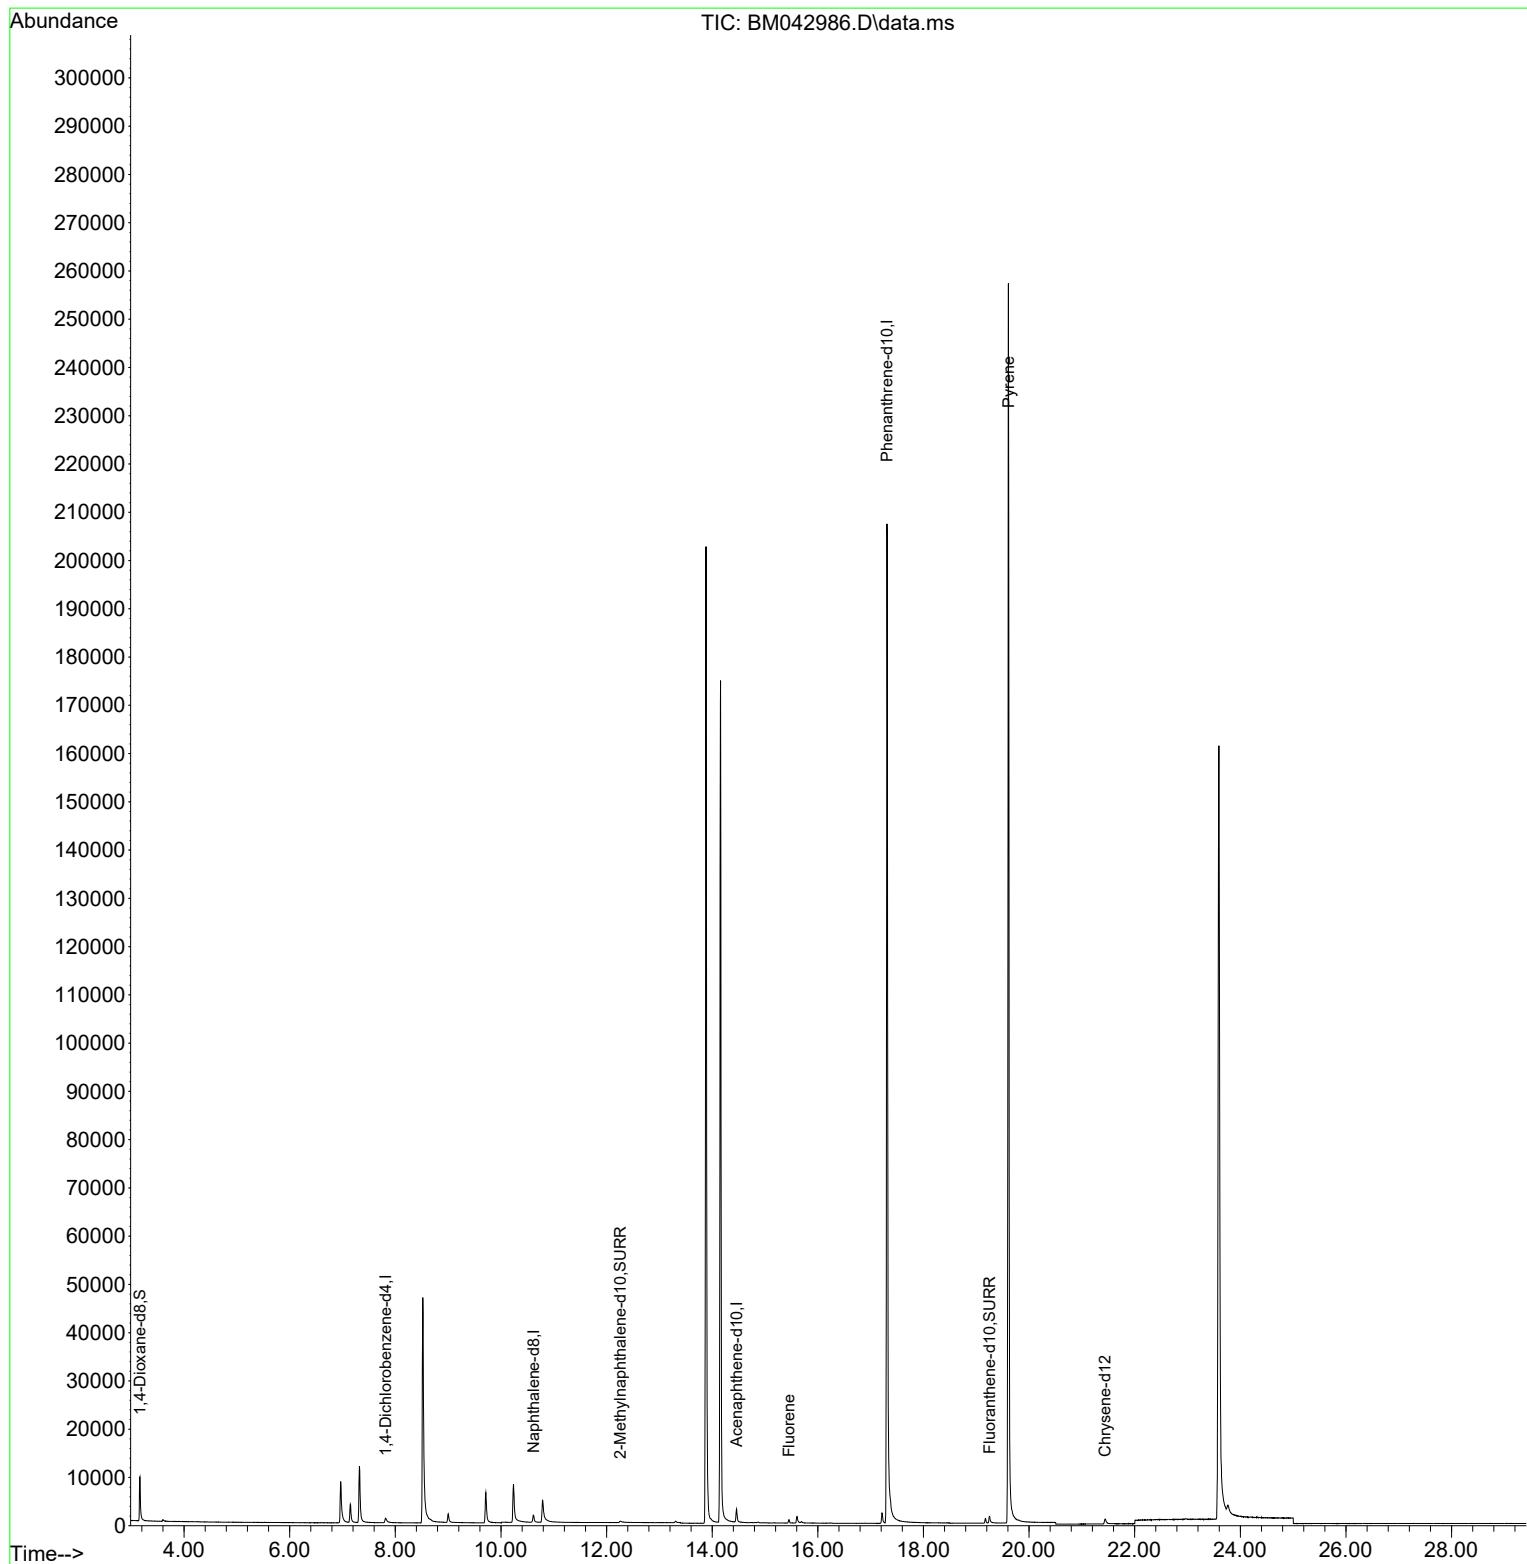


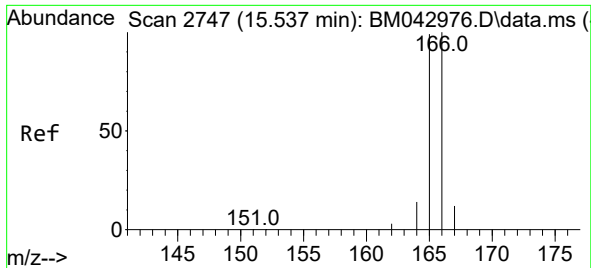

#12
Fluorene
Concen: 0.092 ng/ul
RT: 15.454 min Scan# 21
Delta R.T. -0.083 min
Lab File: BM042986.D
Acq: 24 Nov 2023 19:43

Instrument :
BNA_M
ClientSampleId :
SBLK096

Tgt Ion:166 Resp: 563
Ion Ratio Lower Upper
166 100
165 16.9 79.9 119.9#
167 39.1 14.2 21.4#

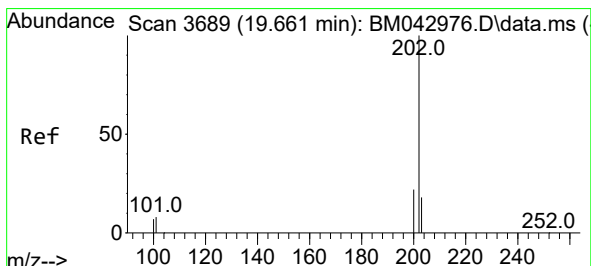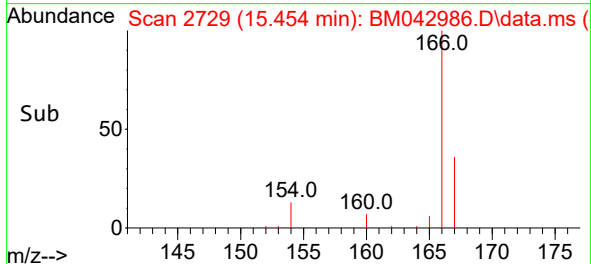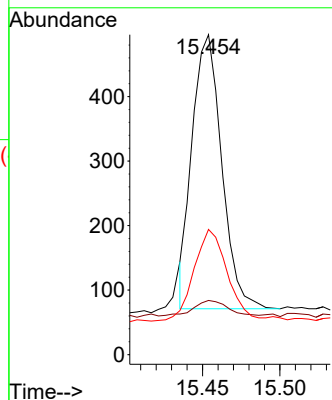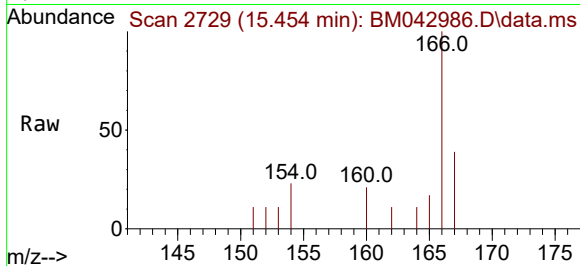

#20
Pyrene
Concen: 0.059 ng/ul
RT: 19.610 min Scan# 3678
Delta R.T. -0.051 min
Lab File: BM042986.D
Acq: 24 Nov 2023 19:43

Tgt Ion:202 Resp: 577
Ion Ratio Lower Upper
202 100
101 170.7 8.7 13.1#
100 1295.0 7.8 11.8#

