

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112423\
 Data File : BM042988.D
 Acq On : 24 Nov 2023 20:56
 Operator : MA/JU
 Sample : 05268-11
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCKD3RE

Quant Time: Nov 24 23:24:01 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 24 15:22:31 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.817	152	820	0.400	ng/ul	#-0.06
4) Naphthalene-d8	10.612	136	2575	0.400	ng/ul	#-0.04
9) Acenaphthene-d10	14.460	164	1425	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.310	188	333857	0.400	ng/ul	# 0.07
17) Chrysene-d12	21.426	240	1664	0.400	ng/ul	0.00
23) Perylene-d12	0.000	264	0	0.000	ng/ul	-23.78
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.164	96	4681	3.720	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.256	152	1036	0.301	ng/ul	0.00
18) Fluoranthene-d10	19.248	212	2941	0.485	ng/ul	-0.01
Target Compounds						
20) Pyrene	19.606	202	781	0.078	ng/ul#	Qvalue 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112423\
Data File : BM042988.D
Acq On : 24 Nov 2023 20:56
Operator : MA/JU
Sample : 05268-11
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKD3RE

Quant Time: Nov 24 23:24:01 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 24 15:22:31 2023
Response via : Initial Calibration

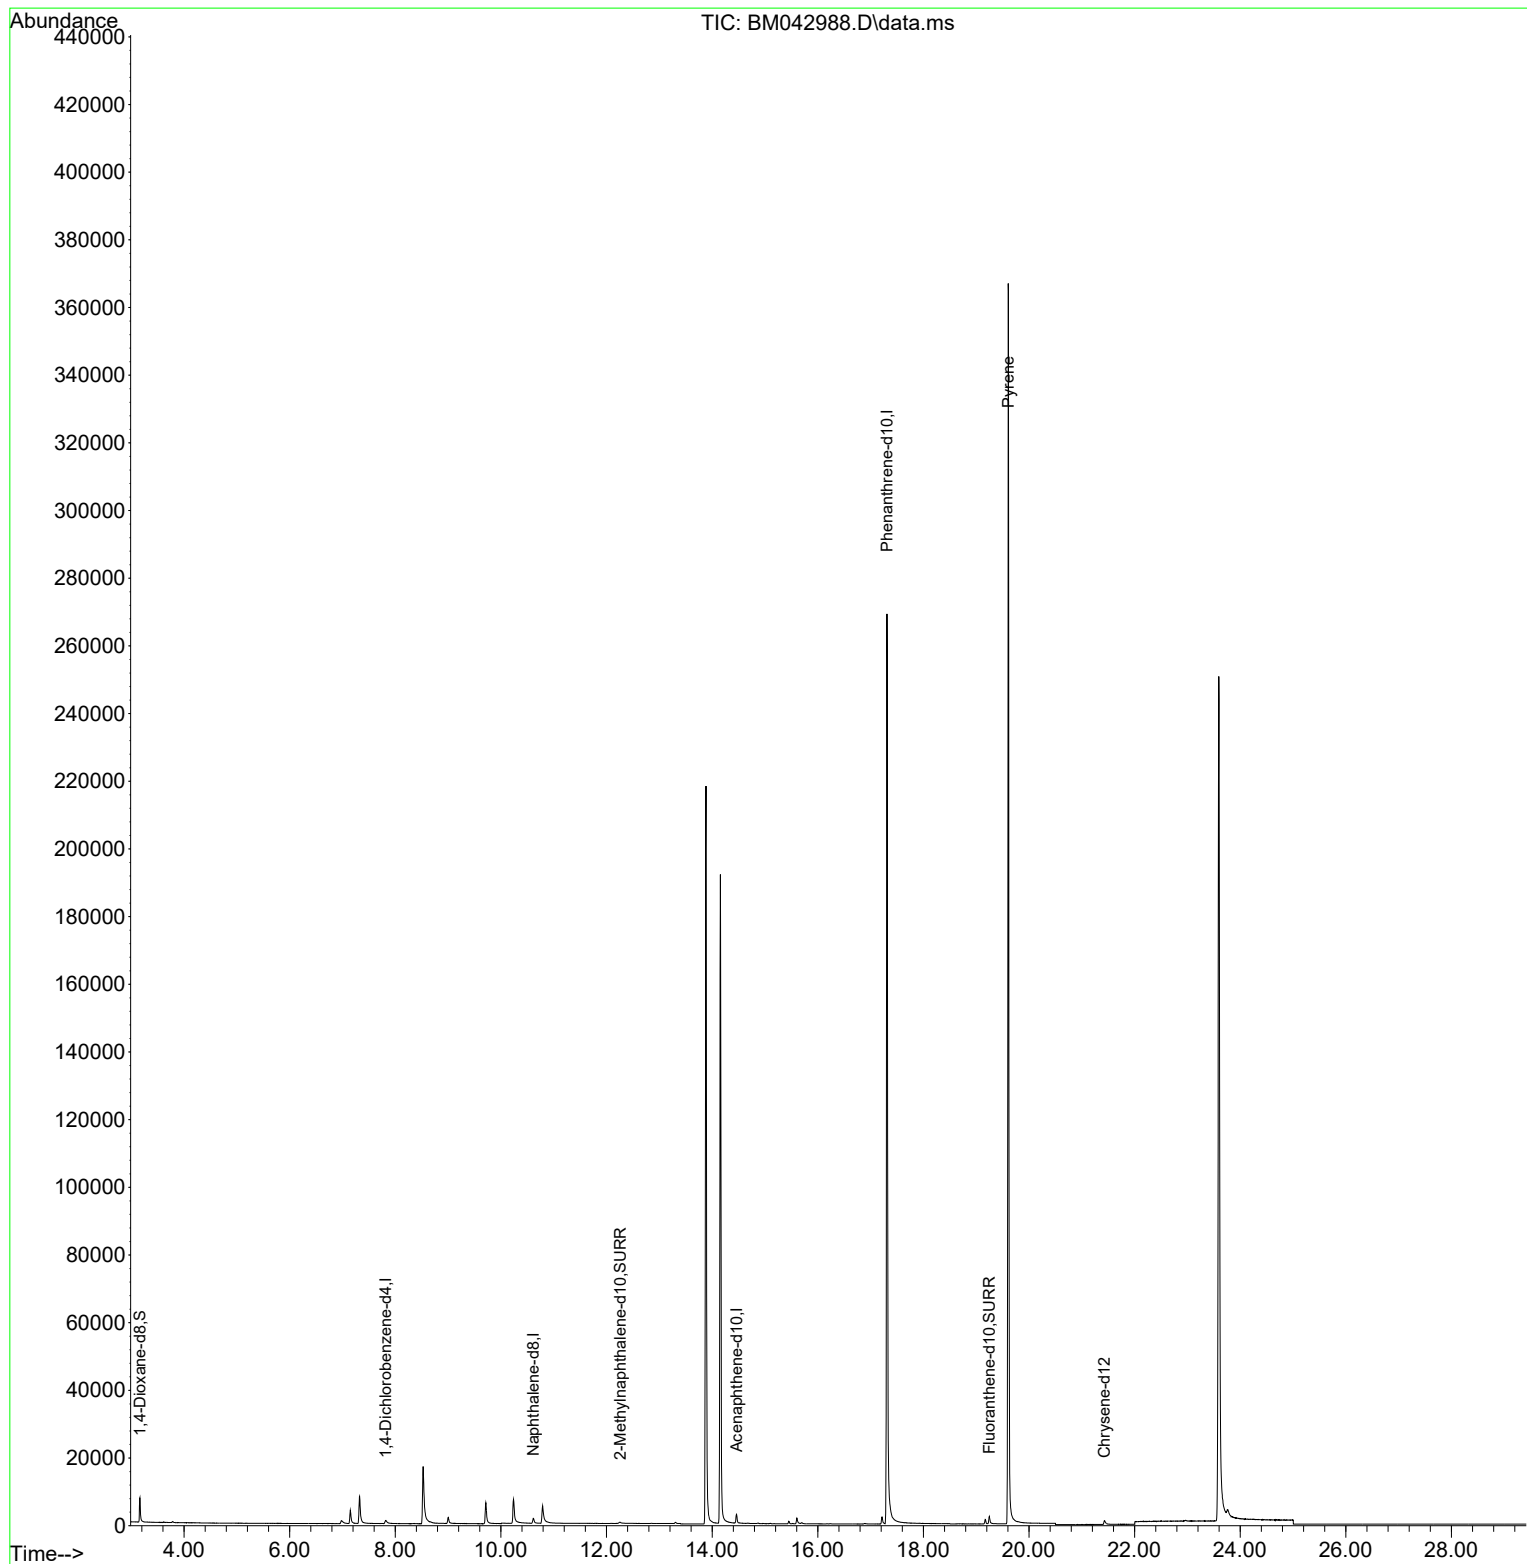

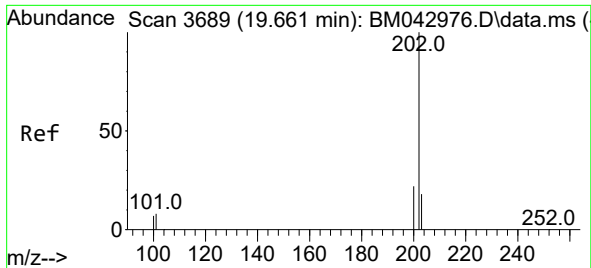

#20

Pyrene

Concen: 0.078 ng/ul

RT: 19.606 min Scan# 30

Delta R.T. -0.054 min

Lab File: BM042988.D


Acq: 24 Nov 2023 20:56

Instrument :

BNA_M

ClientSampleId :

DCKD3RE

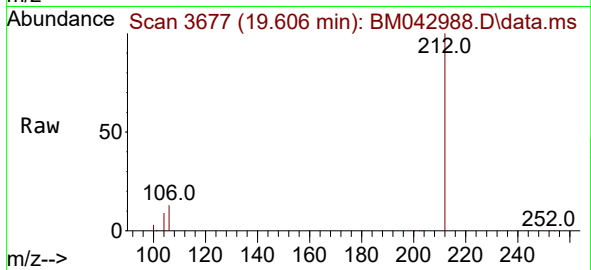

Tgt Ion:202 Resp: 781

Ion Ratio Lower Upper

202 100

101 187.5 8.7 13.1#

100 1527.7 7.8 11.8#

