

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112423\
 Data File : BM043008.D
 Acq On : 25 Nov 2023 09:38
 Operator : MA/JU
 Sample : 05261-12
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCKR1

Quant Time: Nov 27 02:42:42 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 27 02:36:19 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.809	152	1120	0.400	ng/ul	#-0.07
4) Naphthalene-d8	10.612	136	3626	0.400	ng/ul	#-0.04
9) Acenaphthene-d10	14.456	164	2126	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.306	188	285196	0.400	ng/ul	# 0.07
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.42
23) Perylene-d12	23.753	264	7086	0.400	ng/ul	#-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.160	96	5539	3.223	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.229	152	1252	0.258	ng/ul	-0.02
18) Fluoranthene-d10	19.244	212	2958	0.000	ng/ul	-0.02
Target Compounds						Qvalue
10) Acenaphthylene	14.183	152	275	0.025	ng/ul#	56


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112423\
Data File : BM043008.D
Acq On : 25 Nov 2023 09:38
Operator : MA/JU
Sample : 05261-12
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKR1


Quant Time: Nov 27 02:42:42 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 27 02:36:19 2023
Response via : Initial Calibration

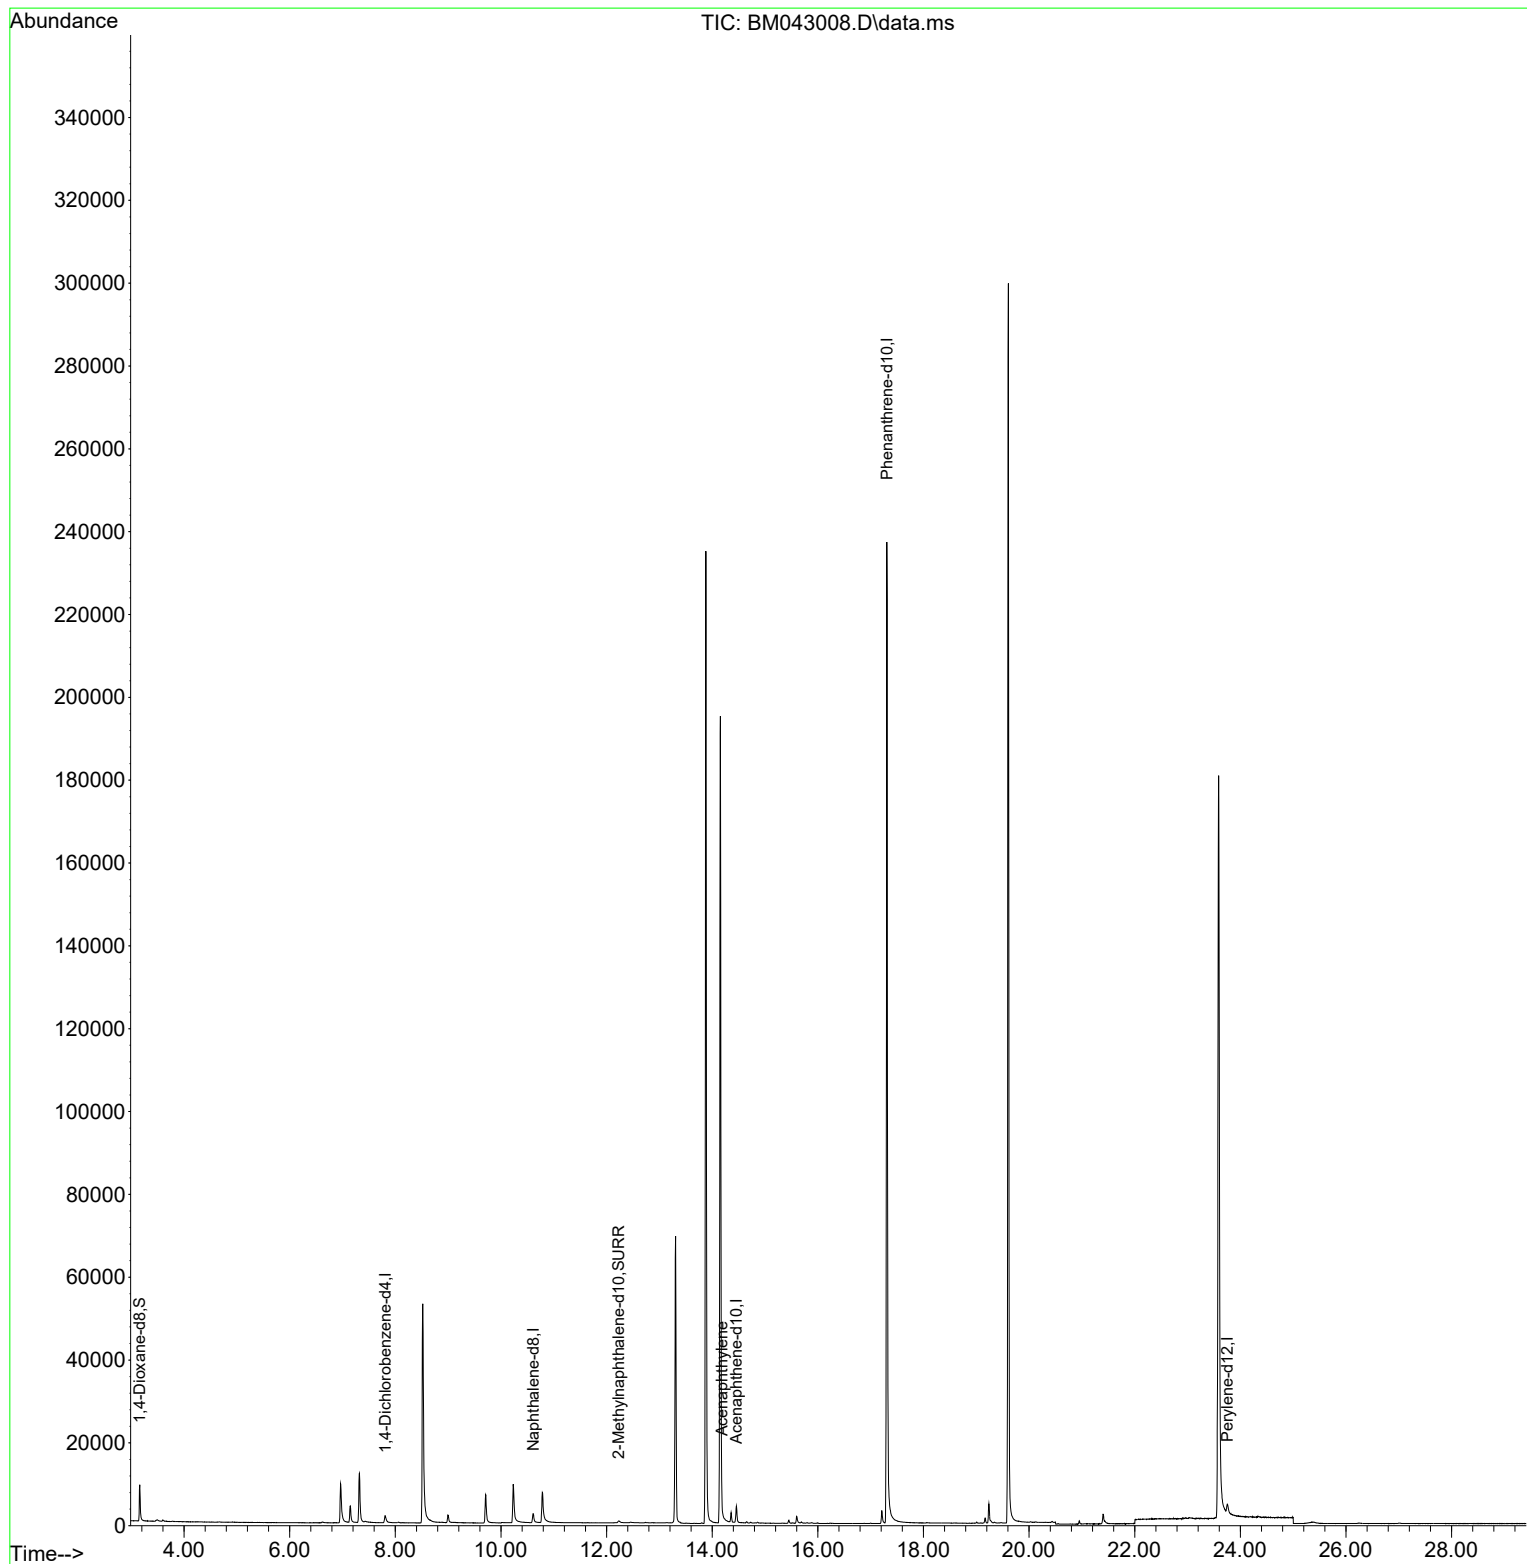

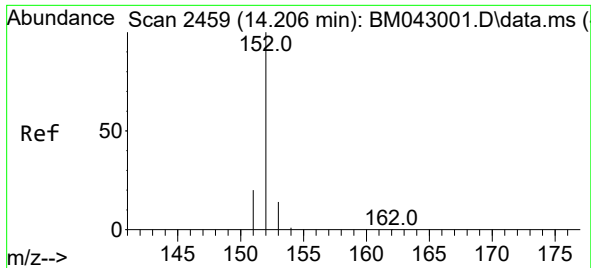

#10
 Acenaphthylene
 Concen: 0.025 ng/ul
 RT: 14.183 min Scan# 2454
 Delta R.T. -0.022 min
 Lab File: BM043008.D
 Acq: 25 Nov 2023 09:38

Instrument :
 BNA_M
 ClientSampleId :
 DCKR1

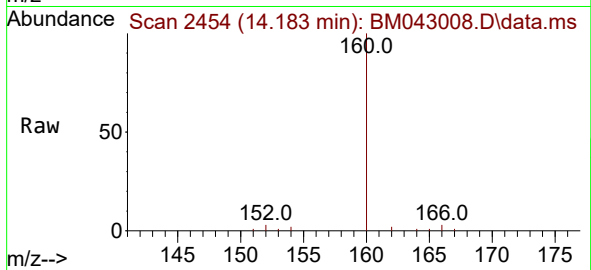

Tgt Ion:152 Resp: 275
 Ion Ratio Lower Upper
 152 100
 151 43.0 19.4 29.0#
 153 41.5 14.6 21.8#

