

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112423\
 Data File : BM043017.D
 Acq On : 25 Nov 2023 15:39
 Operator : MA/JU
 Sample : 05268-09RE
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCKE1

Quant Time: Nov 27 02:43:55 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 27 02:36:19 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.809	152	1036	0.400	ng/ul	#-0.07
4) Naphthalene-d8	10.612	136	3290	0.400	ng/ul	#-0.04
9) Acenaphthene-d10	14.456	164	2006	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.306	188	430466	0.400	ng/ul	# 0.07
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.42
23) Perylene-d12	23.756	264	7301	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.160	96	5307	3.339	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.223	152	1527	0.347	ng/ul	-0.03
18) Fluoranthene-d10	19.244	212	3898	0.000	ng/ul	-0.02
Target Compounds						
26) Benzo(a)pyrene	23.589	252	1852	0.069	ng/ul#	Qvalue 81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112423\
Data File : BM043017.D
Acq On : 25 Nov 2023 15:39
Operator : MA/JU
Sample : 05268-09RE
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKE1


Quant Time: Nov 27 02:43:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 27 02:36:19 2023
Response via : Initial Calibration

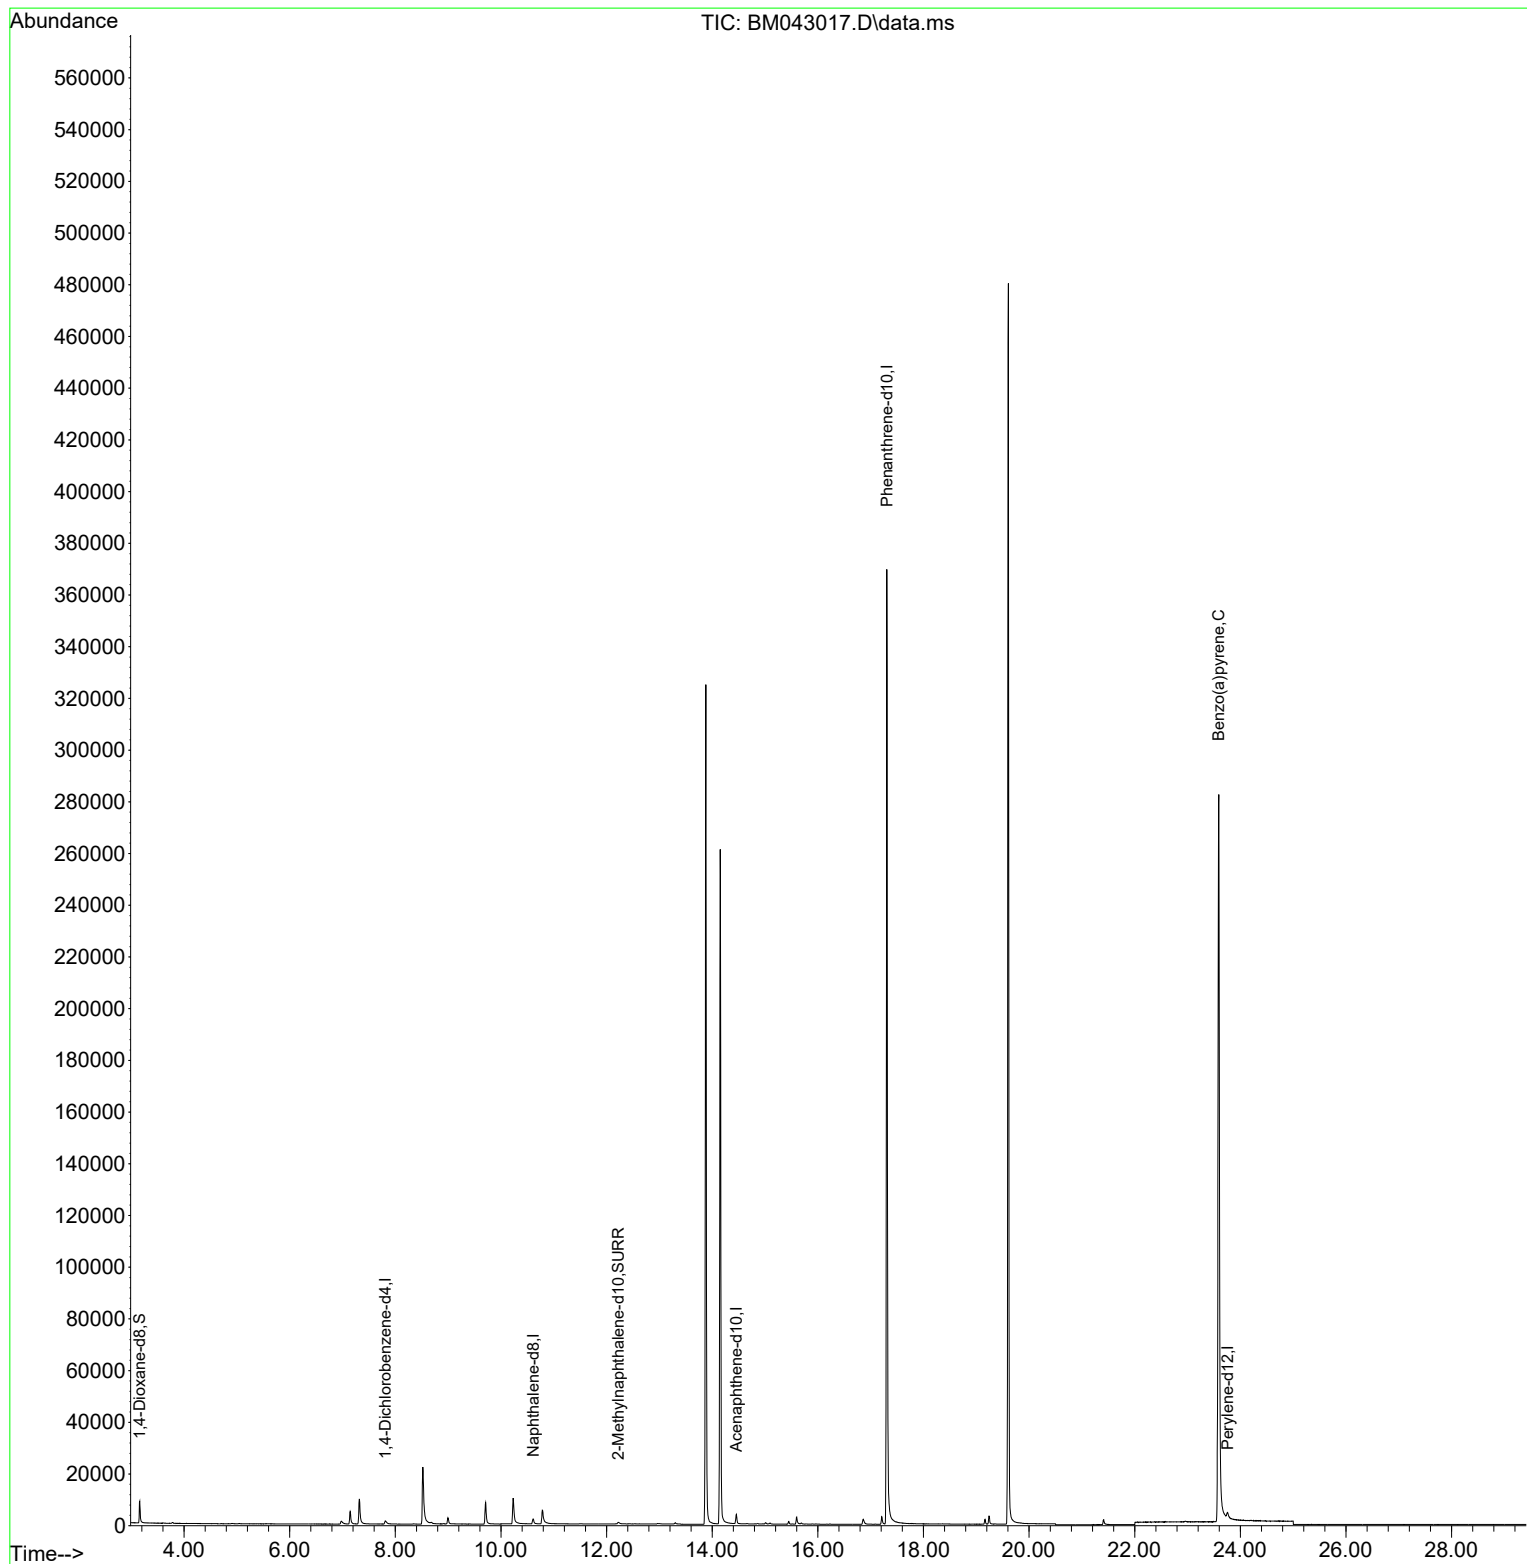

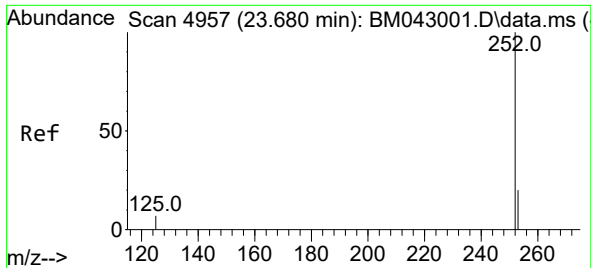

#26
Benzo(a)pyrene
Concen: 0.069 ng/ul
RT: 23.589 min Scan# 4957
Delta R.T. -0.097 min
Lab File: BM043017.D
Acq: 25 Nov 2023 15:39

Instrument :
BNA_M
ClientSampleId :
DCKE1

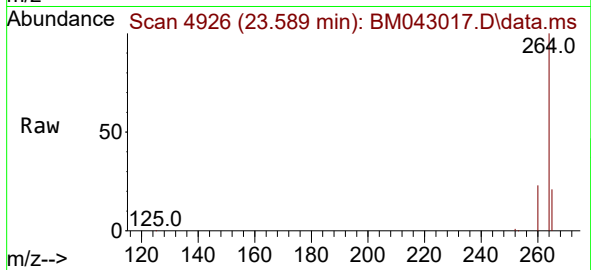

Tgt Ion:252 Resp: 1852
Ion Ratio Lower Upper
252 100
253 55.1 36.6 55.0#
125 34.6 16.2 24.4#

