

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112423\
 Data File : BM043020.D
 Acq On : 25 Nov 2023 17:27
 Operator : MA/JU
 Sample : 05336-14
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCKE5

Quant Time: Nov 27 02:44:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 27 02:36:19 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.813	152	809	0.400	ng/ul	#-0.07
4) Naphthalene-d8	10.612	136	2680	0.400	ng/ul	#-0.04
9) Acenaphthene-d10	14.456	164	1595	0.400	ng/ul	#-0.01
13) Phenanthrene-d10	17.306	188	359604	0.400	ng/ul	# 0.07
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.42
23) Perylene-d12	0.000	264	0	0.000	ng/ul	-23.78
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.160	96	4585	3.694	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.245	152	1158	0.323	ng/ul	0.00
18) Fluoranthene-d10	19.244	212	2972	0.000	ng/ul	-0.02
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.189	88	36	0.027	ng/ul#	79

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112423\
Data File : BM043020.D
Acq On : 25 Nov 2023 17:27
Operator : MA/JU
Sample : 05336-14
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKE5

Quant Time: Nov 27 02:44:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 27 02:36:19 2023
Response via : Initial Calibration

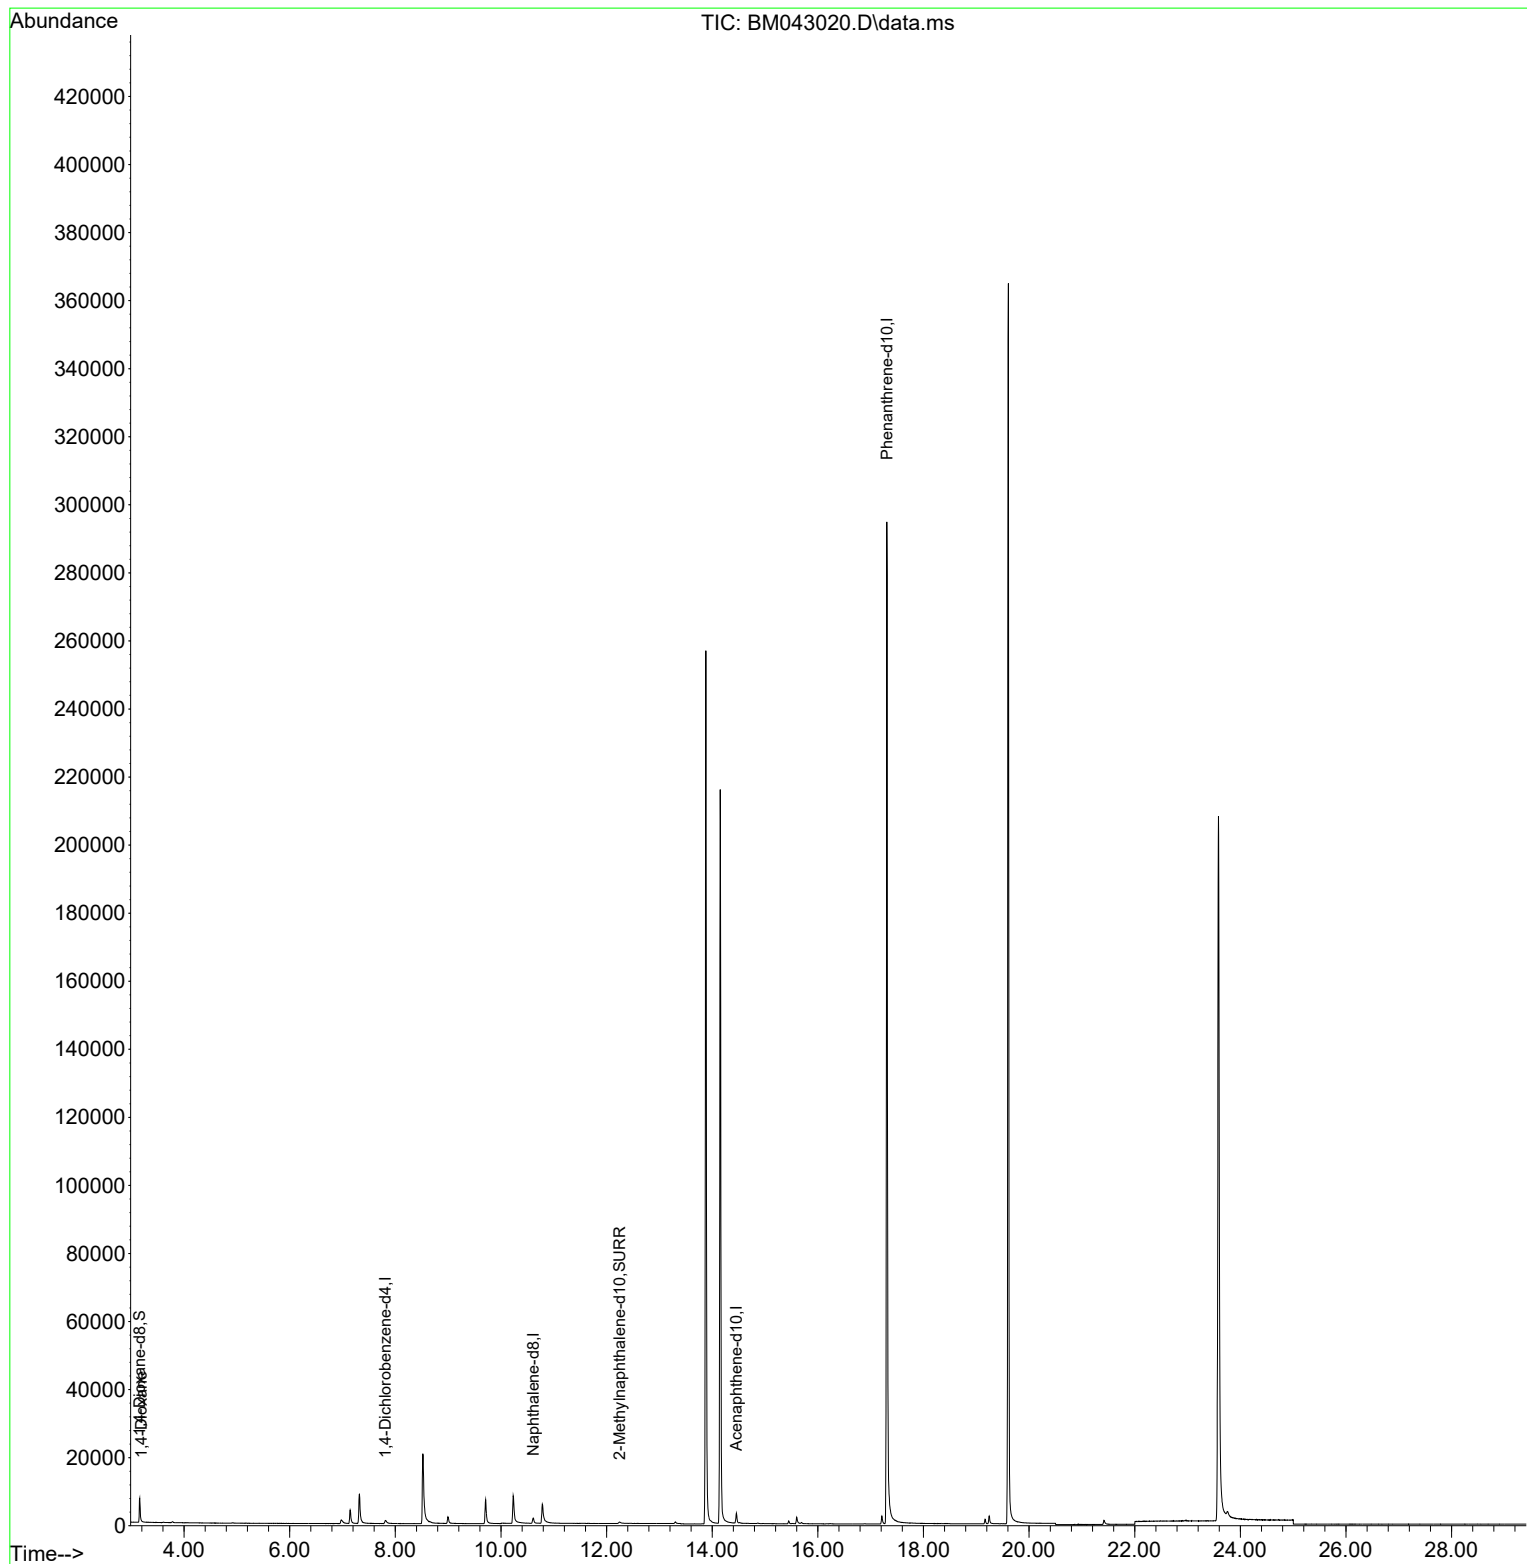


Abundance Scan 53 (3.206 min): BM043001.D\data.ms (-47)

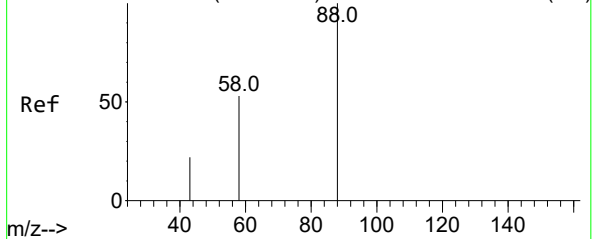

#2
1,4-Dioxane
Concen: 0.027 ng/ul
RT: 3.189 min Scan# 49
Delta R.T. -0.017 min
Lab File: BM043020.D
Acq: 25 Nov 2023 17:27

Instrument :
BNA_M
ClientSampleId :
DCKE5

Abundance Scan 49 (3.189 min): BM043020.D\data.ms

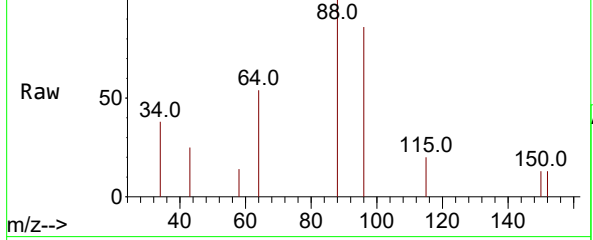

Tgt Ion:	88	Resp:	36
Ion	Ratio	Lower	Upper
88	100		
43	25.5	22.8	34.2
58	14.1	26.8	40.2#

Abundance Scan 49 (3.189 min): BM043020.D\data.ms (-39)

