

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112423\
 Data File : BM043021.D
 Acq On : 25 Nov 2023 18:03
 Operator : MA/JU
 Sample : 05336-15
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCKE7

Quant Time: Nov 27 02:44:17 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 27 02:36:19 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.817	152	691	0.400	ng/ul	#-0.06
4) Naphthalene-d8	10.612	136	2287	0.400	ng/ul	#-0.04
9) Acenaphthene-d10	14.456	164	1366	0.400	ng/ul	#-0.01
13) Phenanthrene-d10	17.306	188	292795	0.400	ng/ul	# 0.07
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.42
23) Perylene-d12	0.000	264	0	0.000	ng/ul	-23.78
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.160	96	5144	4.852	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.240	152	994	0.325	ng/ul	0.00
18) Fluoranthene-d10	19.244	212	2697	0.000	ng/ul	-0.02
Target Compounds						
12) Fluorene	15.451	166	596	0.110	ng/ul#	Qvalue 22


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112423\
Data File : BM043021.D
Acq On : 25 Nov 2023 18:03
Operator : MA/JU
Sample : 05336-15
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKE7


Quant Time: Nov 27 02:44:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 27 02:36:19 2023
Response via : Initial Calibration

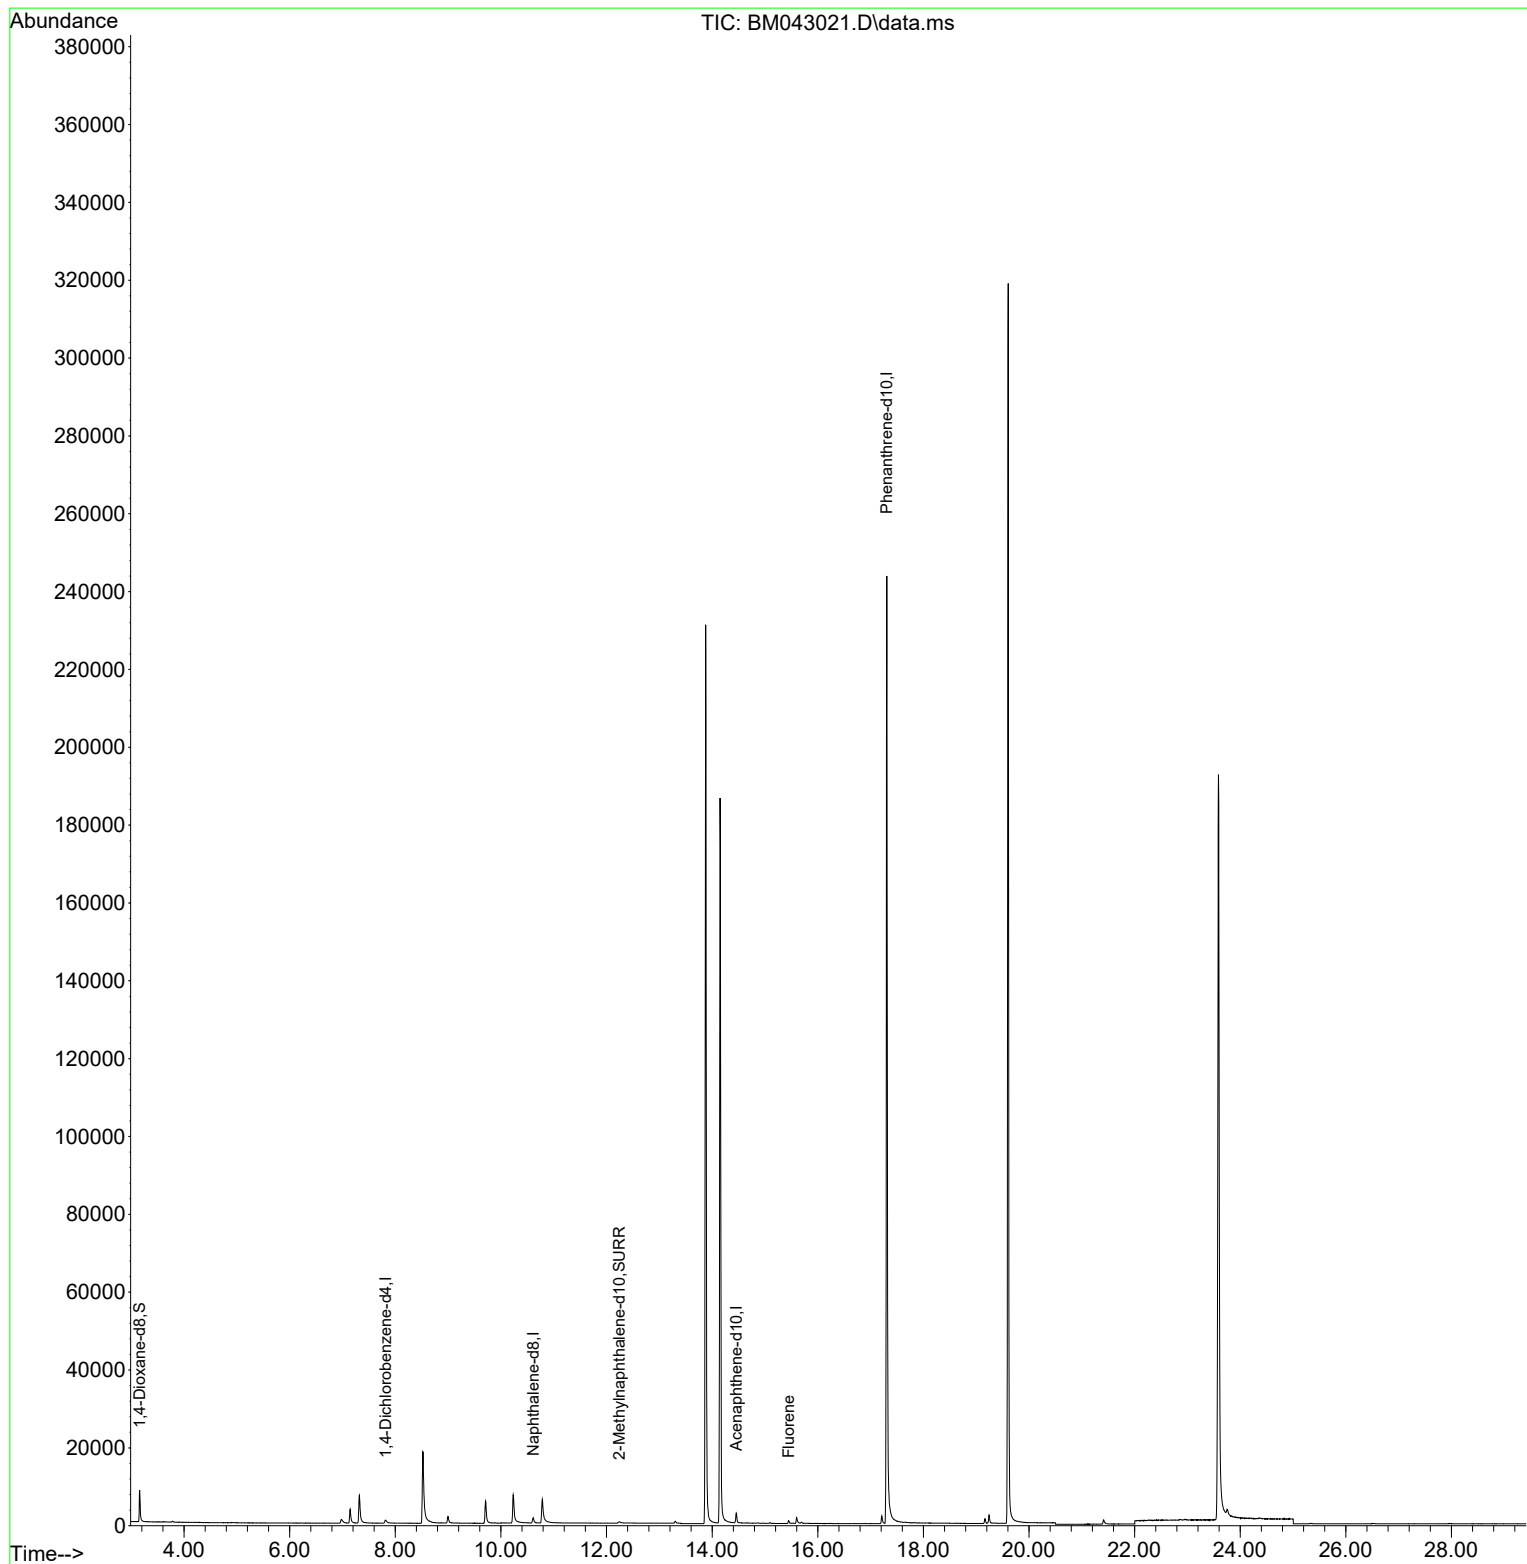

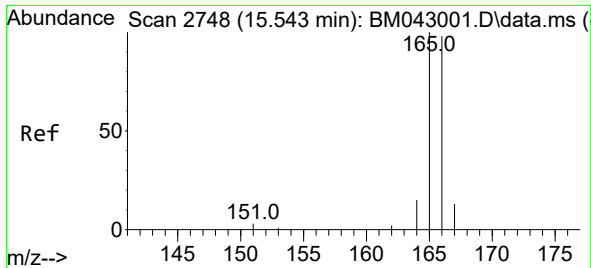

#12
 Fluorene
 Concen: 0.110 ng/ul
 RT: 15.451 min Scan# 21
 Delta R.T. -0.086 min
 Lab File: BM043021.D
 Acq: 25 Nov 2023 18:03

Instrument :
 BNA_M
 ClientSampleId :
 DCKE7

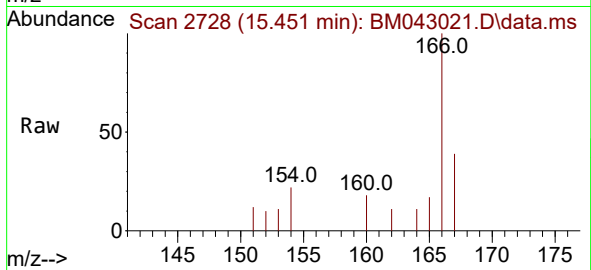

Tgt Ion:166 Resp: 596
 Ion Ratio Lower Upper
 166 100
 165 16.8 79.9 119.9#
 167 38.9 14.2 21.4#

