

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112423\
 Data File : BM043022.D
 Acq On : 25 Nov 2023 18:39
 Operator : MA/JU
 Sample : 05336-16
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCKP7

Quant Time: Nov 27 02:44:22 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 27 02:36:19 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.813	152	796	0.400	ng/ul	#-0.07
4) Naphthalene-d8	10.611	136	2713	0.400	ng/ul	#-0.04
9) Acenaphthene-d10	14.454	164	1653	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.309	188	346521	0.400	ng/ul	# 0.07
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.42
23) Perylene-d12	0.000	264	0	0.000	ng/ul	-23.78
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.159	96	4144	3.393	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.227	152	1206	0.332	ng/ul	-0.02
18) Fluoranthene-d10	19.242	212	3224	0.000	ng/ul	-0.02
Target Compounds						
						Qvalue
10) Acenaphthylene	14.181	152	402	0.048	ng/ul#	76
11) Acenaphthene	14.519	153	3003	0.470	ng/ul	98
12) Fluorene	15.518	166	650	0.099	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112423\
Data File : BM043022.D
Acq On : 25 Nov 2023 18:39
Operator : MA/JU
Sample : 05336-16
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKP7

Quant Time: Nov 27 02:44:22 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 27 02:36:19 2023
Response via : Initial Calibration




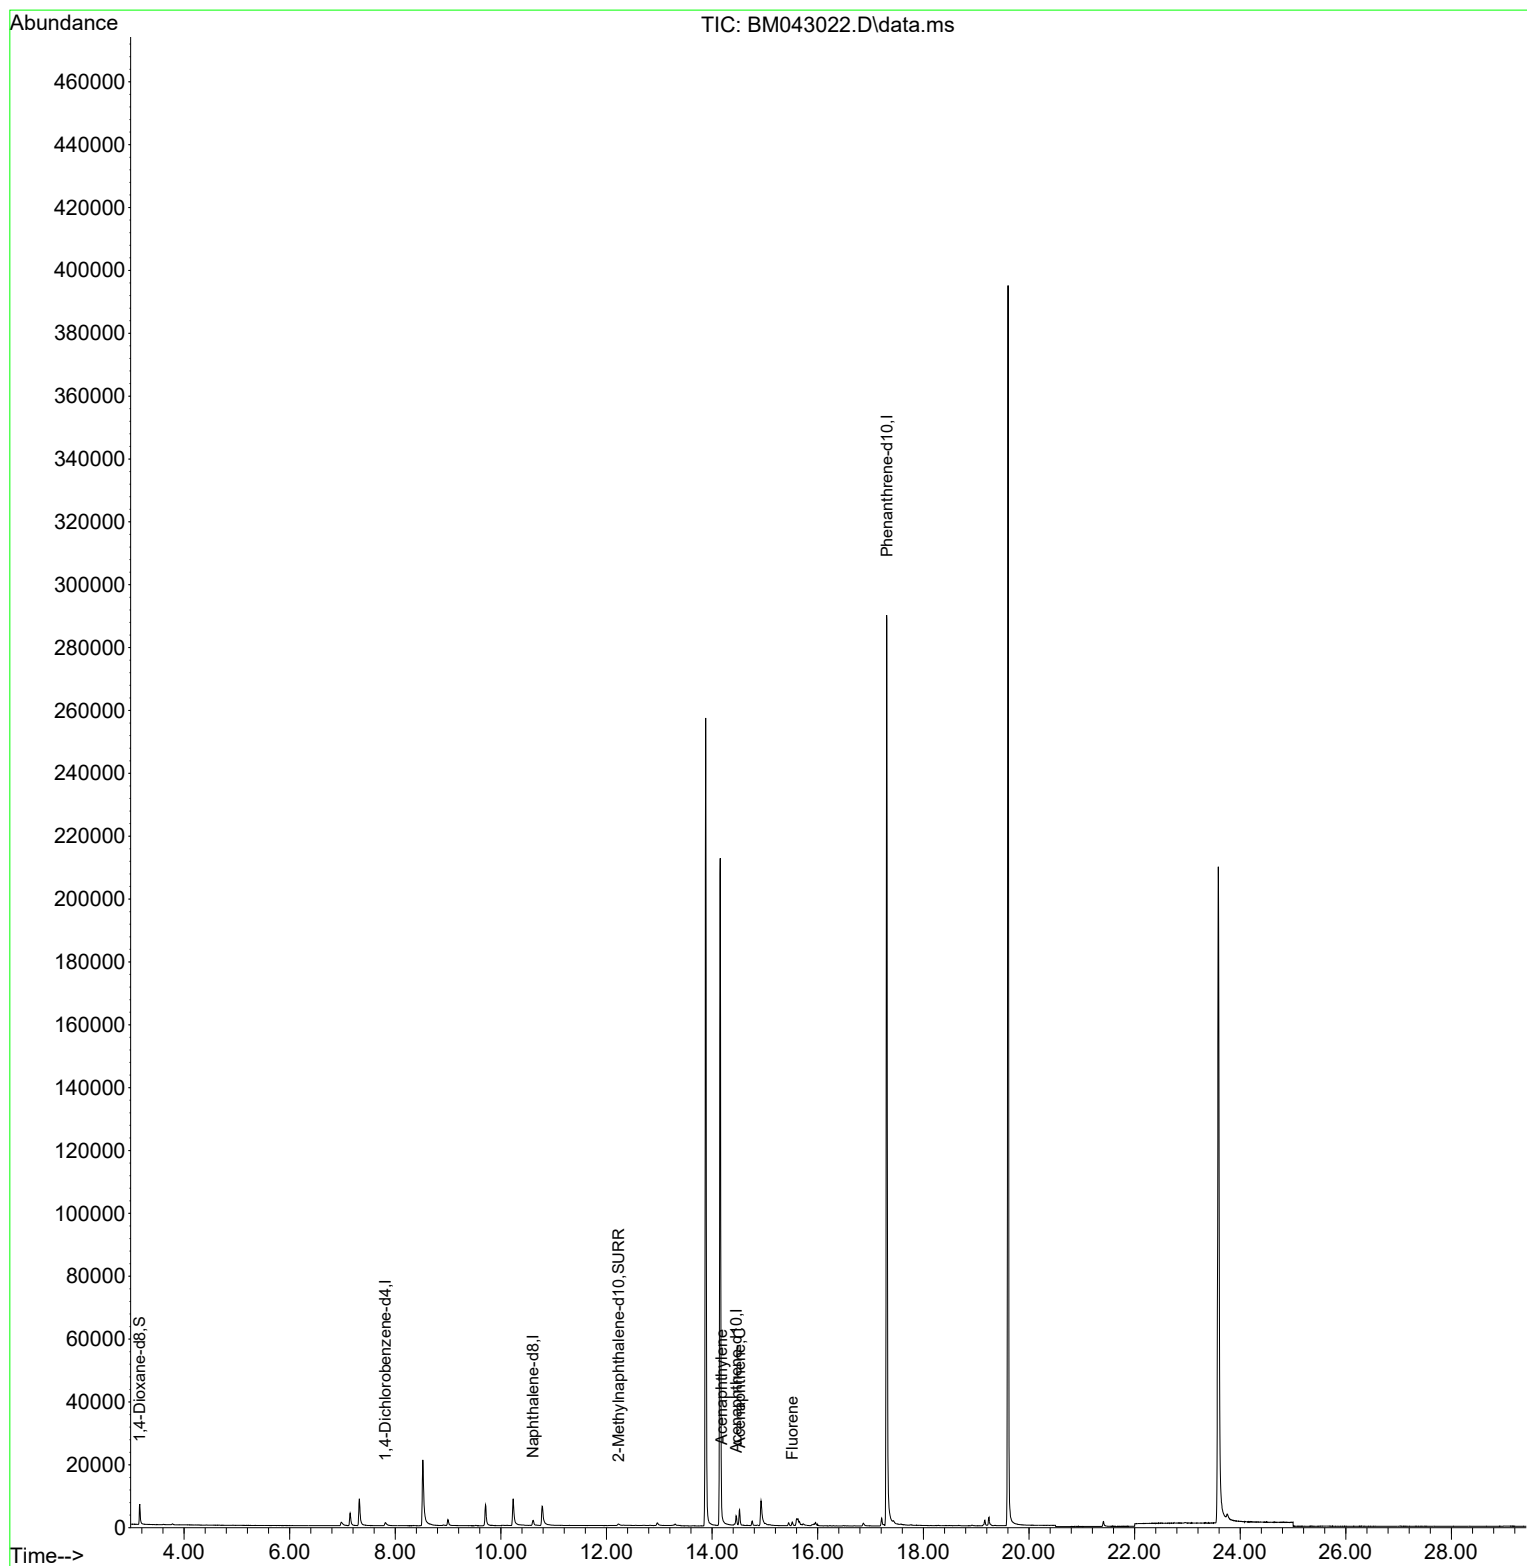


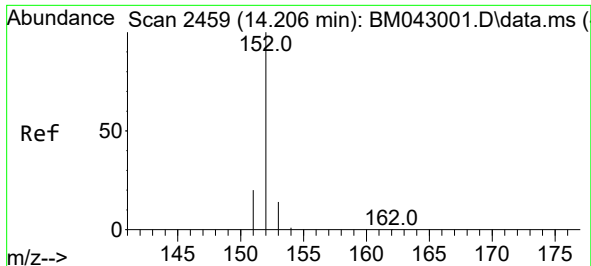

#10
Acenaphthylene
Concen: 0.048 ng/ul
RT: 14.181 min Scan# 2459
Delta R.T. -0.023 min
Lab File: BM043022.D
Acq: 25 Nov 2023 18:39




Instrument :
BNA_M
ClientSampleId :
DCKP7


Tgt Ion:152 Resp: 402
Ion Ratio Lower Upper
152 100
151 34.2 19.4 29.0#
153 31.0 14.6 21.8#

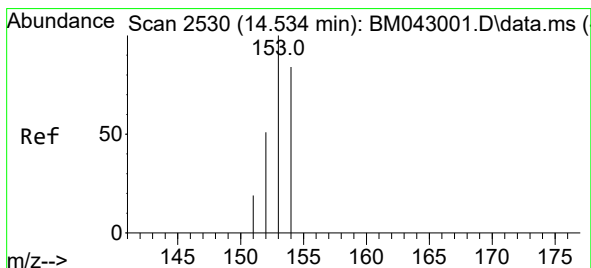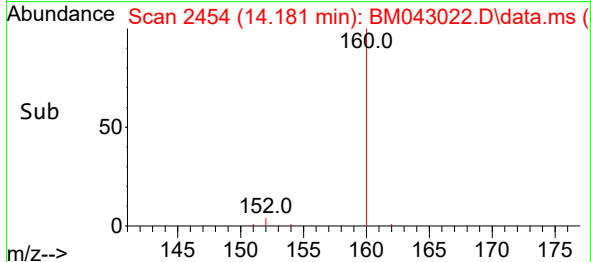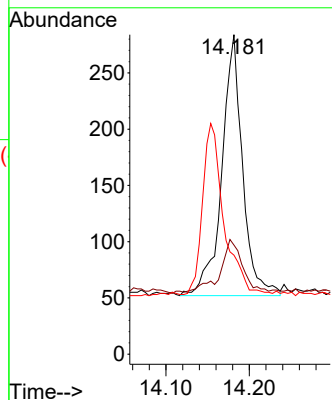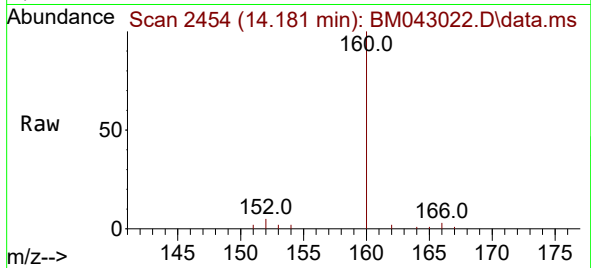

#11
Acenaphthene
Concen: 0.470 ng/ul
RT: 14.519 min Scan# 2527
Delta R.T. -0.014 min
Lab File: BM043022.D
Acq: 25 Nov 2023 18:39


Tgt Ion:153 Resp: 3003
Ion Ratio Lower Upper
153 100
152 51.9 43.9 65.9
154 87.8 70.6 105.8

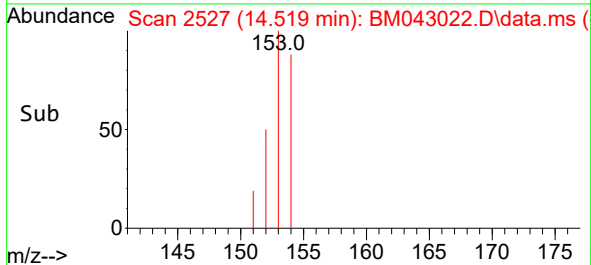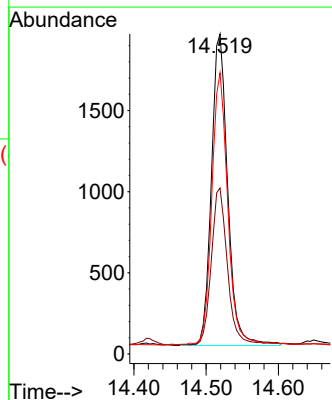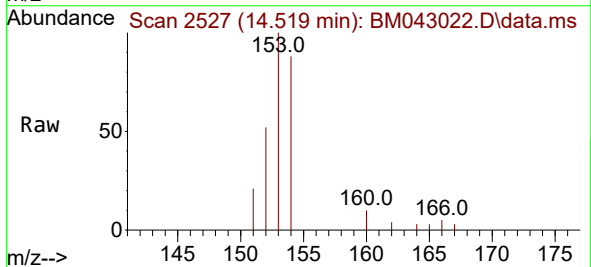

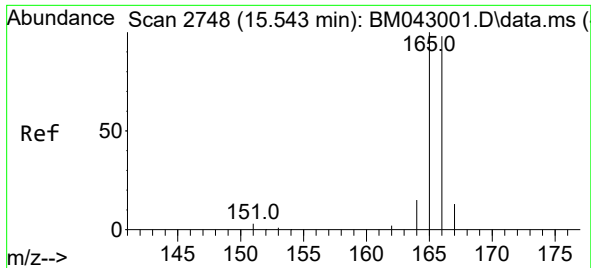

#12
Fluorene
Concen: 0.099 ng/ul
RT: 15.518 min Scan# 21
Delta R.T. -0.018 min
Lab File: BM043022.D
Acq: 25 Nov 2023 18:39

Instrument :
BNA_M
ClientSampleId :
DCKP7

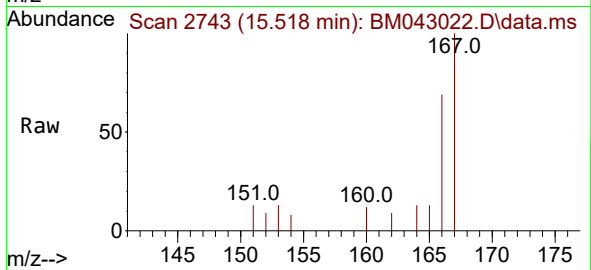

Tgt Ion:166 Resp: 650
Ion Ratio Lower Upper
166 100
165 18.5 79.9 119.9#
167 143.9 14.2 21.4#

