

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112423\
 Data File : BM043024.D
 Acq On : 25 Nov 2023 19:51
 Operator : MA/JU
 Sample : 05264-10
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SLCS192

Quant Time: Nov 27 02:44:35 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 27 02:36:19 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.813	152	746	0.400	ng/ul	#-0.07
4) Naphthalene-d8	10.612	136	2700	0.400	ng/ul	#-0.04
9) Acenaphthene-d10	14.456	164	1723	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.306	188	471332	0.400	ng/ul	# 0.07
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.42
23) Perylene-d12	0.000	264	0	0.000	ng/ul	-23.78
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.159	96	4849	4.236	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.240	152	1402	0.388	ng/ul	0.00
18) Fluoranthene-d10	19.244	212	3768	0.000	ng/ul	-0.02
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.176	88	27	0.022	ng/ul#	78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112423\
Data File : BM043024.D
Acq On : 25 Nov 2023 19:51
Operator : MA/JU
Sample : 05264-10
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SLCS192


Quant Time: Nov 27 02:44:35 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 27 02:36:19 2023
Response via : Initial Calibration

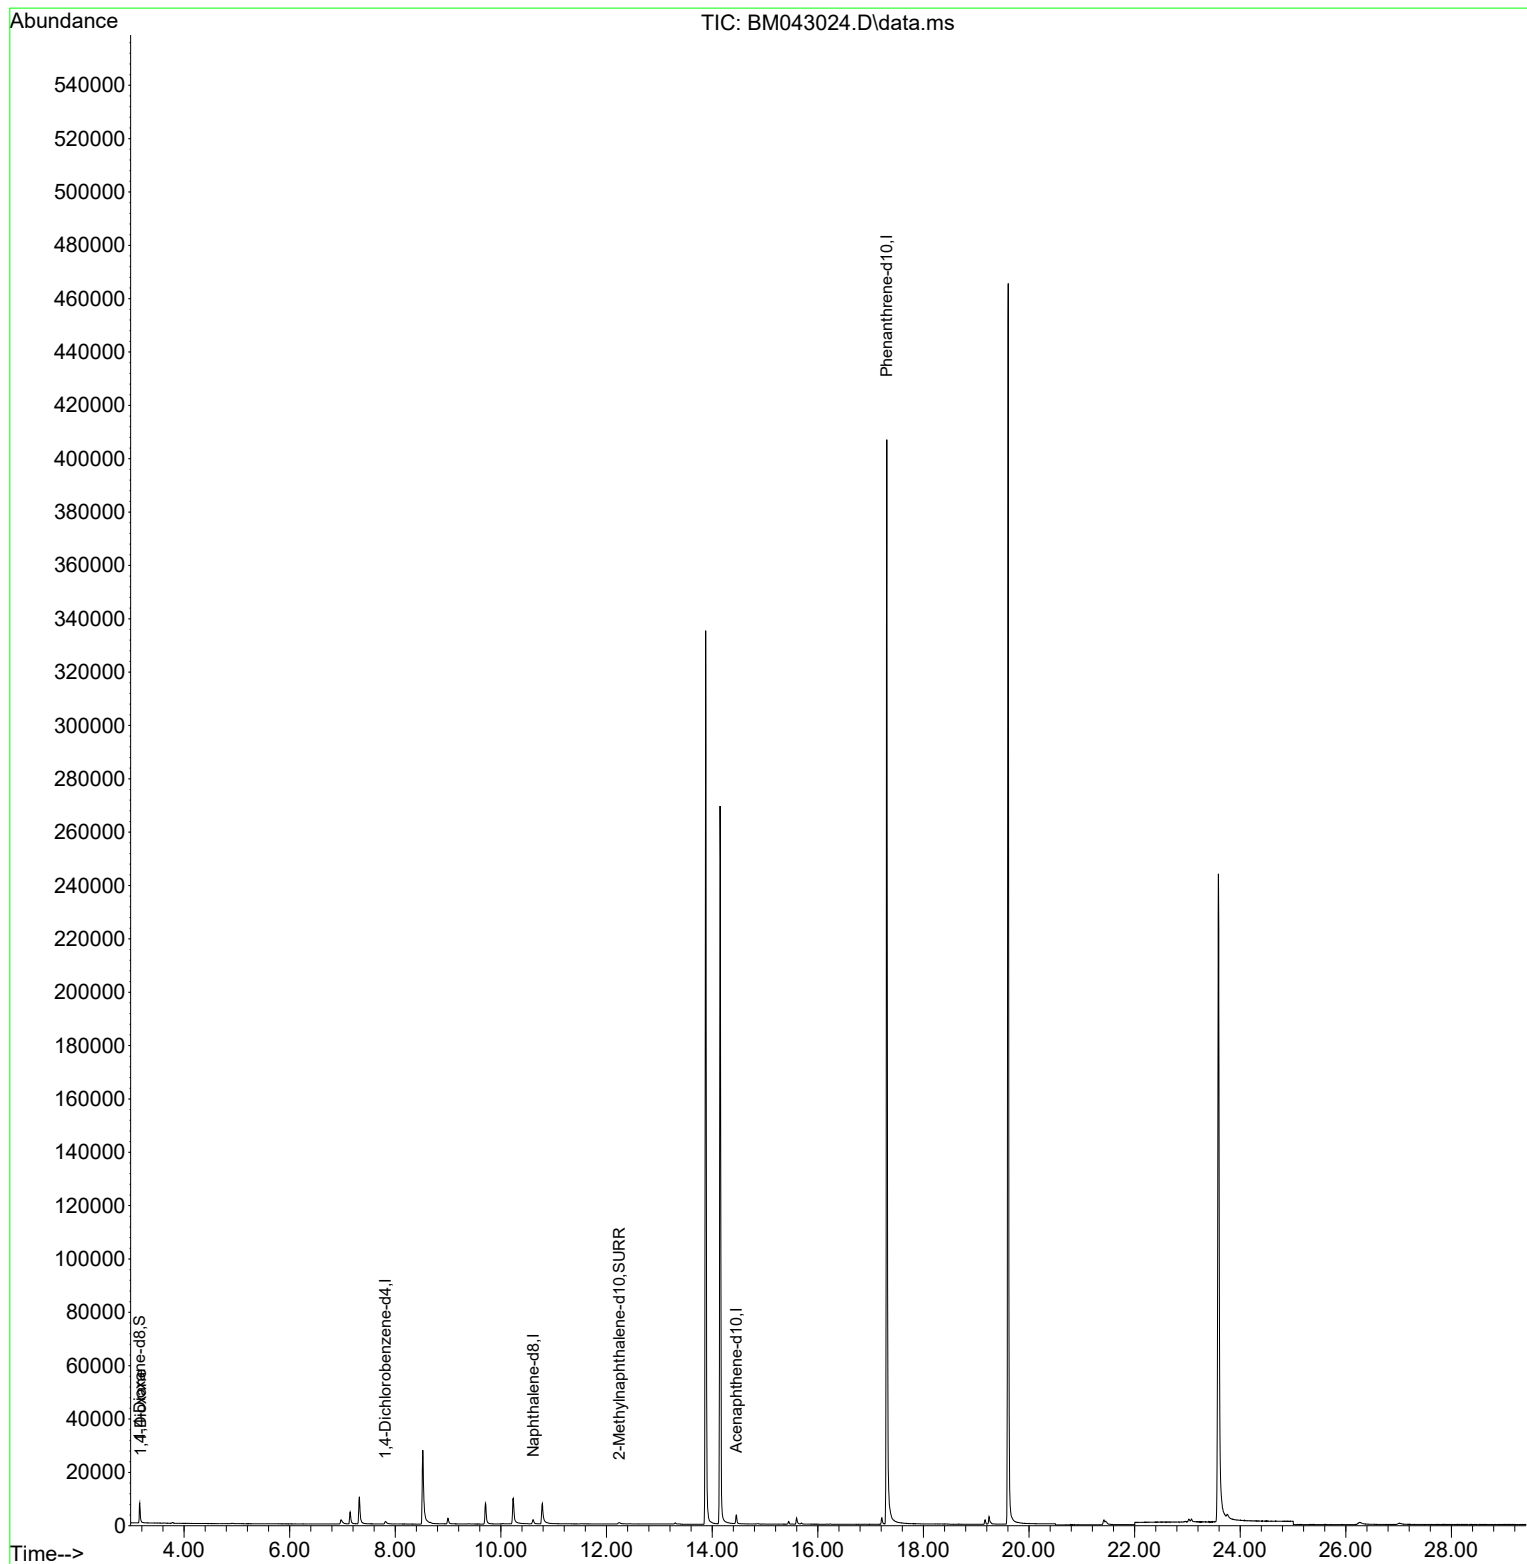

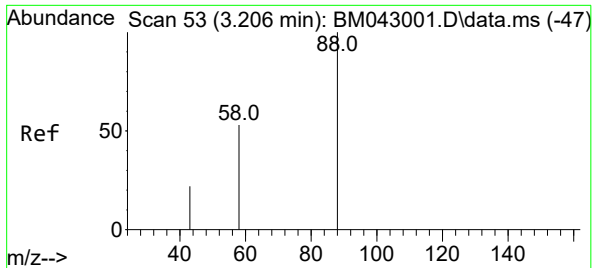

#2
 1,4-Dioxane
 Concen: 0.022 ng/ul
 RT: 3.176 min Scan# 40
 Delta R.T. -0.029 min
 Lab File: BM043024.D
 Acq: 25 Nov 2023 19:51

Instrument :
 BNA_M
 ClientSampleId :
 SLCS192

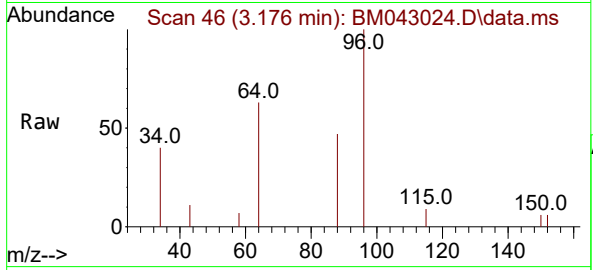

Tgt Ion: 88 Resp: 27

Ion	Ratio	Lower	Upper
88	100		
43	24.2	22.8	34.2
58	14.0	26.8	40.2#

