

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112423\
 Data File : BM043028.D
 Acq On : 25 Nov 2023 22:52
 Operator : MA/JU
 Sample : PB157274BL
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK100

Quant Time: Nov 27 02:45:13 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 27 02:36:19 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.817	152	1011	0.400	ng/ul	#-0.06
4) Naphthalene-d8	10.612	136	3381	0.400	ng/ul	#-0.04
9) Acenaphthene-d10	14.456	164	2039	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.306	188	332910	0.400	ng/ul	# 0.07
17) Chrysene-d12	21.426	240	2008	0.400	ng/ul	0.00
23) Perylene-d12	0.000	264	0	0.000	ng/ul	-23.78
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.160	96	6430	4.145	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.251	152	1139	0.252	ng/ul	0.00
18) Fluoranthene-d10	19.244	212	2595	0.355	ng/ul	-0.02
Target Compounds						
					Qvalue	
12) Fluorene	15.450	166	667	0.082	ng/ul#	20
20) Pyrene	19.606	202	650	0.054	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112423\
Data File : BM043028.D
Acq On : 25 Nov 2023 22:52
Operator : MA/JU
Sample : PB157274BL
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK100

Quant Time: Nov 27 02:45:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 27 02:36:19 2023
Response via : Initial Calibration




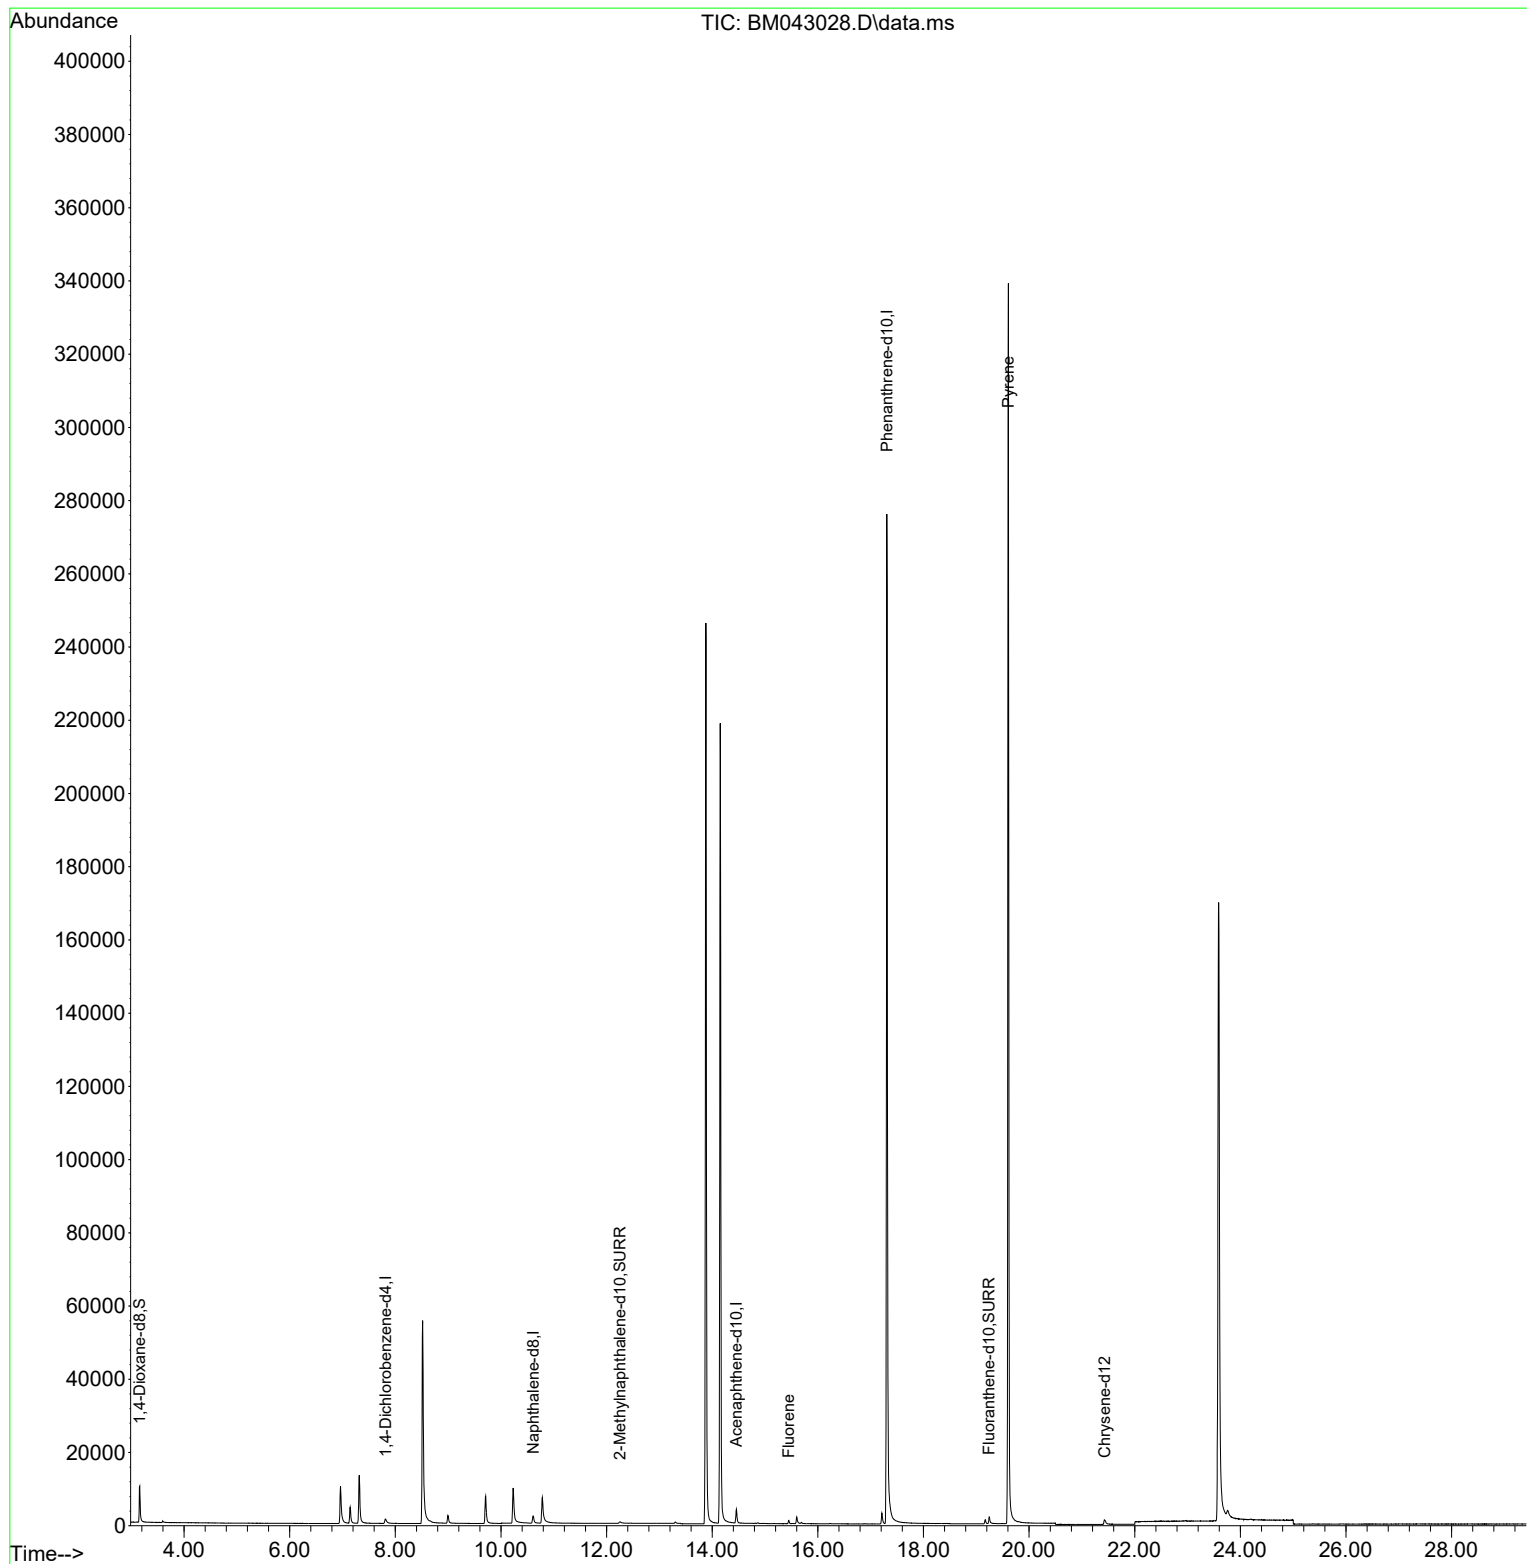


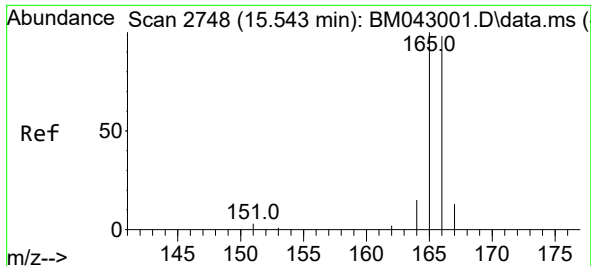

#12
Fluorene
Concen: 0.082 ng/ul
RT: 15.450 min Scan# 21
Delta R.T. -0.087 min
Lab File: BM043028.D
Acq: 25 Nov 2023 22:52

Instrument :
BNA_M
ClientSampleId :
SBLK100

Tgt Ion:166 Resp: 667
Ion Ratio Lower Upper
166 100
165 14.9 79.9 119.9#
167 40.7 14.2 21.4#

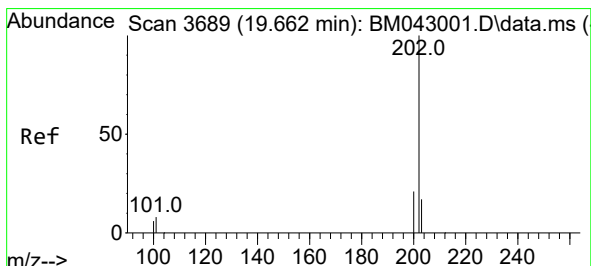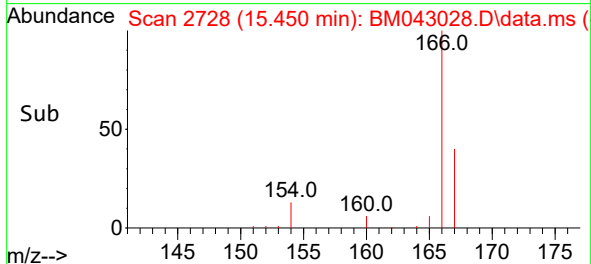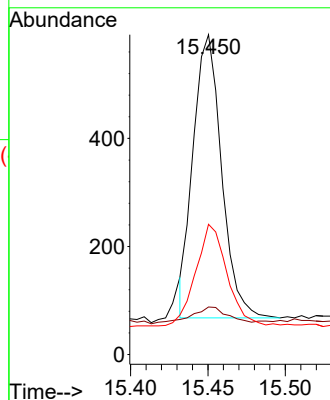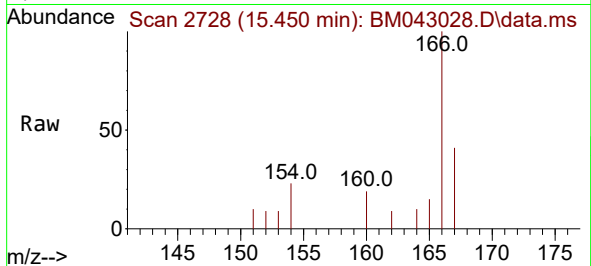

#20
Pyrene
Concen: 0.054 ng/ul
RT: 19.606 min Scan# 3677
Delta R.T. -0.054 min
Lab File: BM043028.D
Acq: 25 Nov 2023 22:52

Tgt Ion:202 Resp: 650
Ion Ratio Lower Upper
202 100
101 182.9 8.7 13.1#
100 1365.1 7.8 11.8#

