

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112423\
 Data File : BM043032.D
 Acq On : 26 Nov 2023 01:18
 Operator : MA/JU
 Sample : 05264-11
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCKS6

Quant Time: Nov 27 02:45:35 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 27 02:36:19 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.809	152	911	0.400	ng/ul	#-0.07
4) Naphthalene-d8	10.611	136	3256	0.400	ng/ul	#-0.04
9) Acenaphthene-d10	14.454	164	1981	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.305	188	364894	0.400	ng/ul	# 0.07
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.42
23) Perylene-d12	0.000	264	0	0.000	ng/ul	-23.78
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.160	96	5915	4.232	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.222	152	1612	0.370	ng/ul	-0.03
18) Fluoranthene-d10	19.242	212	3577	0.000	ng/ul	-0.02
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.193	88	40	0.027	ng/ul#	80
5) Naphthalene	10.660	128	363	0.041	ng/ul#	68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112423\
Data File : BM043032.D
Acq On : 26 Nov 2023 01:18
Operator : MA/JU
Sample : 05264-11
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKS6

Quant Time: Nov 27 02:45:35 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 27 02:36:19 2023
Response via : Initial Calibration




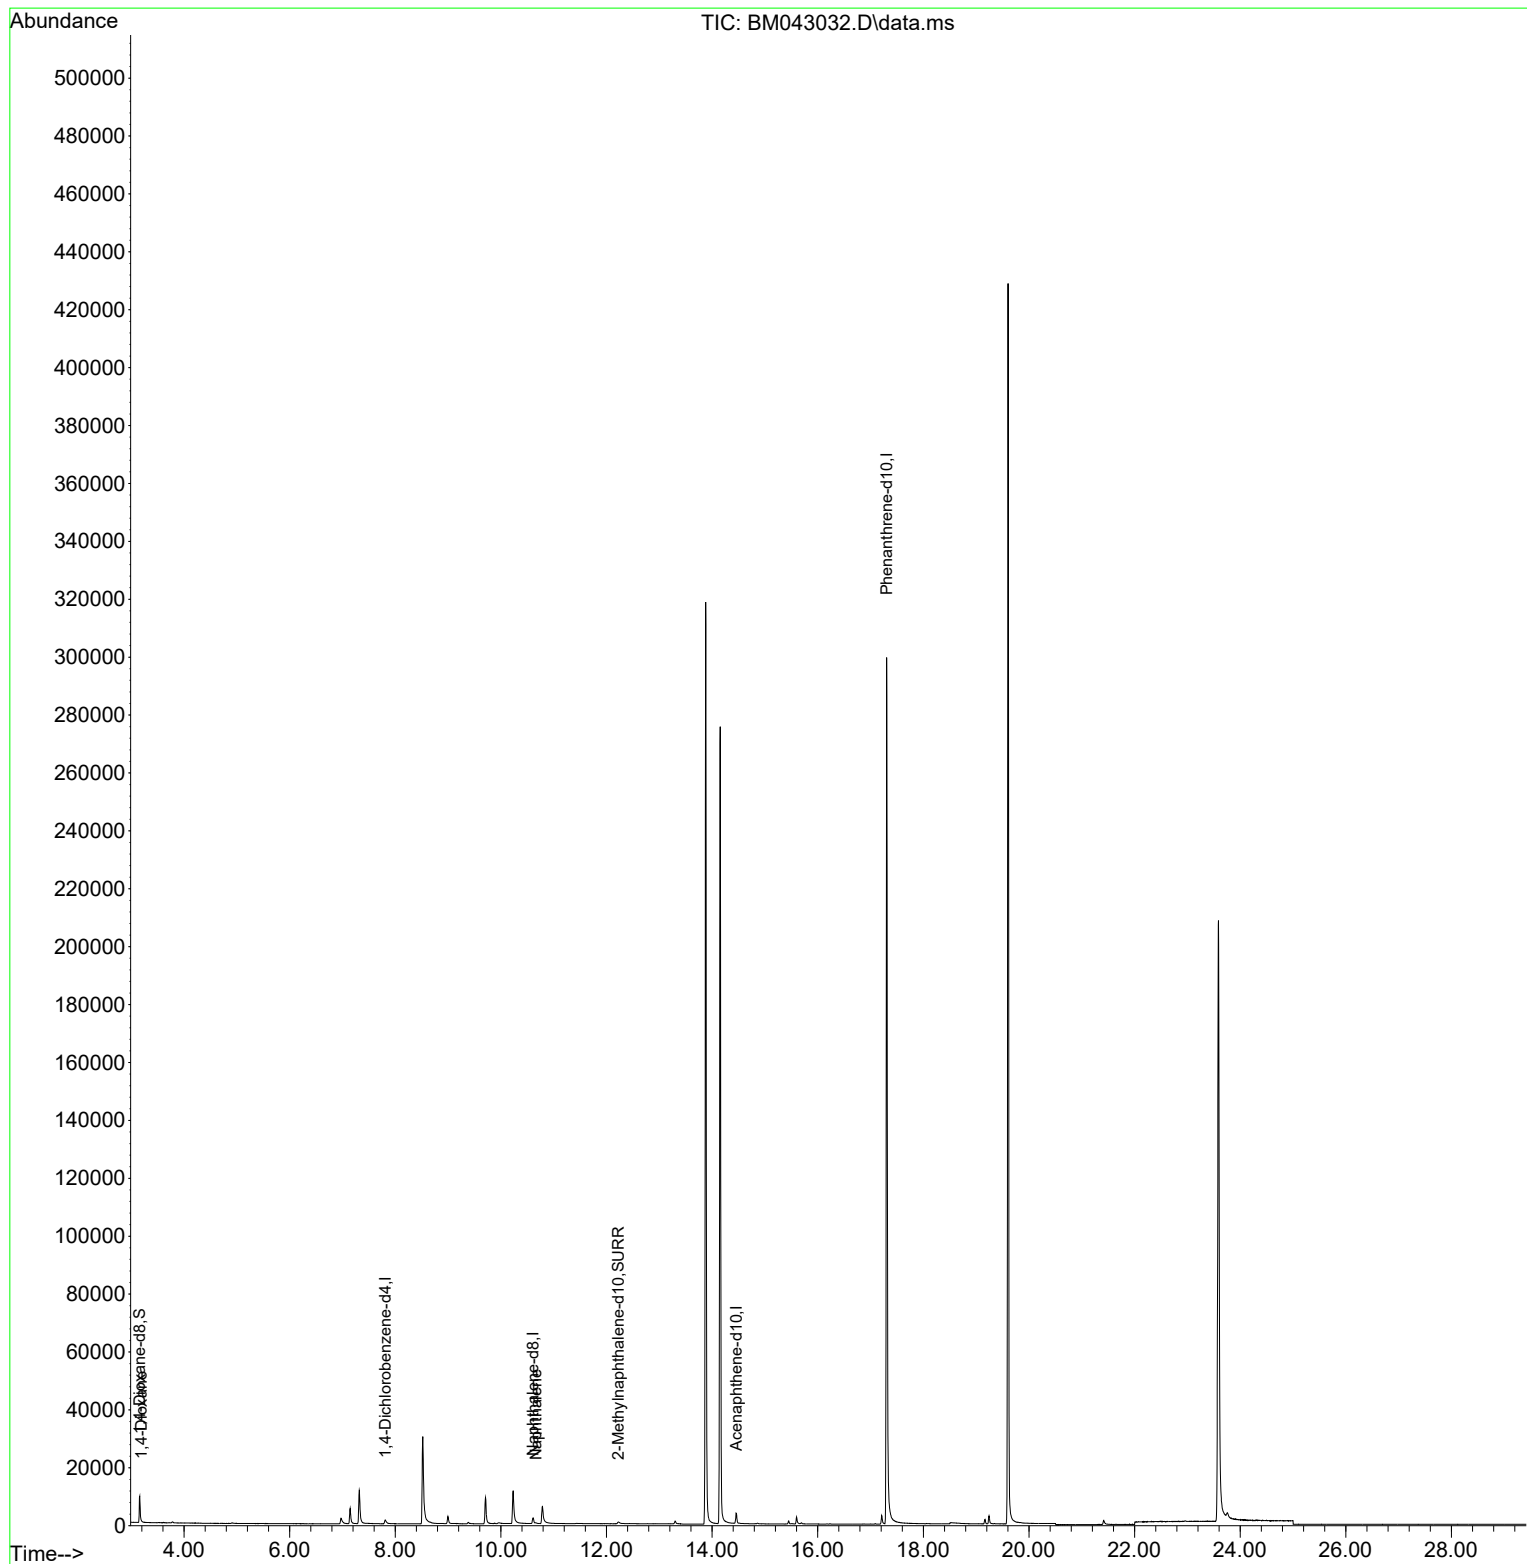


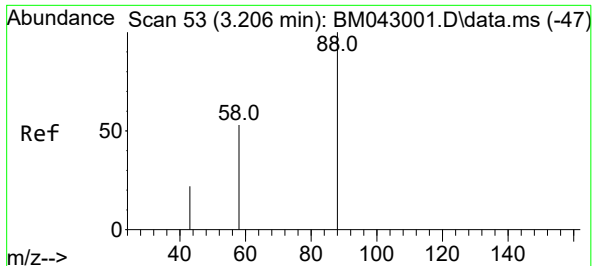

#2
1,4-Dioxane
Concen: 0.027 ng/ul
RT: 3.193 min Scan# 50
Delta R.T. -0.012 min
Lab File: BM043032.D
Acq: 26 Nov 2023 01:18

Instrument :
BNA_M
ClientSampleId :
DCKS6

Tgt Ion: 88 Resp: 40
Ion Ratio Lower Upper
88 100
43 32.1 22.8 34.2
58 15.3 26.8 40.2#

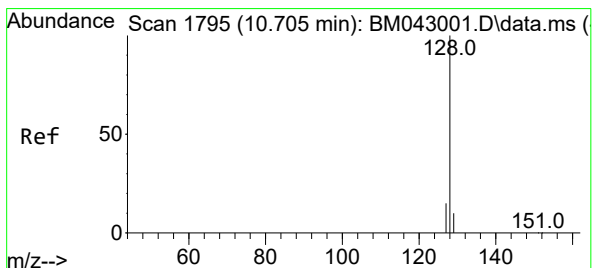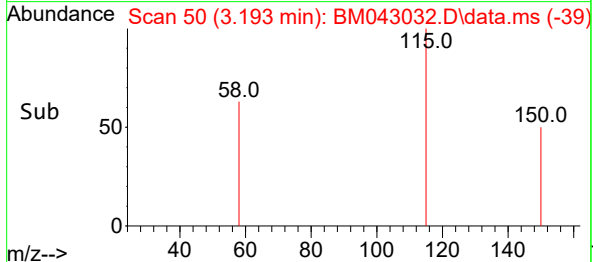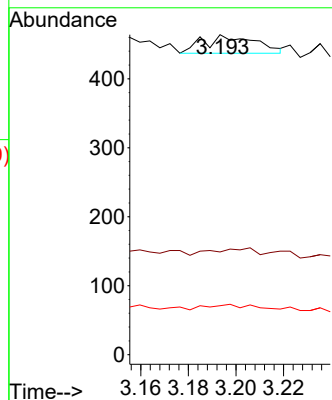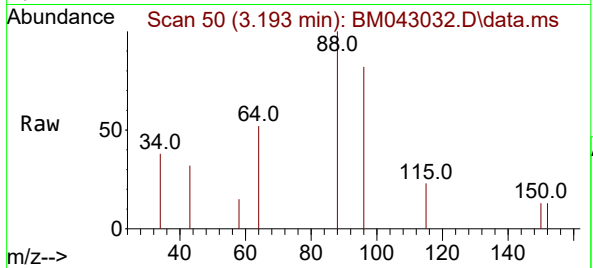

#5
Naphthalene
Concen: 0.041 ng/ul
RT: 10.660 min Scan# 1787
Delta R.T. -0.038 min
Lab File: BM043032.D
Acq: 26 Nov 2023 01:18

Tgt Ion: 128 Resp: 363
Ion Ratio Lower Upper
128 100
129 35.7 16.0 24.0#
127 34.9 16.5 24.7#

