

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112423\
 Data File : BM043034.D
 Acq On : 26 Nov 2023 02:30
 Operator : MA/JU
 Sample : 05264-16
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCKC5

Quant Time: Nov 27 02:45:46 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 27 02:36:19 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.809	152	782	0.400	ng/ul	#-0.07
4) Naphthalene-d8	10.611	136	2564	0.400	ng/ul	#-0.04
9) Acenaphthene-d10	14.454	164	1563	0.400	ng/ul	#-0.01
13) Phenanthrene-d10	17.304	188	374226	0.400	ng/ul	# 0.07
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.42
23) Perylene-d12	0.000	264	0	0.000	ng/ul	-23.78
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.159	96	4164	3.470	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.233	152	1403	0.409	ng/ul	-0.02
18) Fluoranthene-d10	19.242	212	3674	0.000	ng/ul	-0.02
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.189	88	44	0.034	ng/ul#	81
12) Fluorene	15.514	166	158	0.025	ng/ul#	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112423\
Data File : BM043034.D
Acq On : 26 Nov 2023 02:30
Operator : MA/JU
Sample : 05264-16
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKC5

Quant Time: Nov 27 02:45:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 27 02:36:19 2023
Response via : Initial Calibration




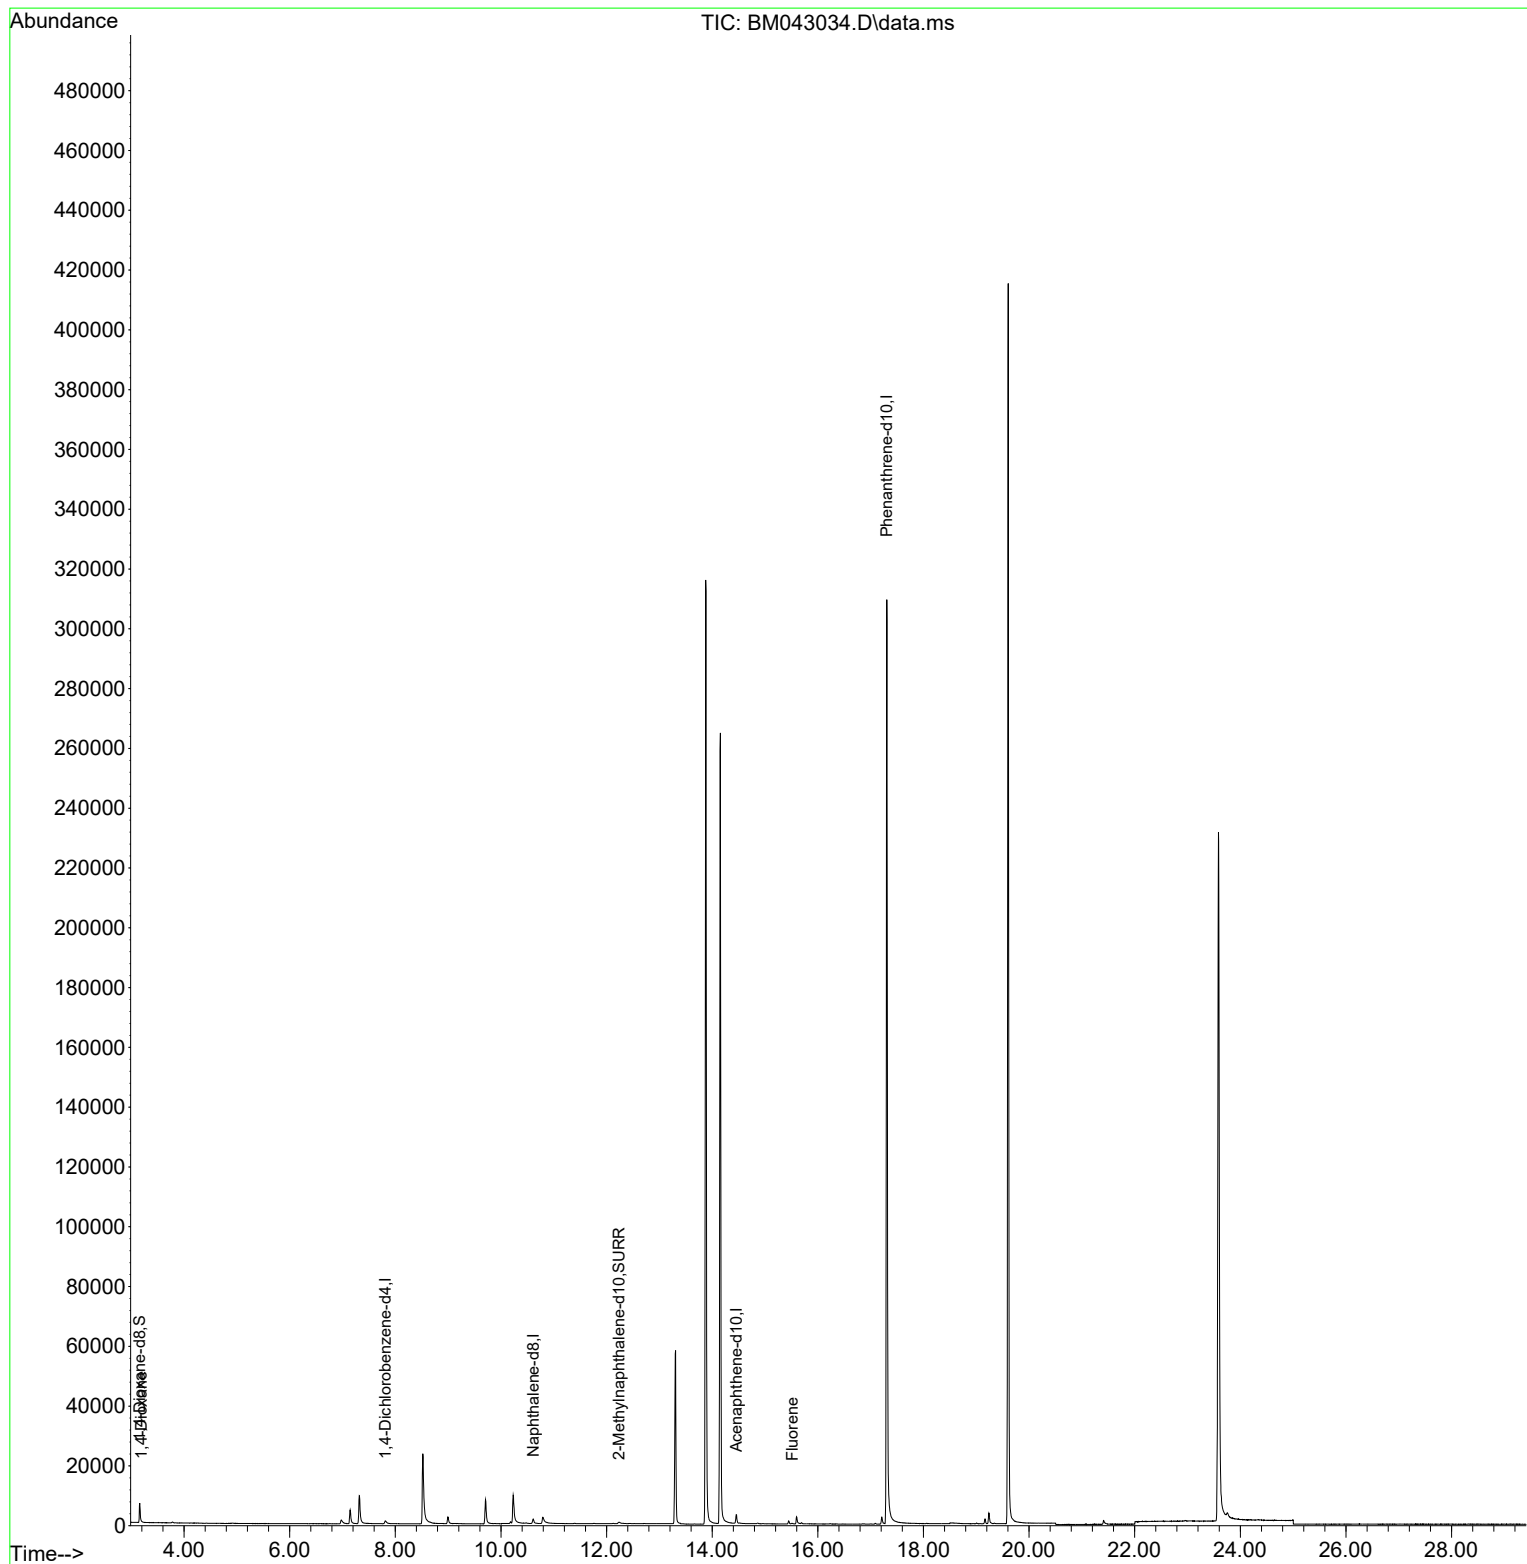


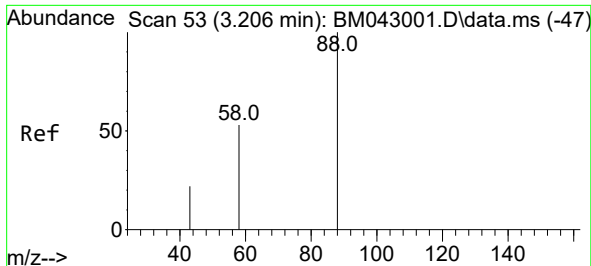

#2
1,4-Dioxane
Concen: 0.034 ng/ul
RT: 3.189 min Scan# 49
Delta R.T. -0.017 min
Lab File: BM043034.D
Acq: 26 Nov 2023 02:30

Instrument :
BNA_M
ClientSampleId :
DCKC5

Tgt Ion: 88 Resp: 44
Ion Ratio Lower Upper
88 100
43 28.7 22.8 34.2
58 13.8 26.8 40.2#

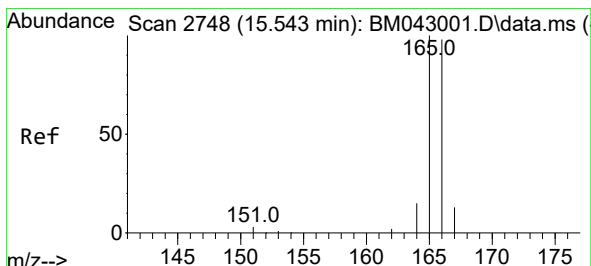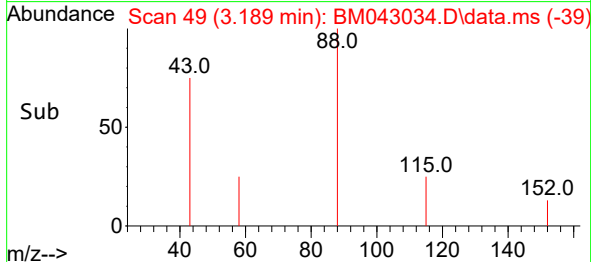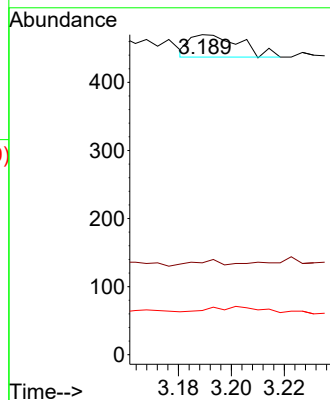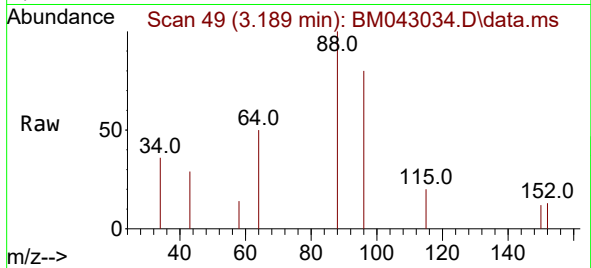

#12
Fluorene
Concen: 0.025 ng/ul
RT: 15.514 min Scan# 2742
Delta R.T. -0.023 min
Lab File: BM043034.D
Acq: 26 Nov 2023 02:30

Tgt Ion:166 Resp: 158
Ion Ratio Lower Upper
166 100
165 88.4 79.9 119.9
167 45.9 14.2 21.4#

