

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112423\
 Data File : BM043035.D
 Acq On : 26 Nov 2023 03:07
 Operator : MA/JU
 Sample : 05336-07
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCKC6

Quant Time: Nov 27 02:45:51 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 27 02:36:19 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.813	152	973	0.400	ng/ul	#-0.07
4) Naphthalene-d8	10.606	136	3272	0.400	ng/ul	#-0.04
9) Acenaphthene-d10	14.456	164	1886	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.306	188	419307	0.400	ng/ul	# 0.07
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.42
23) Perylene-d12	23.756	264	6350	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.160	96	4706	3.152	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.234	152	1322	0.302	ng/ul	-0.02
18) Fluoranthene-d10	19.244	212	3530	0.000	ng/ul	-0.02
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.164	88	77	0.048	ng/ul#	79
12) Fluorene	15.506	166	498	0.067	ng/ul#	88
26) Benzo(a)pyrene	23.586	252	1415	0.061	ng/ul#	76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112423\
Data File : BM043035.D
Acq On : 26 Nov 2023 03:07
Operator : MA/JU
Sample : 05336-07
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKC6

Quant Time: Nov 27 02:45:51 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 27 02:36:19 2023
Response via : Initial Calibration




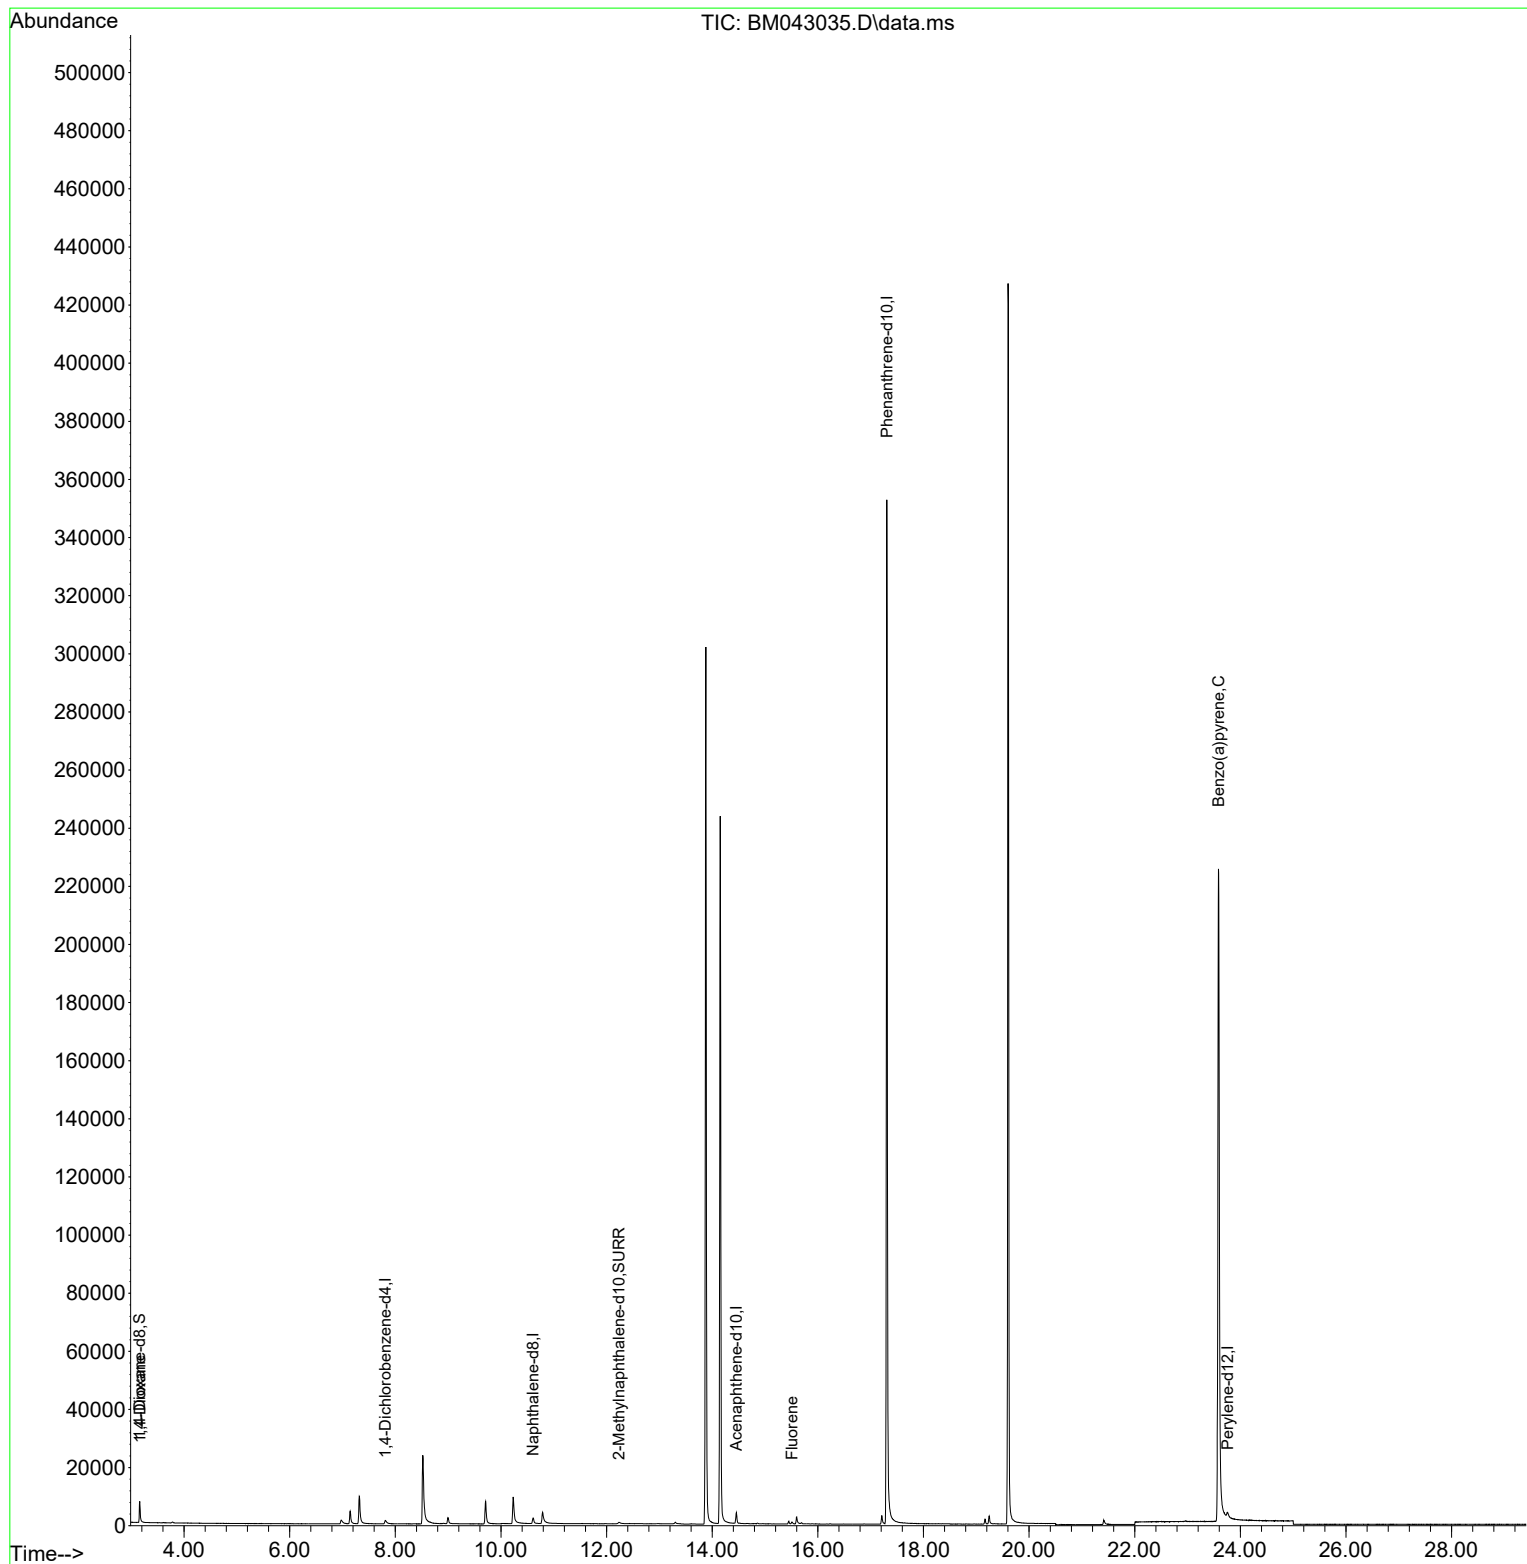


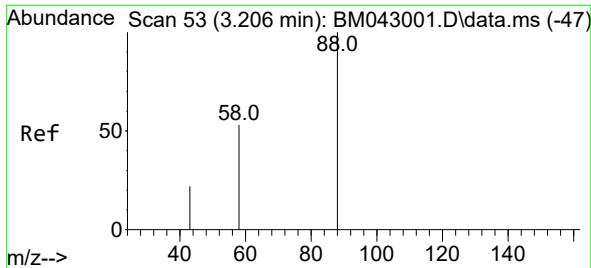

#2
1,4-Dioxane
Concen: 0.048 ng/ul
RT: 3.164 min Scan# 41
Delta R.T. -0.042 min
Lab File: BM043035.D
Acq: 26 Nov 2023 03:07




Instrument :
BNA_M
ClientSampleId :
DCKC6


Tgt Ion: 88 Resp: 77
Ion Ratio Lower Upper
88 100
43 27.0 22.8 34.2
58 13.2 26.8 40.2#

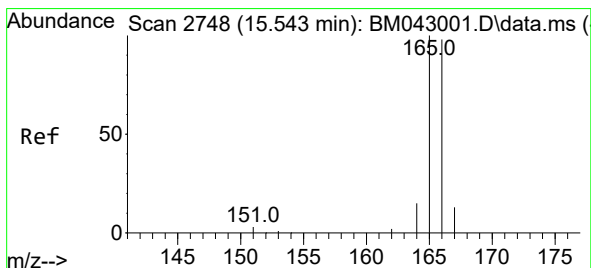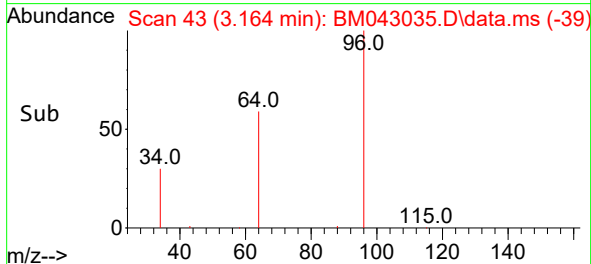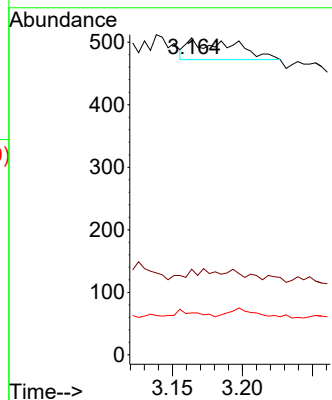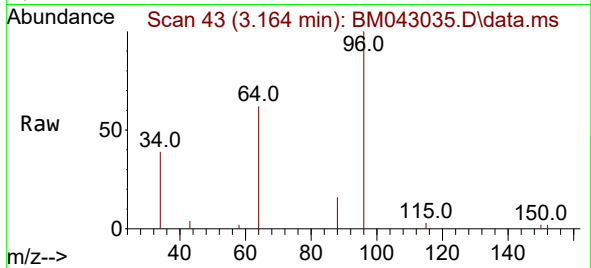

#12
Fluorene
Concen: 0.067 ng/ul
RT: 15.506 min Scan# 2740
Delta R.T. -0.031 min
Lab File: BM043035.D
Acq: 26 Nov 2023 03:07


Tgt Ion: 166 Resp: 498
Ion Ratio Lower Upper
166 100
165 90.2 79.9 119.9
167 28.4 14.2 21.4#

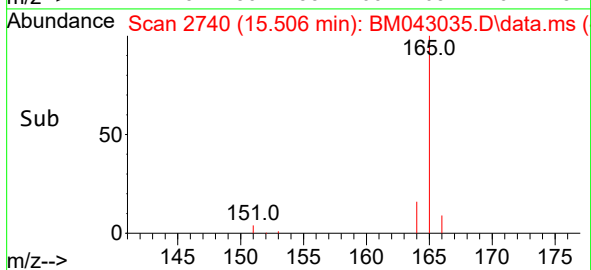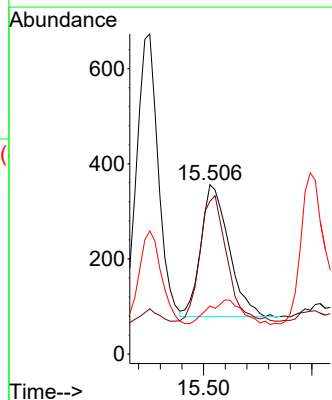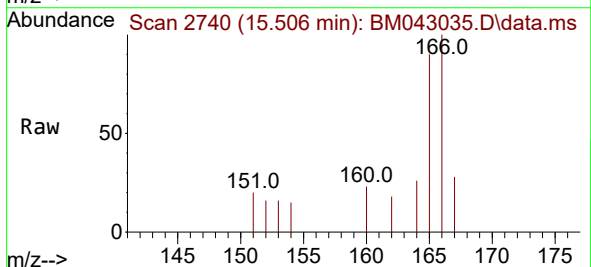

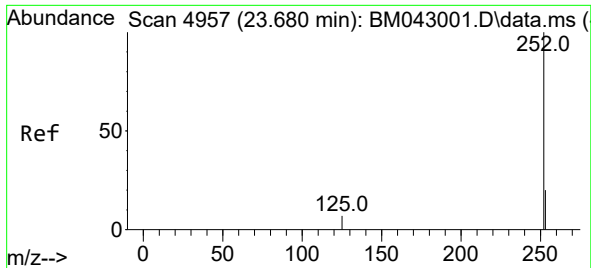

#26
 Benzo(a)pyrene
 Concen: 0.061 ng/ul
 RT: 23.586 min Scan# 49
 Delta R.T. -0.100 min
 Lab File: BM043035.D
 Acq: 26 Nov 2023 03:07

Instrument :
 BNA_M
 ClientSampleId :
 DCKC6

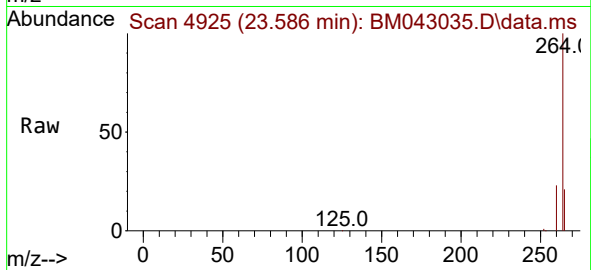

Tgt Ion:252 Resp: 1415
 Ion Ratio Lower Upper
 252 100
 253 58.8 36.6 55.0#
 125 35.8 16.2 24.4#

