




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112423\
Data File : BM042975.D
Acq On : 24 Nov 2023 12:26
Operator : MA/JU
Sample : SST0.273
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SSTD0.2023

Manual IntegrationsAPPROVED

Quant Time: Nov 25 00:07:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 24 15:22:31 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2023
Supervised By :mohammad ahmed 11/28/2023

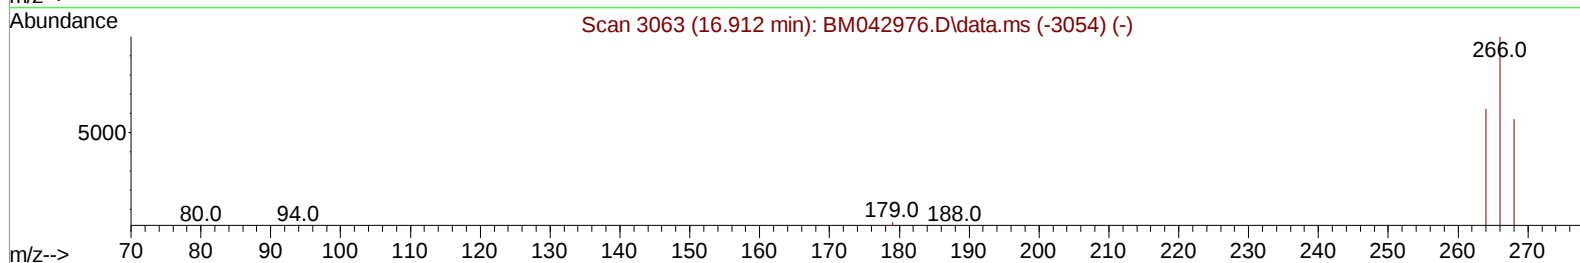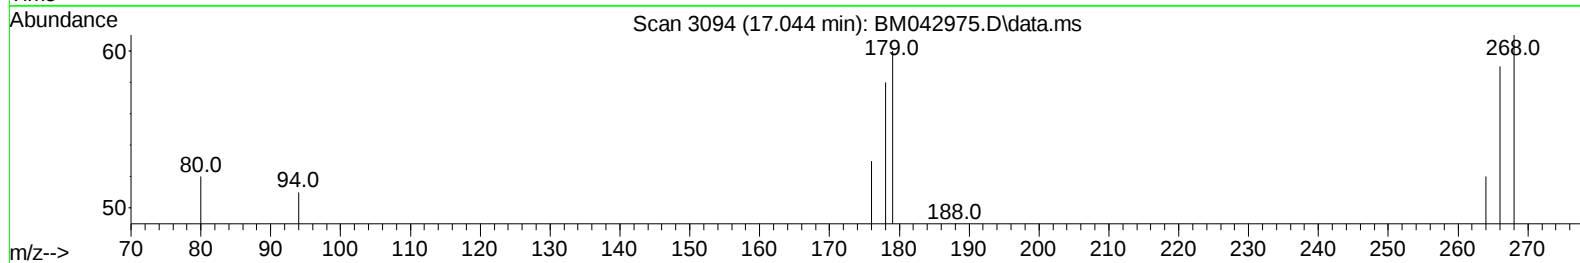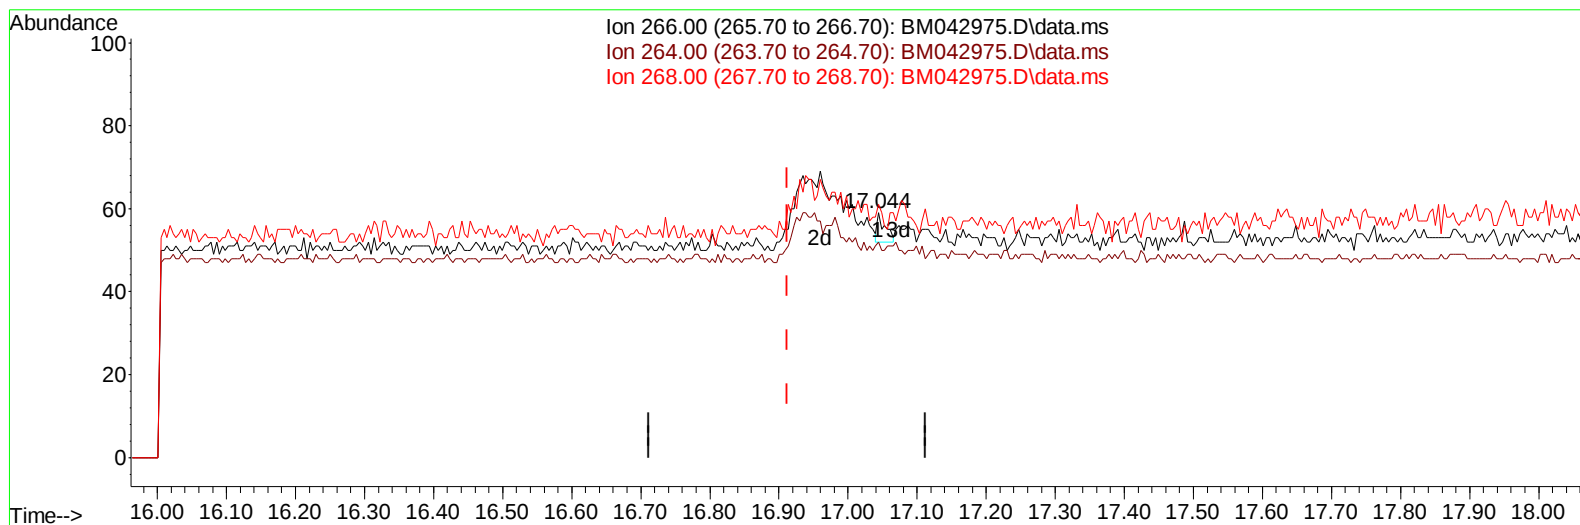

TIC: BM042975.D\data.ms

(14) Pentachloropheno1

17.044min (+ 0.132) 0.01 ng/u1

response	5	
Ion	Exp%	Act%
266.00	100.00	100.00
264.00	61.00	60.00
268.00	64.70	60.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112423\
 Data File : BM042975.D
 Acq On : 24 Nov 2023 12:26
 Operator : MA/JU
 Sample : SSTD0.273
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD0.2023

Manual IntegrationsAPPROVED

Quant Time: Nov 24 14:34:56 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 24 14:31:08 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2023
 Supervised By :mohammad ahmed 11/28/2023

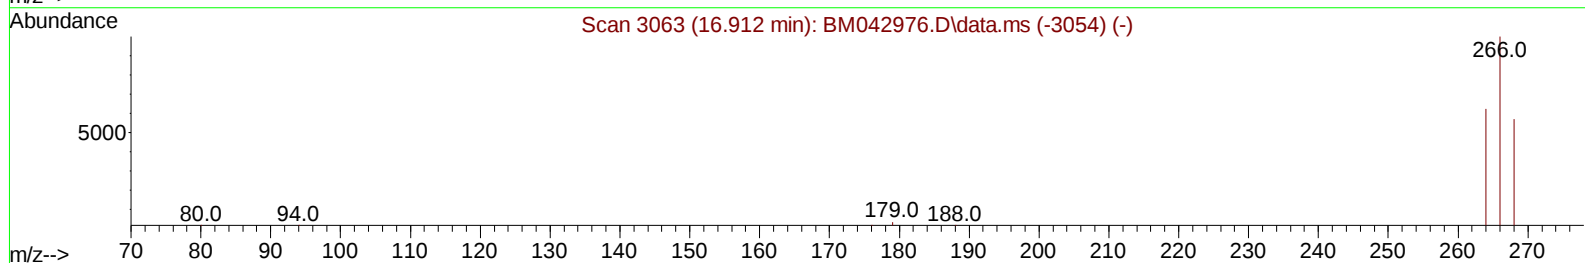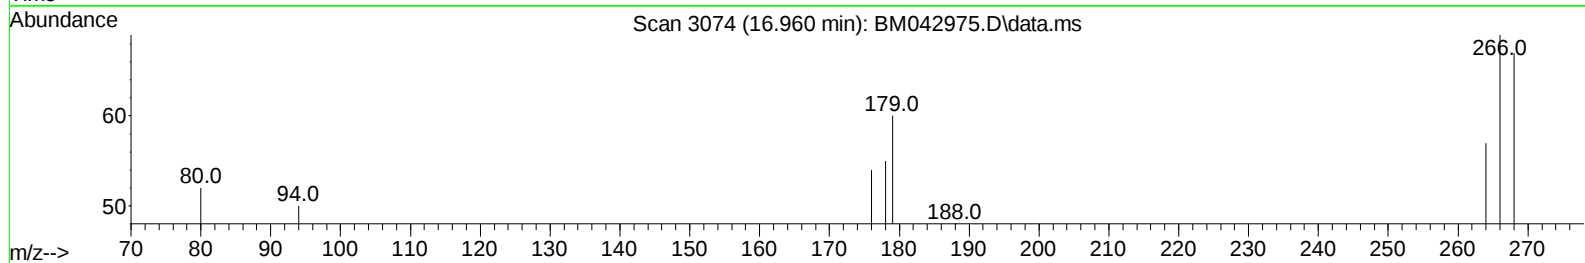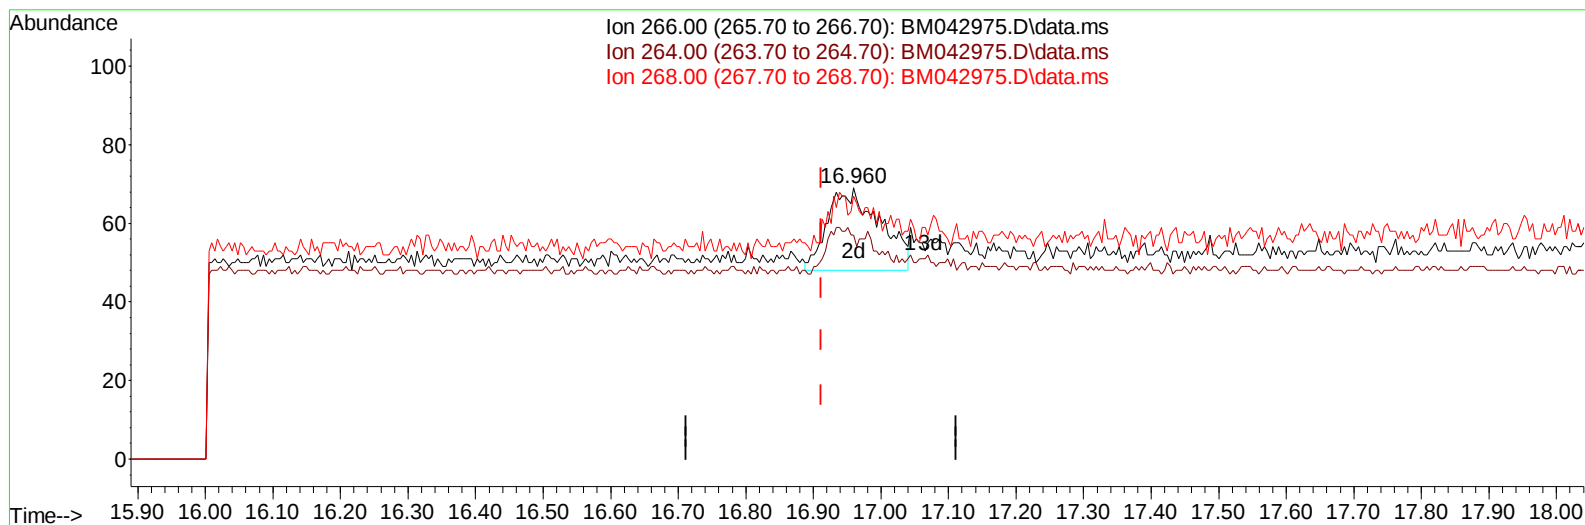

TIC: BM042975.D\data.ms

(14) Pentachlorophenol

16.960min (+ 0.048) 0.11 ng/ul m

response 112

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	61.00	2.68#
268.00	64.70	2.68#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112423\
 Data File : BM042975.D
 Acq On : 24 Nov 2023 12:26
 Operator : MA/JU
 Sample : SST00.273
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SST00.2023

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/27/2023
 Supervised By :mohammad ahmed 11/28/2023

Quant Time: Nov 24 14:34:56 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 24 14:31:08 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.918	152		494	0.400	ng/ul	0.04
4) Naphthalene-d8	10.684	136		1782	0.400	ng/ul	# 0.03
9) Acenaphthene-d10	14.479	164		1103	0.400	ng/ul	0.01
13) Phenanthrene-d10	17.255	188		2123	0.400	ng/ul	# 0.02
17) Chrysene-d12	21.432	240		1385	0.400	ng/ul	# 0.00
23) Perylene-d12	23.785	264		1885	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.172	96		200	0.266	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.295	152		436	0.191	ng/ul	0.05
18) Fluoranthene-d10	19.276	212		966	0.211	ng/ul	0.02
Target Compounds				Qvalue			
2) 1,4-Dioxane	3.202	88		233	0.277	ng/ul#	91
5) Naphthalene	10.733	128		964	0.178	ng/ul#	67
7) 2-Methylnaphthalene	12.372	142		492	0.153	ng/ul	93
8) 1-Methylnaphthalene	12.548	142		622	0.183	ng/ul	97
10) Acenaphthylene	14.215	152		1077	0.154	ng/ul#	83
11) Acenaphthene	14.544	153		825	0.166	ng/ul	97
12) Fluorene	15.566	166		814	0.152	ng/ul#	95
14) Pentachlorophenol	16.960	266		112m	0.106	ng/ul	
15) Phenanthrene	17.302	178		1191	0.166	ng/ul#	81
16) Anthracene	17.416	178		1129	0.154	ng/ul#	78
19) Fluoranthene	19.309	202		1499	0.176	ng/ul#	82
20) Pyrene	19.671	202		1641	0.179	ng/ul#	89
21) Benzo(a)anthracene	21.426	228		798	0.131	ng/ul#	85
22) Chrysene	21.467	228		1758	0.210	ng/ul	95
24) Benzo(b)fluoranthene	23.060	252		1271	0.171	ng/ul	75
25) Benzo(k)fluoranthene	23.115	252		1689	0.182	ng/ul#	73
26) Benzo(a)pyrene	23.697	252		1317	0.174	ng/ul#	68
27) Indeno(1,2,3-cd)pyrene	26.279	276		1810	0.177	ng/ul#	100
28) Dibenzo(a,h)anthracene	26.299	278		1411	0.185	ng/ul#	67
29) Benzo(g,h,i)perylene	27.030	276		1822	0.205	ng/ul#	83

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112423\
Data File : BM042975.D
Acq On : 24 Nov 2023 12:26
Operator : MA/JU
Sample : SST00.273
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SSTD0.2023

Manual IntegrationsAPPROVED

Quant Time: Nov 24 14:34:56 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 24 14:31:08 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2023
Supervised By :mohammad ahmed 11/28/2023

