




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112423\
Data File : BM042995.D
Acq On : 25 Nov 2023 01:10
Operator : MA/JU
Sample : 05268-12DL 5X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKD4DL

Manual IntegrationsAPPROVED

Quant Time: Nov 25 02:05:04 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 24 15:22:31 2023
Response via : Initial Calibration

Reviewed By :Yogesh
Patel 11/27/2023
Supervised By :mohammad
anmed 11/28/2023

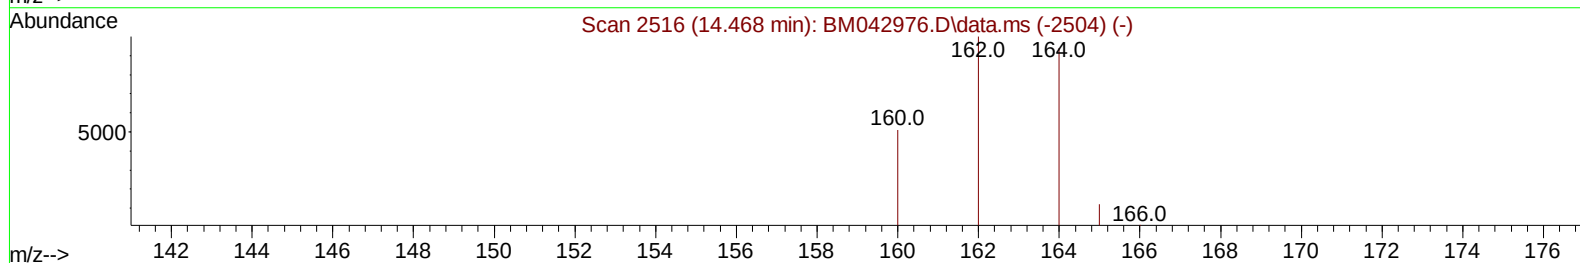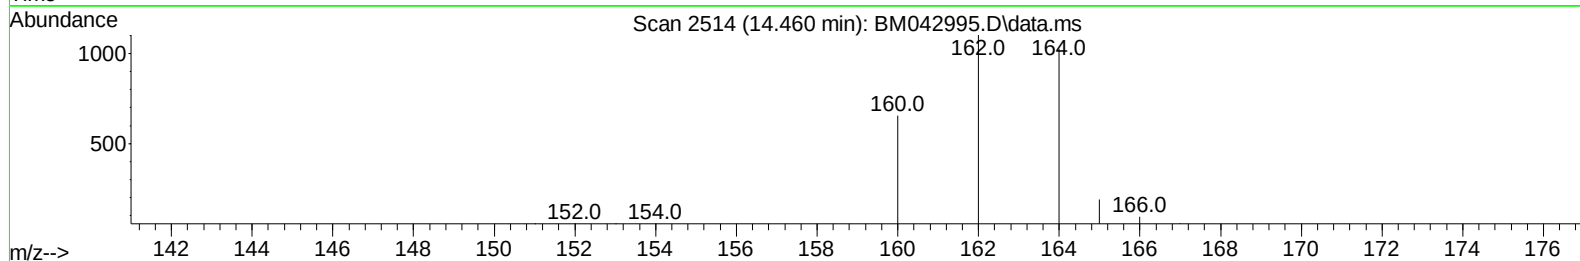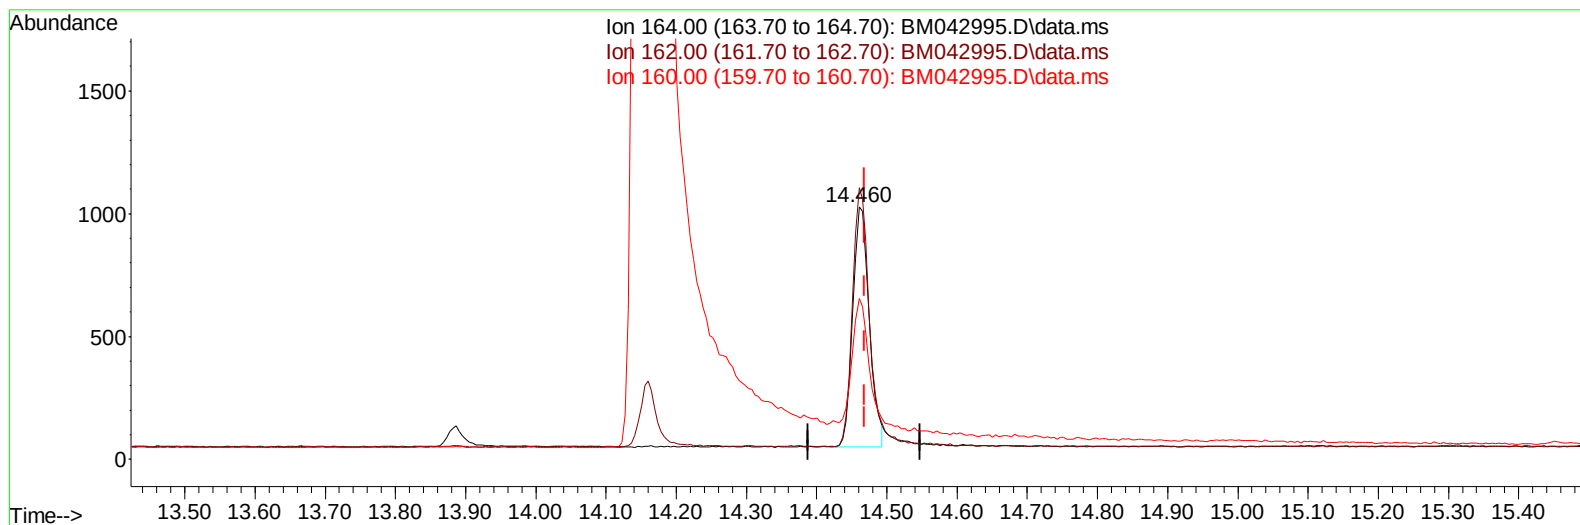

TIC: BM042995.D\data.ms

(9) Acenaphthene-d10 (I)

14.460min (-0.008) 0.40 ng/u1

response 1575

Ion	Exp%	Act%
164.00	100.00	100.00
162.00	106.50	107.59
160.00	57.20	63.88
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112423\
 Data File : BM042995.D
 Acq On : 25 Nov 2023 01:10
 Operator : MA/JU
 Sample : 05268-12DL 5X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCKD4DL

Manual IntegrationsAPPROVED

Quant Time: Nov 25 02:05:04 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 24 15:22:31 2023
 Response via : Initial Calibration

Reviewed By :Yogesh
 Patel 11/27/2023
 Supervised By :mohammad
 ahmed 11/28/2023

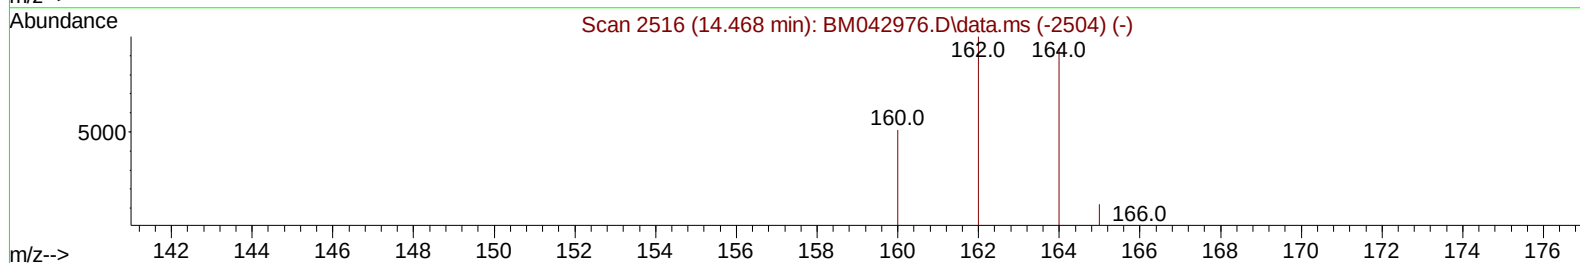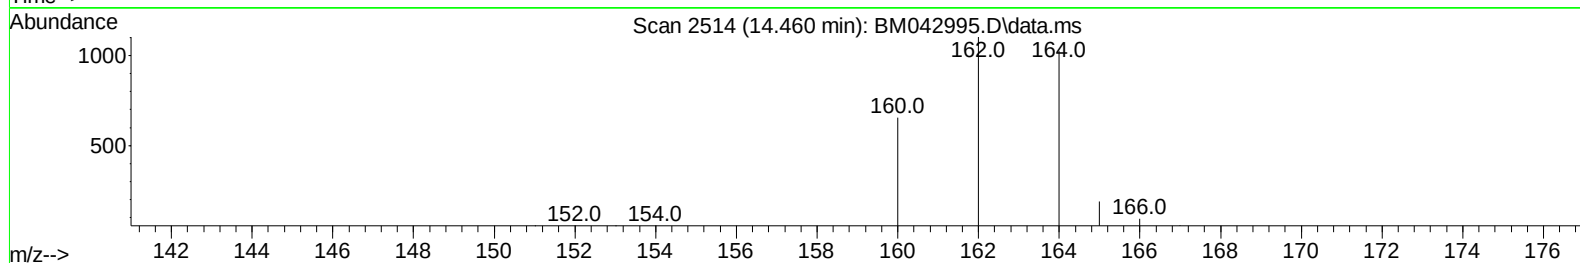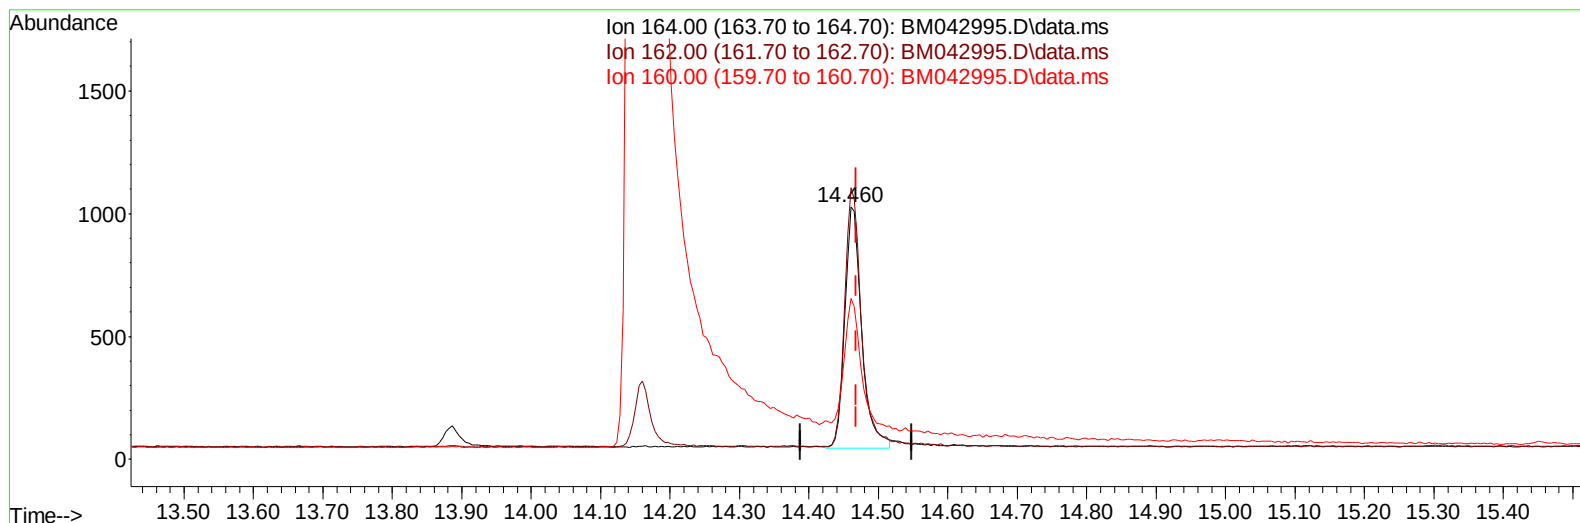

TIC: BM042995.D\data.ms

(9) Acenaphthene-d10 (I)

14.460min (-0.008) 0.40 ng/ul m

response 1663

Ion	Exp%	Act%
164.00	100.00	100.00
162.00	106.50	107.59
160.00	57.20	63.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112423\
 Data File : BM042995.D
 Acq On : 25 Nov 2023 01:10
 Operator : MA/JU
 Sample : 05268-12DL 5X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCKD4DL

Manual IntegrationsAPPROVED

Reviewed By :Yogesh
 Patel 11/27/2023
 Supervised By :mohammad
 ahmed 11/28/2023

Quant Time: Nov 25 02:05:04 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 24 15:22:31 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.830	152		847	0.400	ng/ul	#-0.05
4) Naphthalene-d8	10.623	136		2598	0.400	ng/ul	#-0.03
9) Acenaphthene-d10	14.460	164		1663m	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.217	188		3397	0.400	ng/ul	-0.02
17) Chrysene-d12	21.420	240		1837	0.400	ng/ul	0.00
23) Perylene-d12	23.761	264		3562	0.400	ng/ul	#-0.02
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.168	96		547	0.421	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.278	152		234	0.067	ng/ul	0.03
18) Fluoranthene-d10	19.248	212		666	0.100	ng/ul	-0.01
Target Compounds							Qvalue
14) Pentachlorophenol	16.871	266		1633	1.776	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112423\
Data File : BM042995.D
Acq On : 25 Nov 2023 01:10
Operator : MA/JU
Sample : 05268-12DL 5X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKD4DL

Manual IntegrationsAPPROVED

Quant Time: Nov 25 02:05:04 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 24 15:22:31 2023
Response via : Initial Calibration

Reviewed By :Yogesh
Patel 11/27/2023
Supervised By :mohammad
ahmed 11/28/2023

