




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112423\
 Data File : BM043030.D
 Acq On : 26 Nov 2023 00:41
 Operator : MA/JU
 Sample : 05264-14
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCKS5

Manual IntegrationsAPPROVED

Quant Time: Nov 27 02:45:30 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 27 02:36:19 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/28/2023
 Supervised By :mohammad ahmed 11/28/2023

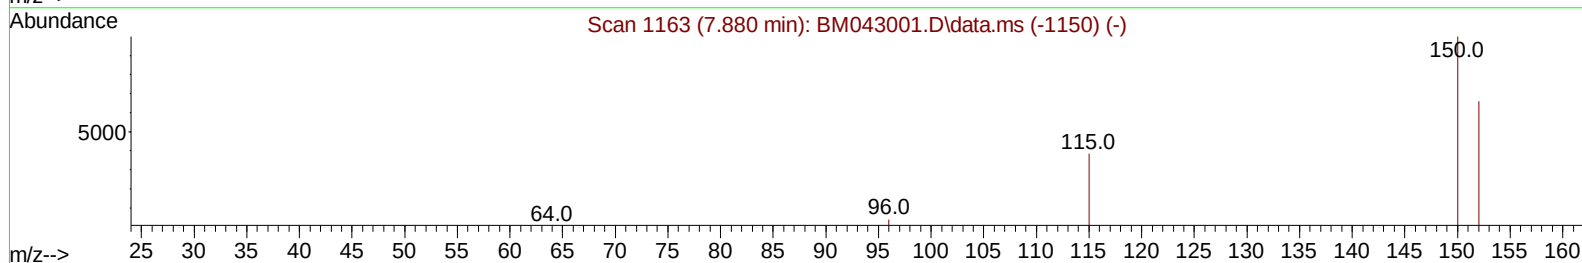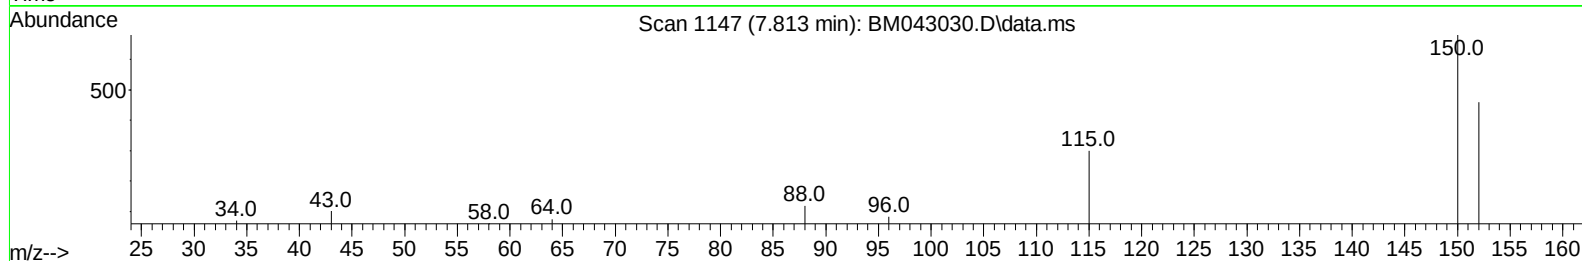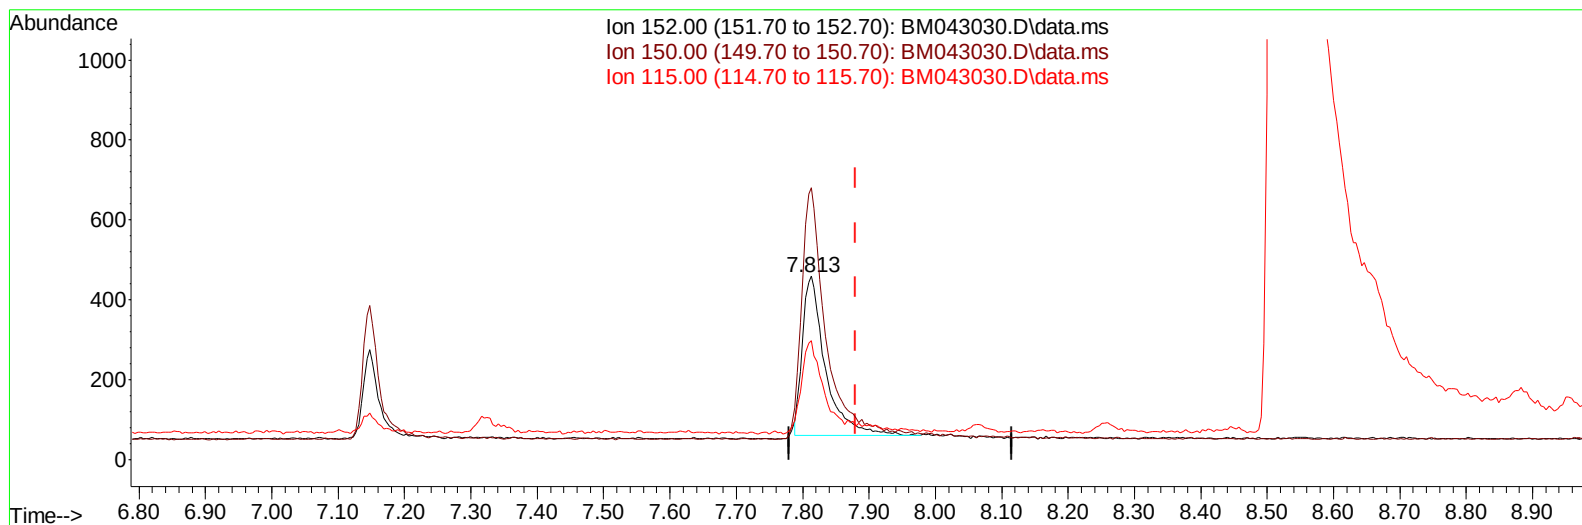

TIC: BM043030.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.813min (-0.067) 0.40 ng/ul

response 966

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	124.60	148.15
115.00	89.60	64.92#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112423\
 Data File : BM043030.D
 Acq On : 26 Nov 2023 00:41
 Operator : MA/JU
 Sample : 05264-14
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCKS5

Manual IntegrationsAPPROVED

Quant Time: Nov 27 02:45:30 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 27 02:36:19 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/28/2023
 Supervised By :mohammad ahmed 11/28/2023

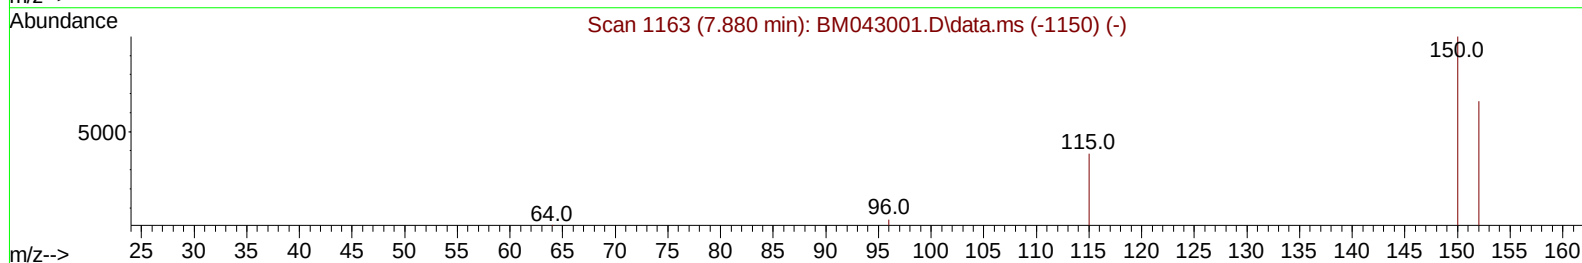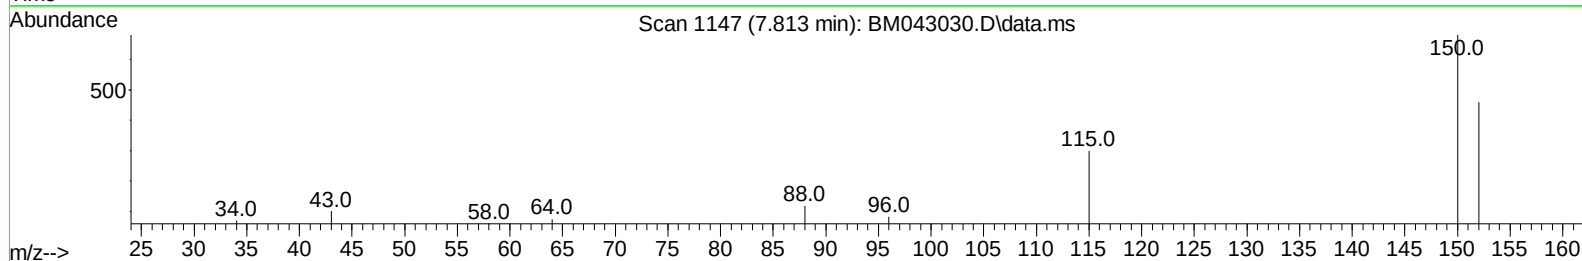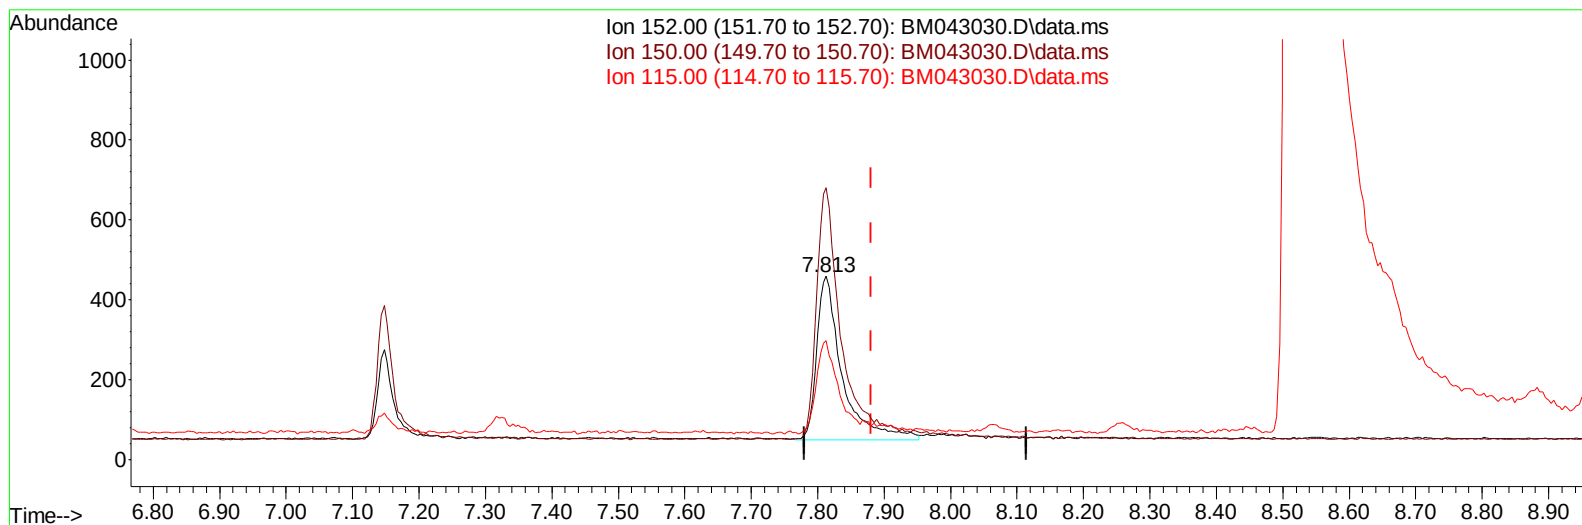

TIC: BM043030.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.813min (-0.067) 0.40 ng/ul m

response 1095

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	124.60	148.15
115.00	89.60	64.92#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112423\
 Data File : BM043030.D
 Acq On : 26 Nov 2023 00:41
 Operator : MA/JU
 Sample : 05264-14
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCKS5

Manual IntegrationsAPPROVED

Quant Time: Nov 27 02:45:30 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 27 02:36:19 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/28/2023
 Supervised By :mohammad ahmed 11/28/2023

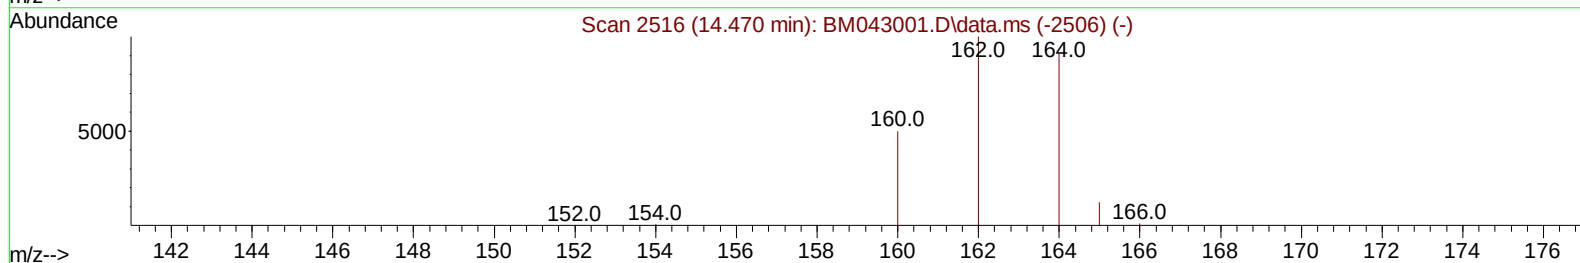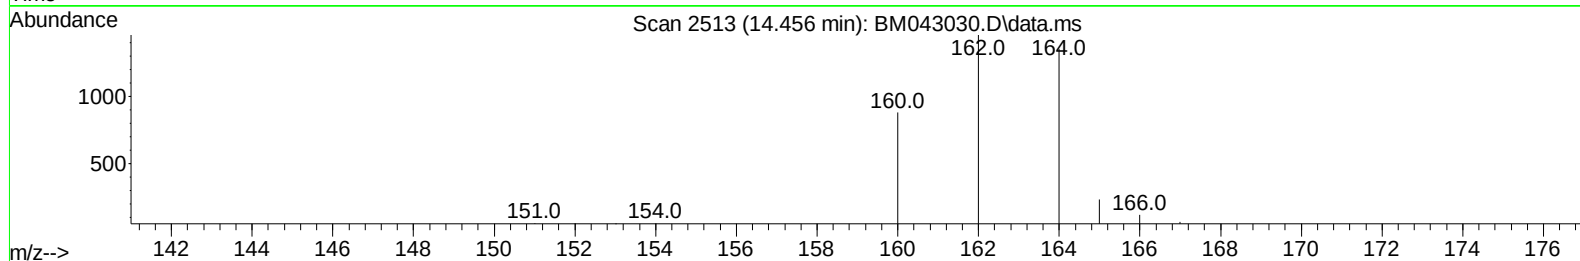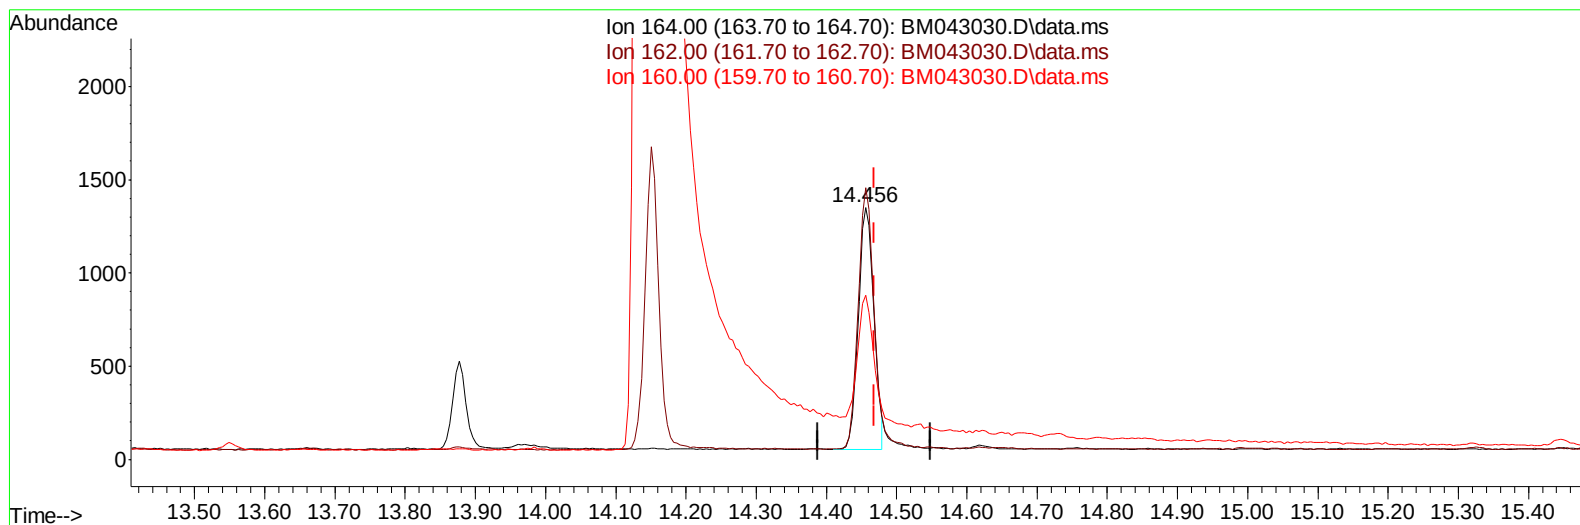

TIC: BM043030.D\data.ms

(9) Acenaphthene-d10 (I)

14.456min (-0.013) 0.40 ng/u1

response 1987

Ion	Exp%	Act%
164.00	100.00	100.00
162.00	106.50	107.69
160.00	57.20	65.09
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112423\
 Data File : BM043030.D
 Acq On : 26 Nov 2023 00:41
 Operator : MA/JU
 Sample : 05264-14
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCKS5

Manual IntegrationsAPPROVED

Quant Time: Nov 27 02:45:30 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 27 02:36:19 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/28/2023
 Supervised By :mohammad ahmed 11/28/2023

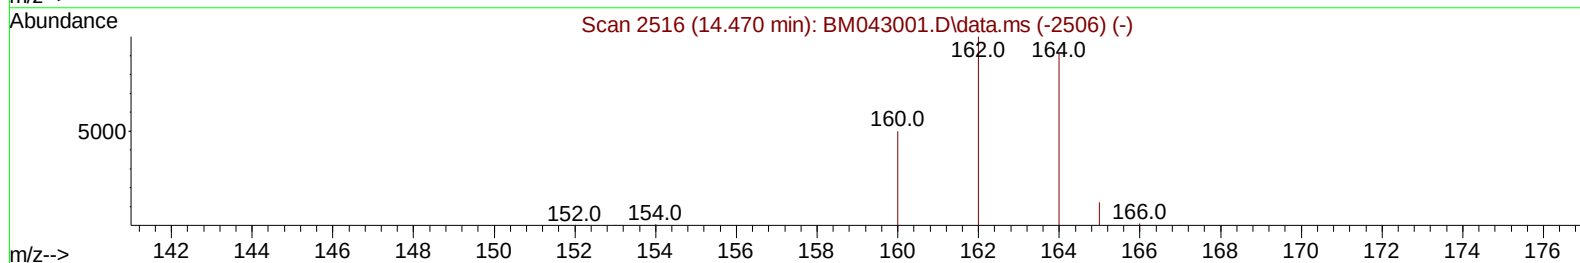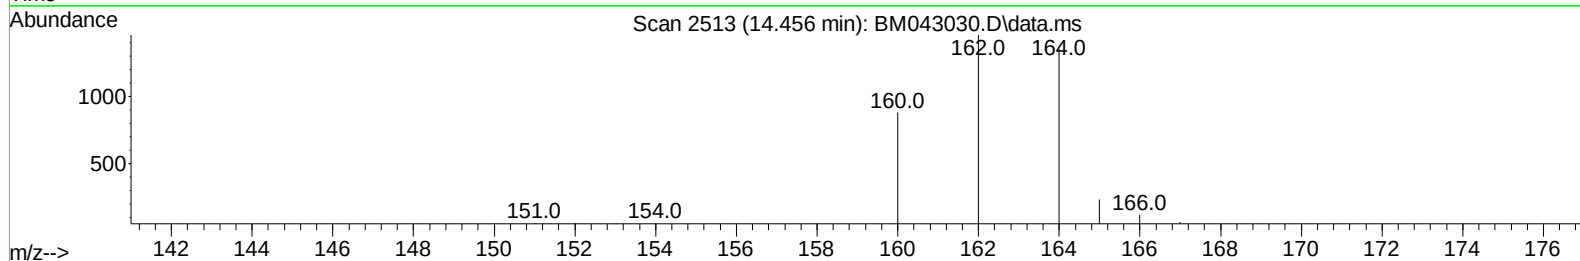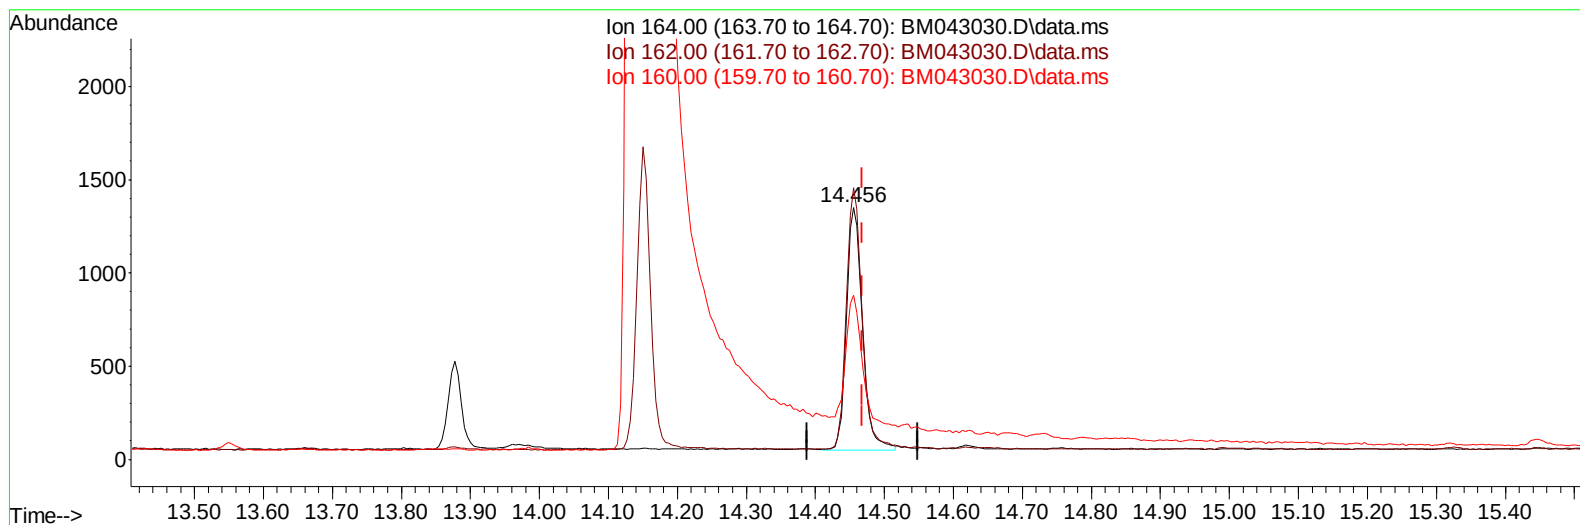

TIC: BM043030.D\data.ms

(9) Acenaphthene-d10 (I)

14.456min (-0.013) 0.40 ng/ul m

response 2098

Ion	Exp%	Act%
164.00	100.00	100.00
162.00	106.50	107.69
160.00	57.20	65.09
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112423\
 Data File : BM043030.D
 Acq On : 26 Nov 2023 00:41
 Operator : MA/JU
 Sample : 05264-14
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCKS5

Manual IntegrationsAPPROVED

Quant Time: Nov 27 02:45:30 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 27 02:36:19 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/28/2023
 Supervised By :mohammad ahmed 11/28/2023

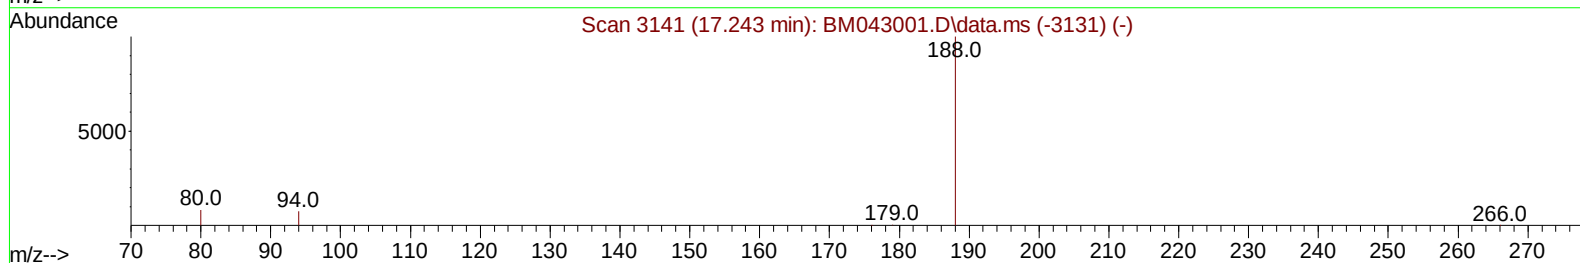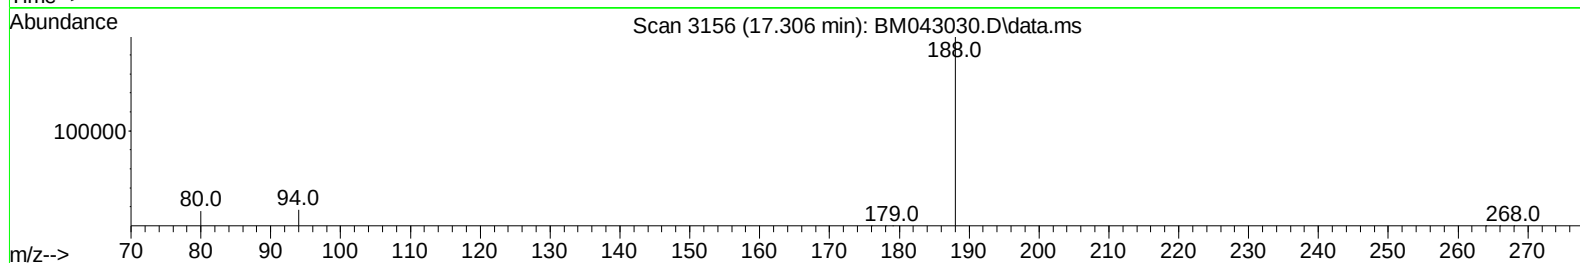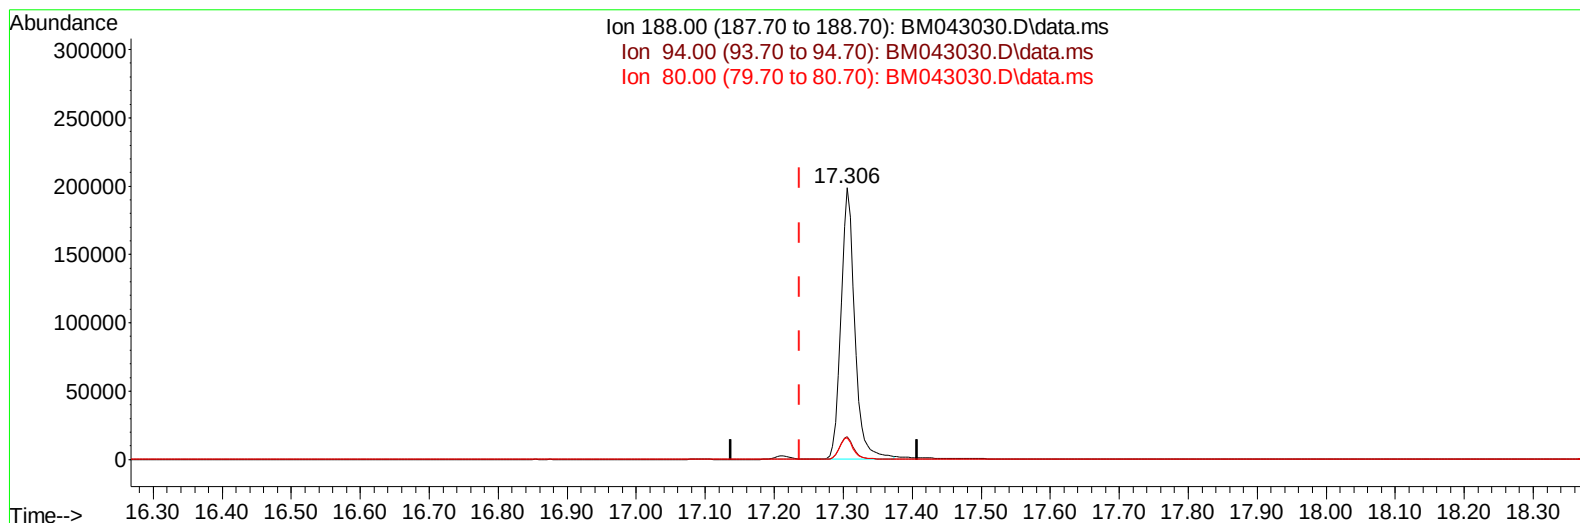

TIC: BM043030.D\data.ms

(13) Phenanthrene-d10 (I)

17.306min (+ 0.069) 0.40 ng/ul

response 276077

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.40	8.39#
80.00	12.70	7.83#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112423\
Data File : BM043030.D
Acq On : 26 Nov 2023 00:41
Operator : MA/JU
Sample : 05264-14
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKS5

Manual IntegrationsAPPROVED

Quant Time: Nov 27 02:45:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 27 02:36:19 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/28/2023
Supervised By :mohammad ahmed 11/28/2023

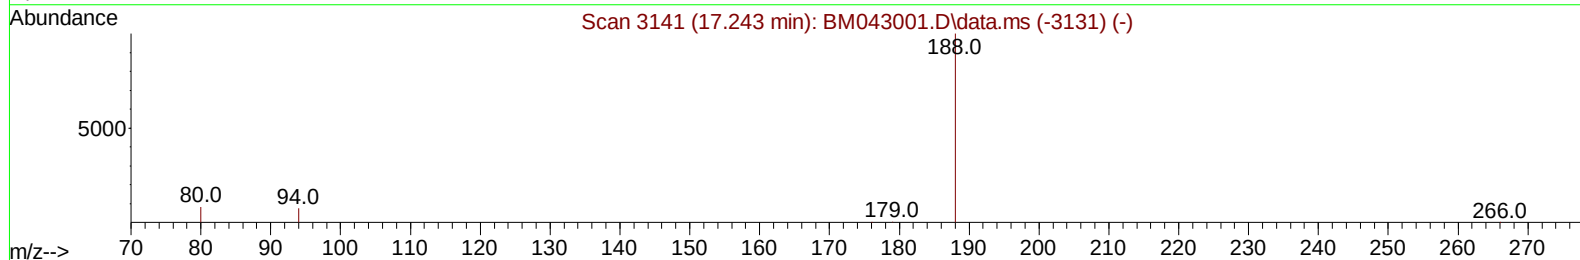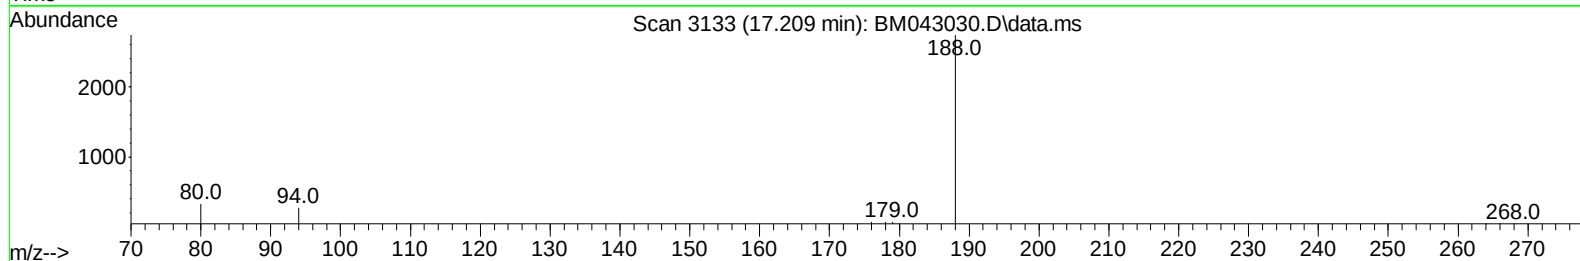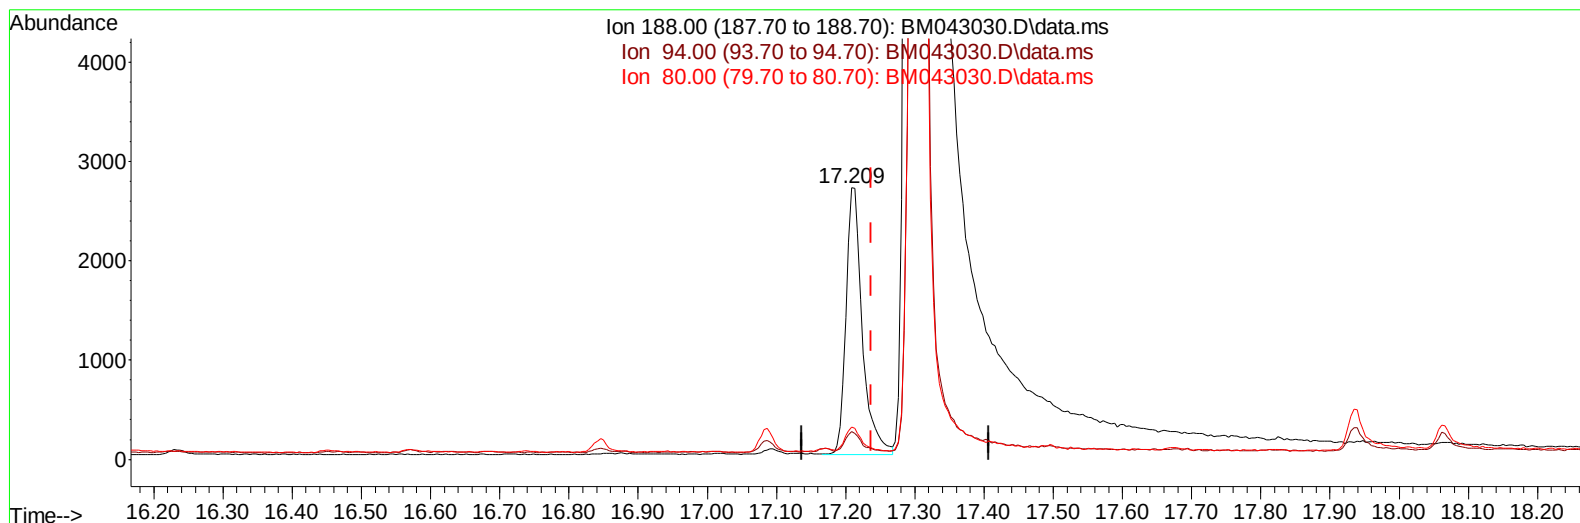

TIC: BM043030.D\data.ms

(13) Phenanthrene-d10 (I)

17.209min (-0.028) 0.40 ng/ul m

response 4378

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.40	10.24
80.00	12.70	11.99
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112423\
 Data File : BM043030.D
 Acq On : 26 Nov 2023 00:41
 Operator : MA/JU
 Sample : 05264-14
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCKS5

Manual IntegrationsAPPROVED

Quant Time: Nov 27 02:45:30 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 27 02:36:19 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/28/2023
 Supervised By :mohammad ahmed 11/28/2023

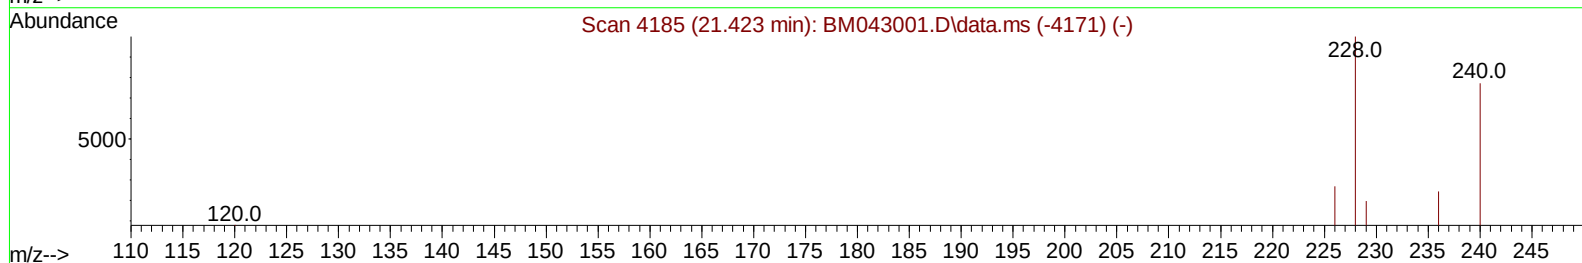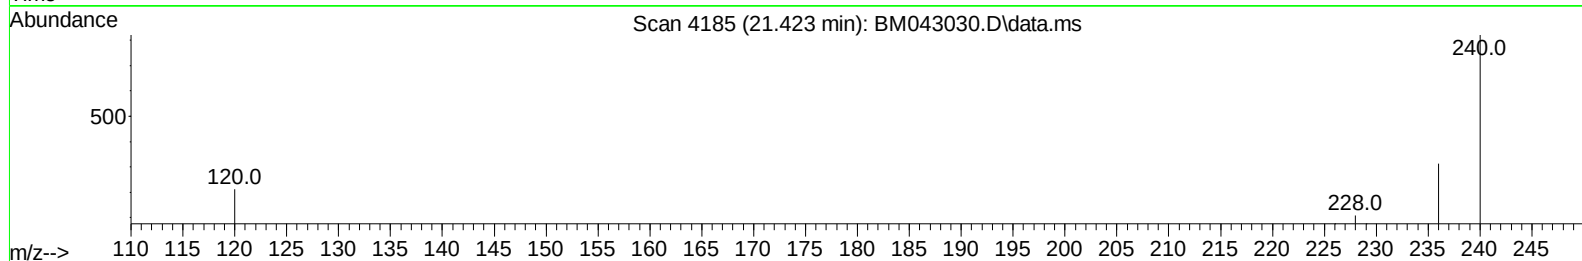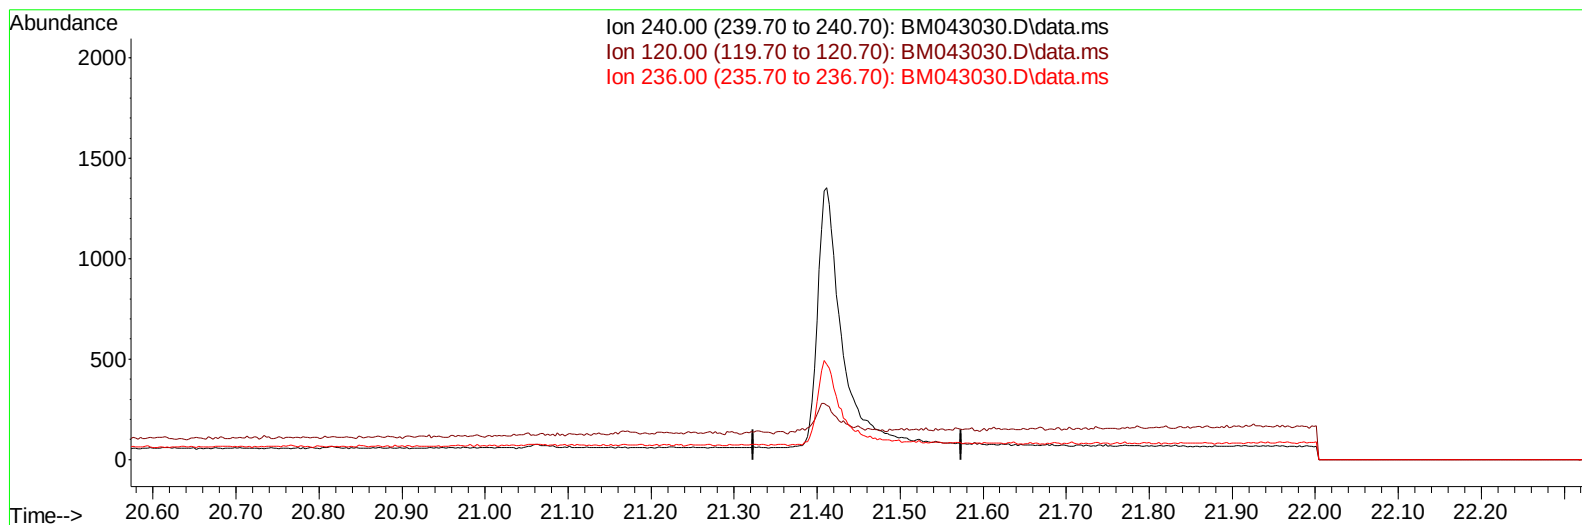

TIC: BM043030.D\data.ms

(17) Chrysene-d12

21.424min (-21.424) 0.00 ng/ul

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	22.80	0.00#
236.00	38.50	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112423\
 Data File : BM043030.D
 Acq On : 26 Nov 2023 00:41
 Operator : MA/JU
 Sample : 05264-14
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCKS5

Manual IntegrationsAPPROVED

Quant Time: Nov 27 02:45:30 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 27 02:36:19 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/28/2023
 Supervised By :mohammad ahmed 11/28/2023

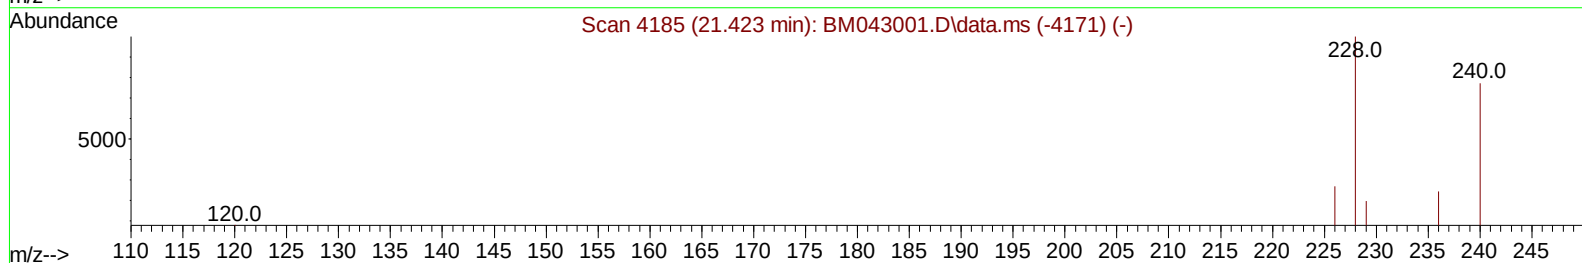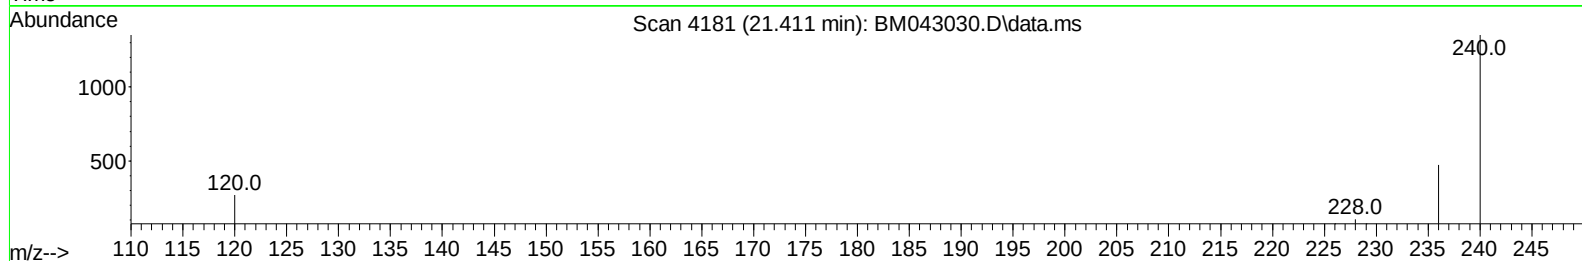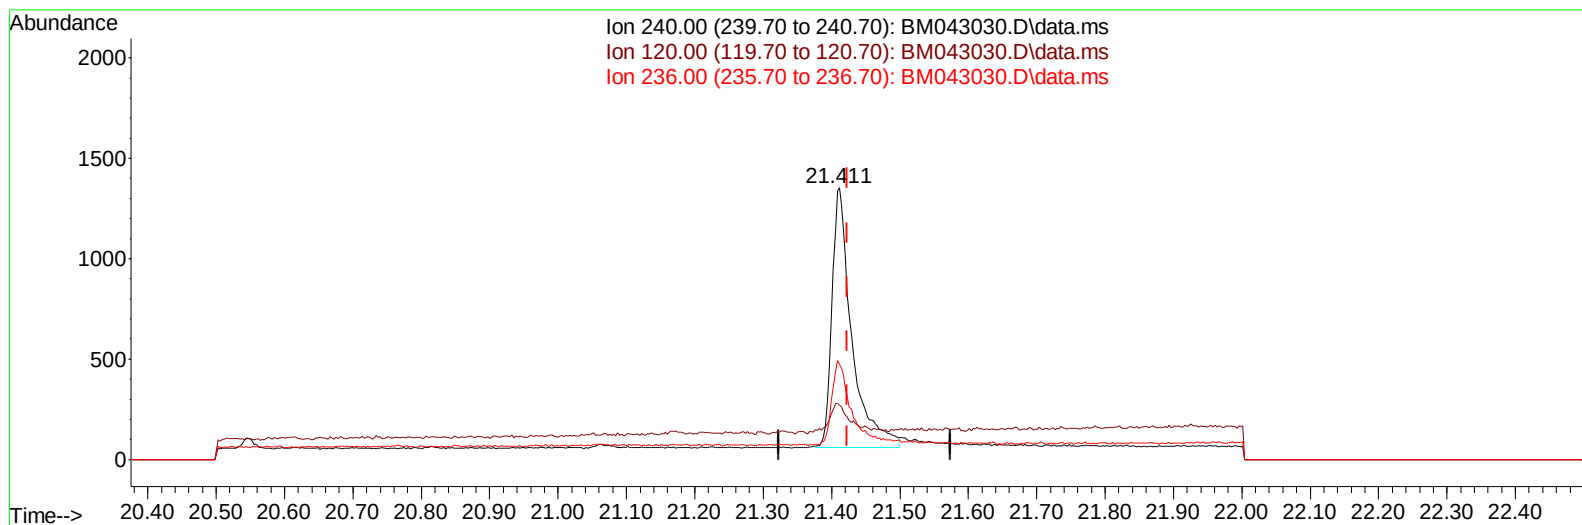

TIC: BM043030.D\data.ms

(17) Chrysene-d12

21.411min (-0.012) 0.40 ng/ul m

response 2598

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	22.80	20.04
236.00	38.50	34.99
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112423\
 Data File : BM043030.D
 Acq On : 26 Nov 2023 00:41
 Operator : MA/JU
 Sample : 05264-14
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCKS5

Manual IntegrationsAPPROVED

Quant Time: Nov 27 23:06:08 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 27 02:36:19 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/28/2023
 Supervised By :mohammad ahmed 11/28/2023

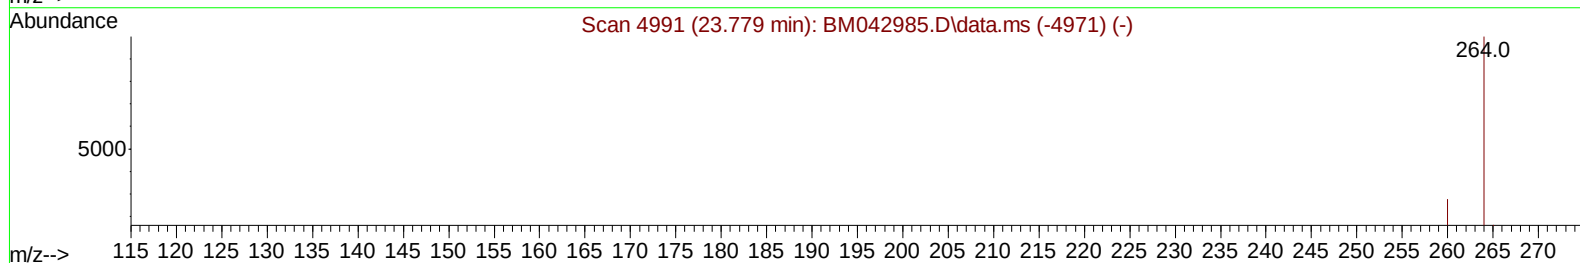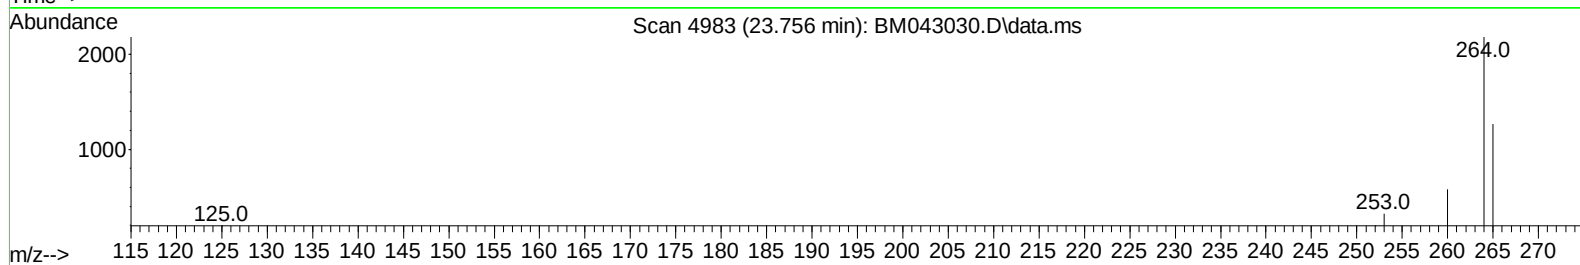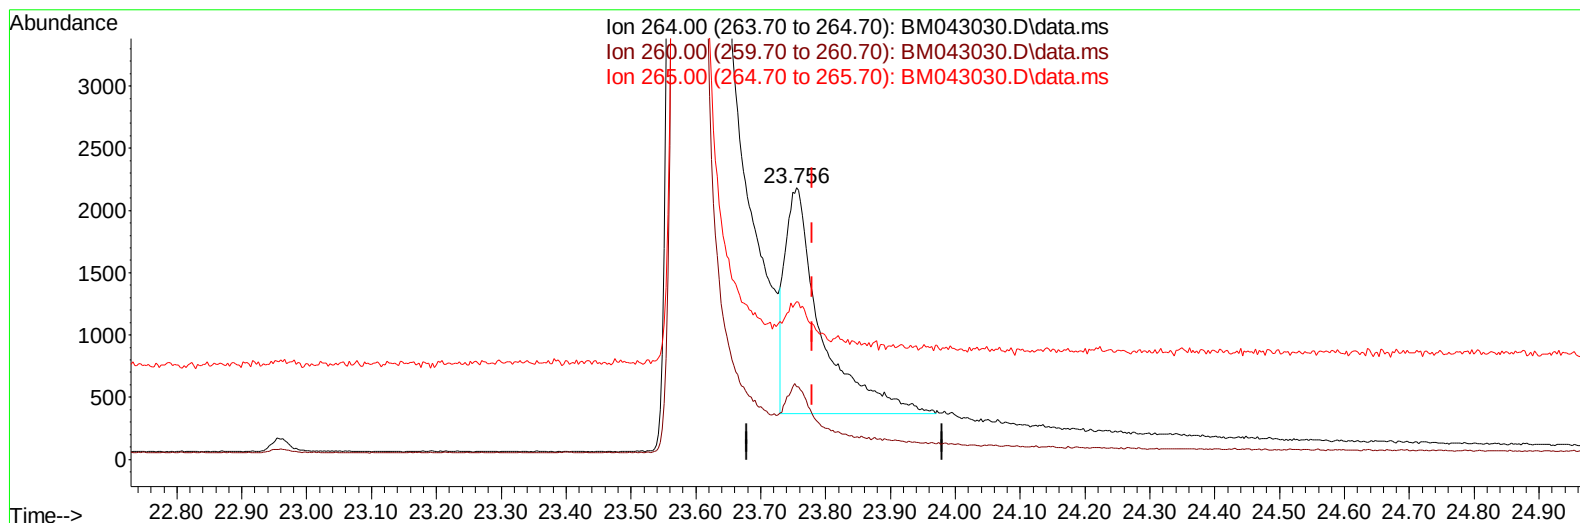

TIC: BM043030.D\data.ms

(23) Perylene-d12 (I)

23.756min (-0.024) 0.40 ng/u1

response 6989

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	33.90	26.73#
265.00	120.30	58.09#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112423\
 Data File : BM043030.D
 Acq On : 26 Nov 2023 00:41
 Operator : MA/JU
 Sample : 05264-14
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCKS5

Manual IntegrationsAPPROVED

Quant Time: Nov 27 02:45:30 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 27 02:36:19 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/28/2023
 Supervised By :mohammad ahmed 11/28/2023

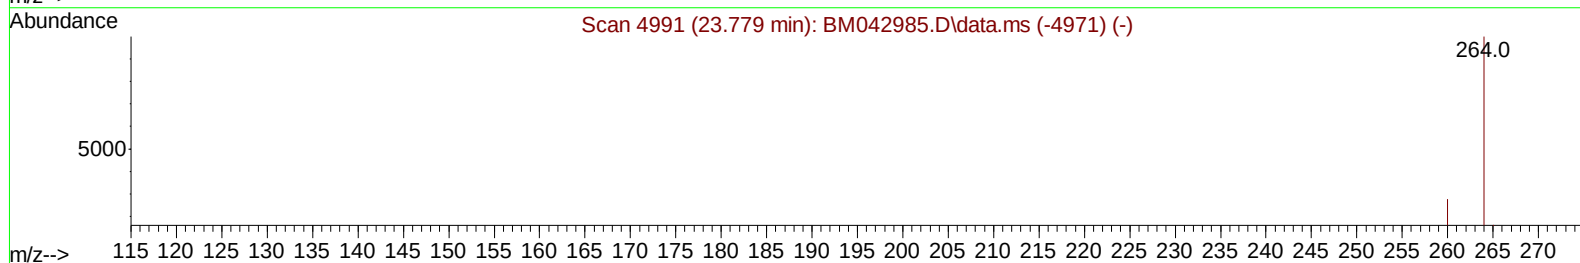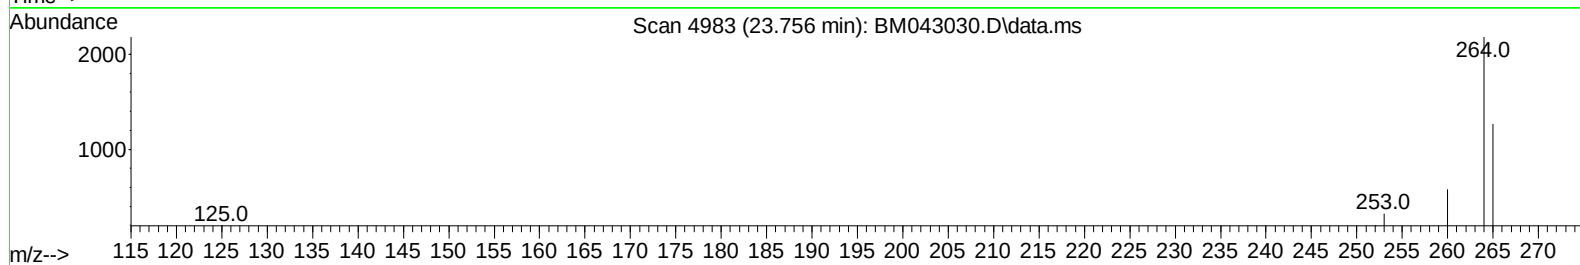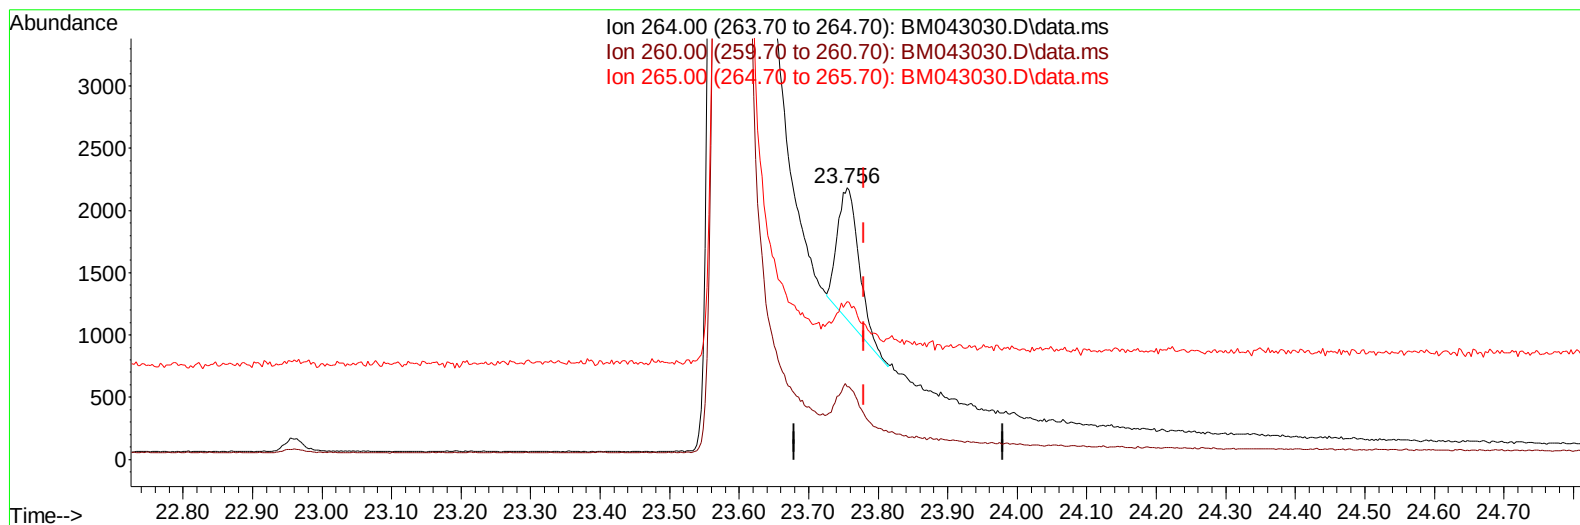

TIC: BM043030.D\data.ms

(23) Perylene-d12 (I)

23.756min (-0.024) 0.40 ng/ul m

response 2237

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	33.90	26.73#
265.00	120.30	58.09#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112423\
 Data File : BM043030.D
 Acq On : 26 Nov 2023 00:41
 Operator : MA/JU
 Sample : 05264-14
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCKS5

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/28/2023
 Supervised By :mohammad ahmed 11/28/2023

Quant Time: Nov 27 02:45:30 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 27 02:36:19 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.813	152	1095m	0.400	ng/ul	-0.07
4) Naphthalene-d8	10.612	136	3279	0.400	ng/ul	#-0.04
9) Acenaphthene-d10	14.456	164	2098m	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.209	188	4378m	0.400	ng/ul	-0.03
17) Chrysene-d12	21.411	240	2598m	0.400	ng/ul	-0.01
23) Perylene-d12	23.756	264	2237m	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.159	96	4449	2.648	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.229	152	1168	0.266	ng/ul	-0.02
18) Fluoranthene-d10	19.244	212	3392	0.358	ng/ul	-0.02

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112423\
Data File : BM043030.D
Acq On : 26 Nov 2023 00:41
Operator : MA/JU
Sample : 05264-14
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKS5

Manual IntegrationsAPPROVED

Quant Time: Nov 27 02:45:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 27 02:36:19 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/28/2023
Supervised By :mohammad ahmed 11/28/2023

