

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112423\
 Data File : BM043031.D
 Acq On : 26 Nov 2023 01:18
 Operator : MA/JU
 Sample : 05264-11
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCKS2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/28/2023
 Supervised By :mohammad ahmed 11/28/2023

Quant Time: Nov 27 02:45:35 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 27 02:36:19 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.809	152	1037m	0.400	ng/ul	-0.07
4) Naphthalene-d8	10.611	136	3256	0.400	ng/ul	#-0.04
9) Acenaphthene-d10	14.454	164	2123m	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.212	188	4174m	0.400	ng/ul	-0.03
17) Chrysene-d12	21.412	240	2235m	0.400	ng/ul	-0.01
23) Perylene-d12	23.756	264	2998m	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.160	96	5915	3.717	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.222	152	1612	0.370	ng/ul	-0.03
18) Fluoranthene-d10	19.242	212	3577	0.439	ng/ul	-0.02
Target Compounds						Qvalue
5) Naphthalene	10.660	128	363	0.041	ng/ul#	68

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112423\
Data File : BM043031.D
Acq On : 26 Nov 2023 01:18
Operator : MA/JU
Sample : 05264-11
Misc :
ALS Vial : 56 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
DCKS2

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/28/2023
Supervised By :mohammad ahmed 11/28/2023


Quant Time: Nov 27 02:45:35 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 27 02:36:19 2023
Response via : Initial Calibration

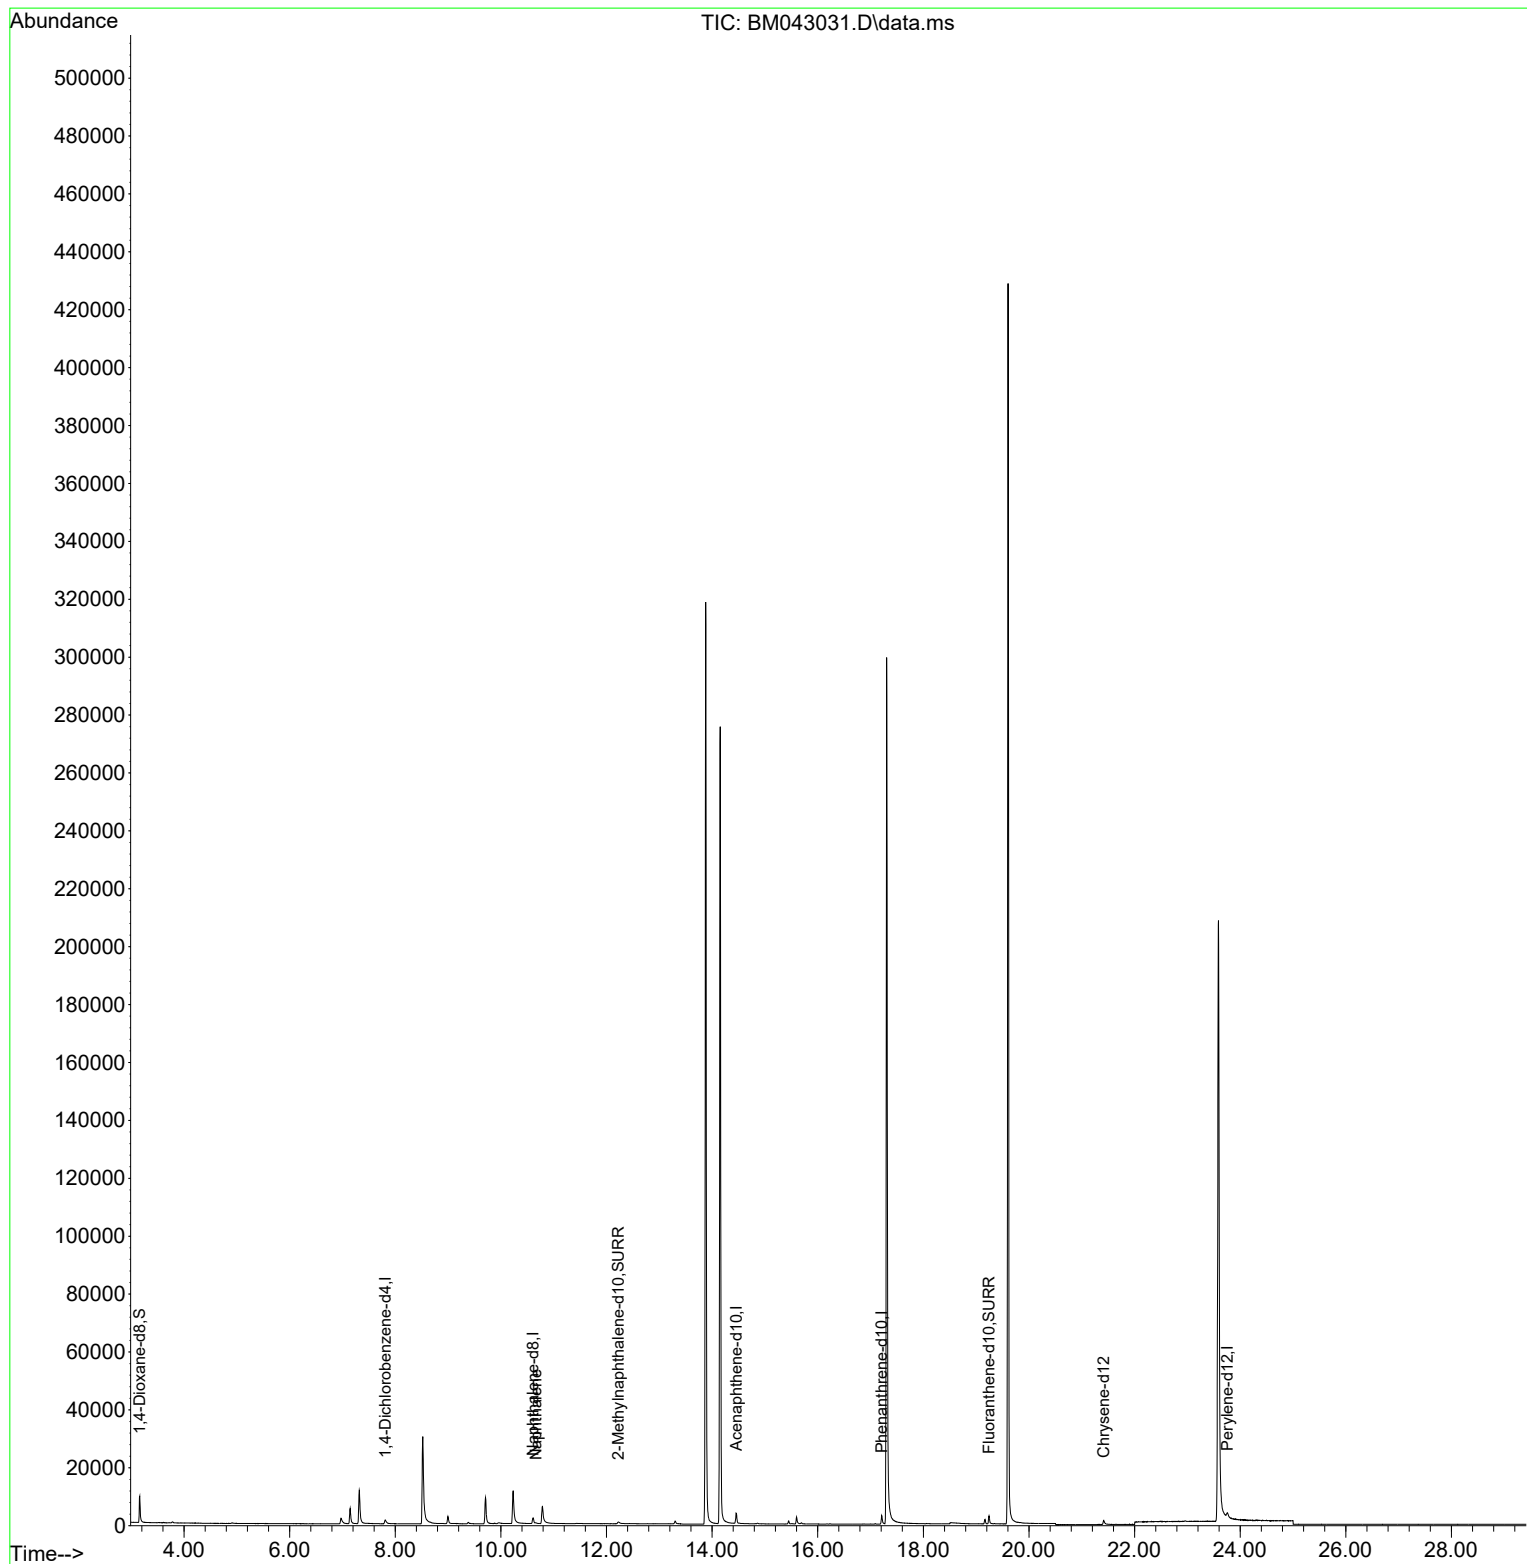

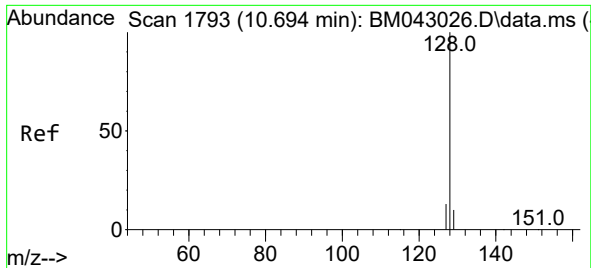

#5
Naphthalene
Concen: 0.041 ng/ul
RT: 10.660 min Scan# 1787
Delta R.T. -0.038 min
Lab File: BM043031.D
Acq: 26 Nov 2023 01:18

Instrument :
BNA_M
ClientSampleId :
DCKS2

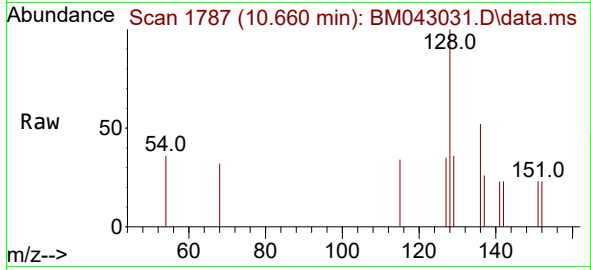

Tgt Ion:128 Resp: 360
Ion Ratio Lower Upper
128 100
129 35.7 16.0 24.0
127 34.9 16.5 24.7

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/28/2023
Supervised By :mohammad ahmed 11/28/2023

