

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112423\
 Data File : BM043034.D
 Acq On : 26 Nov 2023 03:07
 Operator : MA/JU
 Sample : 05336-07
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCKC5

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/28/2023
 Supervised By :mohammad ahmed 11/28/2023

Quant Time: Nov 27 02:45:51 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 27 02:36:19 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.813	152	1145m	0.400	ng/ul	-0.07
4) Naphthalene-d8	10.606	136	3272	0.400	ng/ul	#-0.04
9) Acenaphthene-d10	14.456	164	2147m	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.213	188	4260m	0.400	ng/ul	-0.02
17) Chrysene-d12	21.414	240	2381m	0.400	ng/ul	0.00
23) Perylene-d12	23.756	264	1993m	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.160	96	4706	2.679	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.234	152	1322	0.302	ng/ul	-0.02
18) Fluoranthene-d10	19.244	212	3530	0.407	ng/ul	-0.02
Target Compounds						Qvalue
12) Fluorene	15.506	166	498	0.058	ng/ul#	88

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112423\
Data File : BM043034.D
Acq On : 26 Nov 2023 03:07
Operator : MA/JU
Sample : 05336-07
Misc :
ALS Vial : 59 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
DCKC5

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/28/2023
Supervised By :mohammad ahmed 11/28/2023


Quant Time: Nov 27 02:45:51 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 27 02:36:19 2023
Response via : Initial Calibration

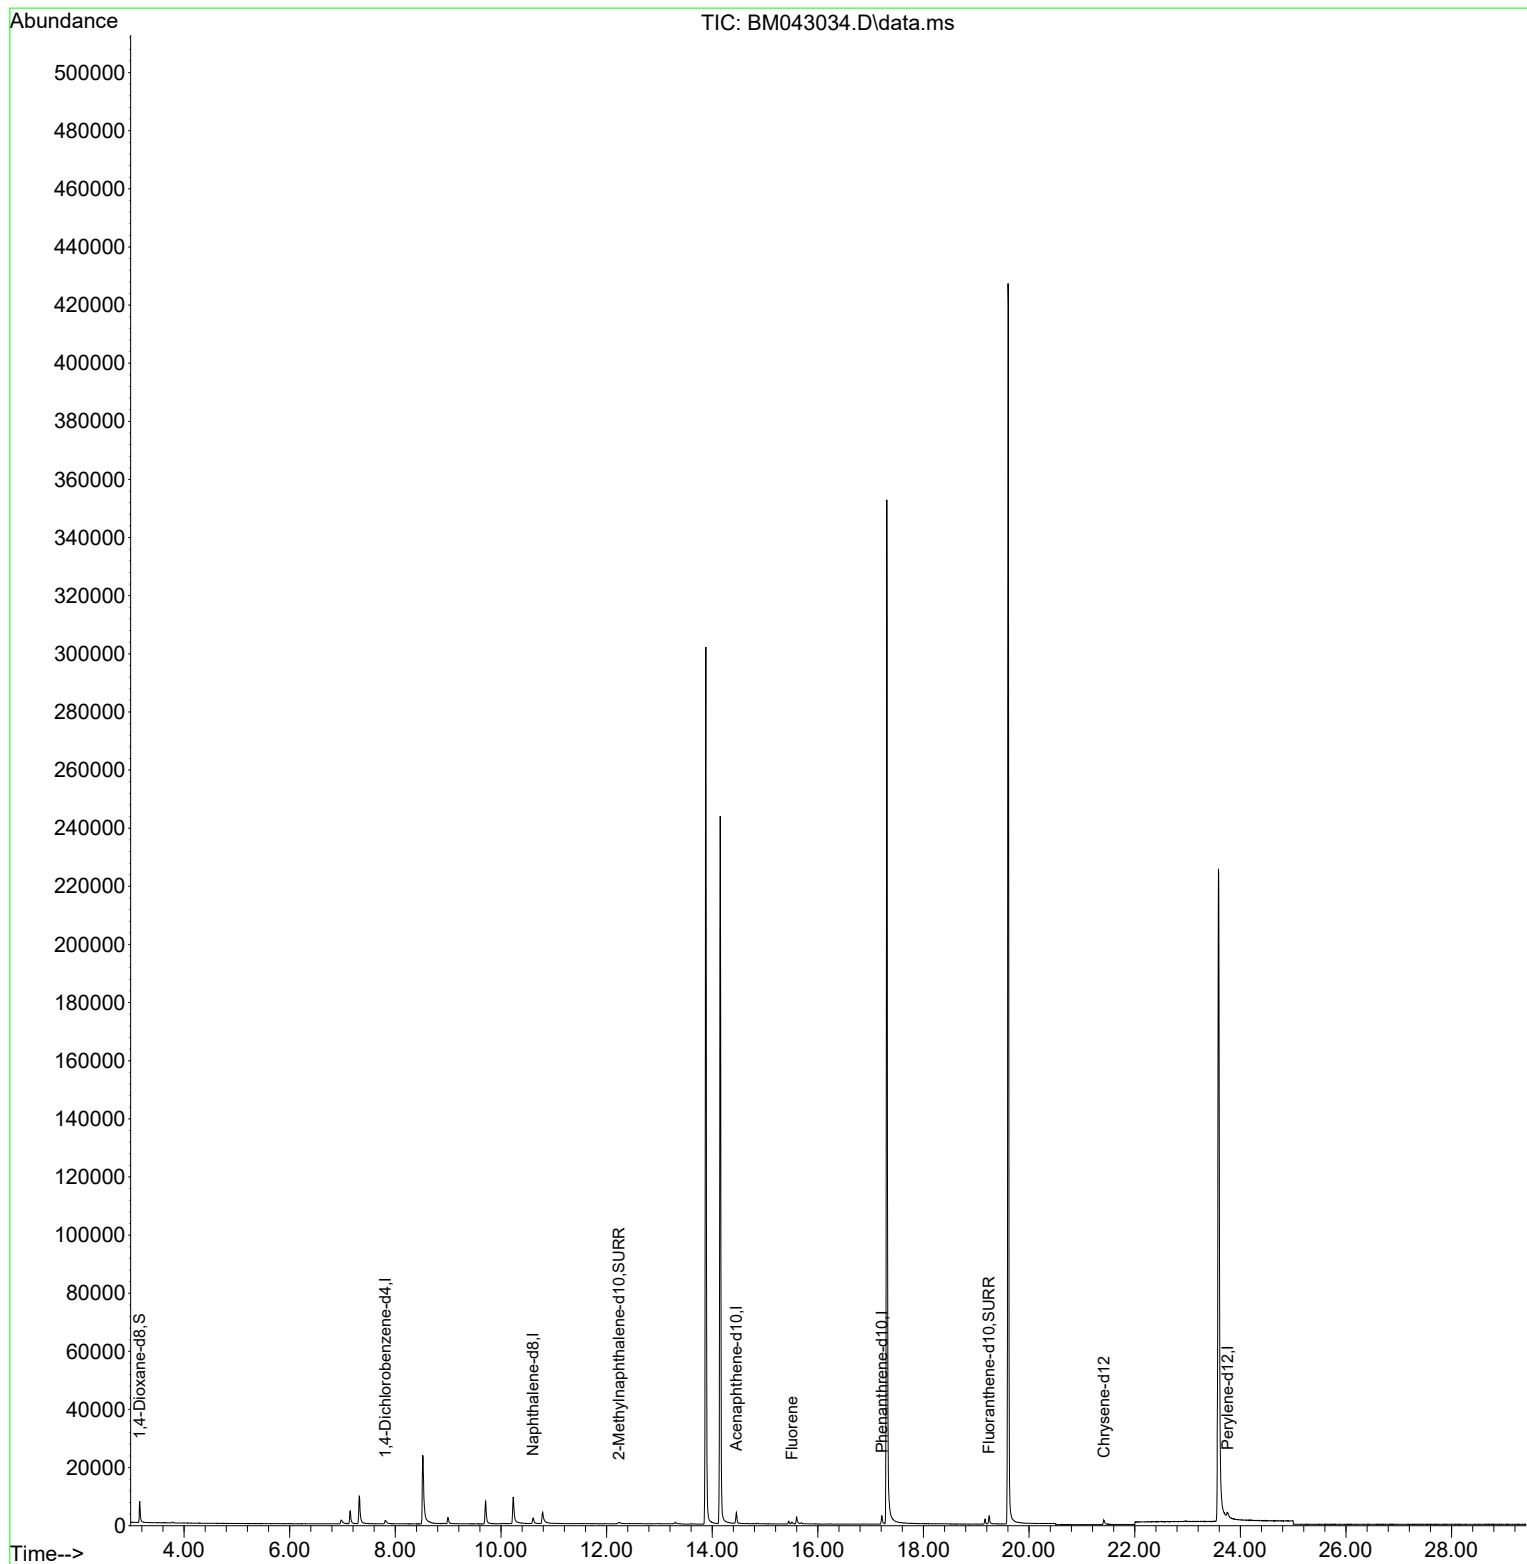

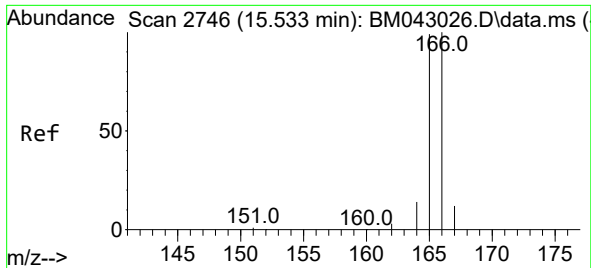

#12
 Fluorene
 Concen: 0.058 ng/ul
 RT: 15.506 min Scan# 21
 Delta R.T. -0.031 min
 Lab File: BM043034.D
 Acq: 26 Nov 2023 03:07

Instrument :
 BNA_M
 ClientSampleId :
 DCKC5

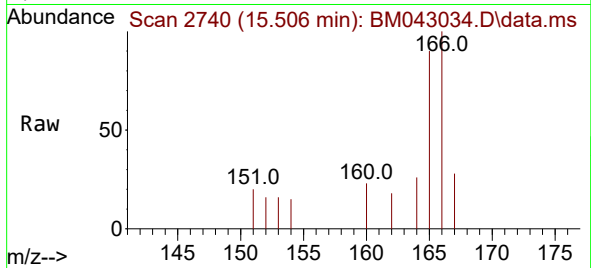

Tgt Ion:166 Resp: 498
 Ion Ratio Lower Upper
 166 100
 165 90.2 79.9 119.9
 167 28.4 14.2 21.4

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/28/2023
 Supervised By :mohammad ahmed 11/28/2023

