

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM112719\
 Data File : BM023919.D
 Acq On : 27 Nov 2019 19:09
 Operator : JU
 Sample : K5888-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JLLP0

Quant Time: Nov 28 00:21:44 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM112719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 27 17:16:22 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.49	152	390974	20.00	ng/ul	0.00
18) Naphthalene-d8	10.26	136	1577610	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.15	164	945881	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.90	188	1866408	20.00	ng/ul	0.00
78) Chrysene-d12	21.12	240	1695516	20.00	ng/ul	0.00
86) Perylene-d12	23.26	264	2074637	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.04	96	19824	2.26	ng/uL	0.00
5) Phenol-d5	6.68	99	409326	11.95	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.84	67	249249	12.51	ng/ul	0.00
9) 2-Chlorophenol-d4	7.03	132	330039	12.46	ng/ul	0.00
13) 4-Methylphenol-d8	8.21	113	297153	10.99	ng/ul	0.00
19) Nitrobenzene-d5	8.65	128	150640	12.30	ng/ul	0.00
22) 2-Nitrophenol-d4	9.36	143	163428	11.74	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.90	165	305747	11.60	ng/ul	0.00
29) 4-Chloroaniline-d4	10.42	131	314424	10.87	ng/ul	0.00
44) Dimethylphthalate-d6	13.57	166	995791	13.55	ng/ul	0.00
47) Acenaphthylene-d8	13.84	160	1081299	12.55	ng/ul	0.00
52) 4-Nitrophenol-d4	14.39	143	94617	7.66	ng/ul	0.01
58) Fluorene-d10	15.15	176	824539	13.33	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.30	200	93824	8.01	ng/ul	0.00
71) Anthracene-d10	17.00	188	1256955	14.10	ng/ul	0.00
79) Pyrene-d10	19.31	212	1384331	15.80	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.13	264	1658743	15.13	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.62	163	242429	3.370	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM112719\
Data File : BM023919.D
Acq On : 27 Nov 2019 19:09
Operator : JU
Sample : K5888-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JLLP0

Quant Time: Nov 28 00:21:44 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM112719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 27 17:16:22 2019
Response via : Initial Calibration

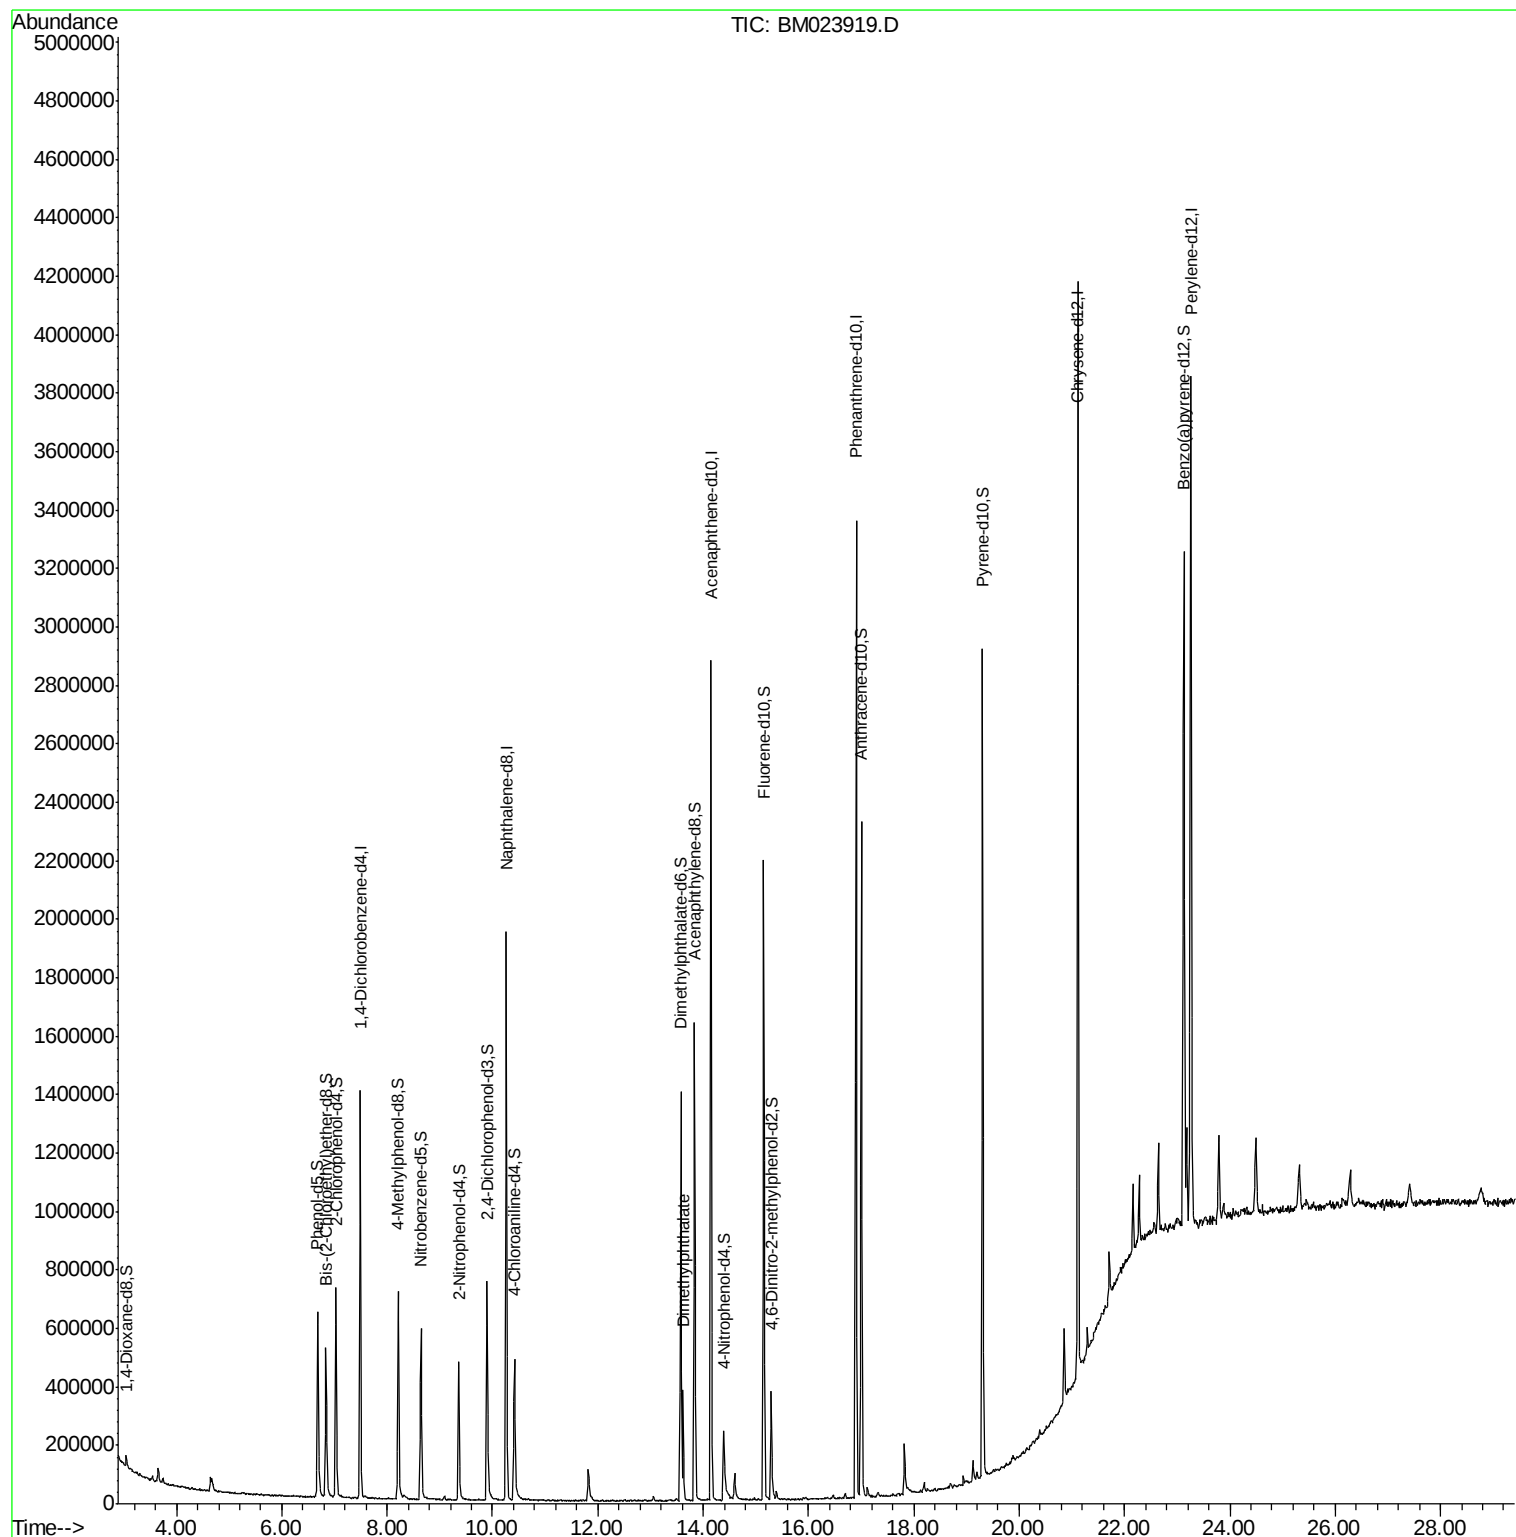

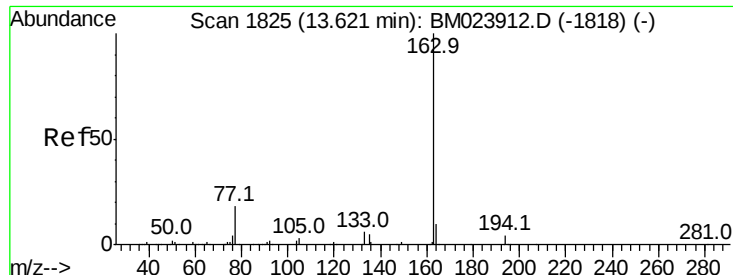

#45

Dimethylphthalate

Concen: 3.370 ng/ul

RT: 13.62 min Scan# 1825

Delta R.T. 0.00 min

Lab File: BM023919.D

Acq: 27 Nov 2019 19:09

Instrument :

BNA_M

ClientSampleId :

JLLP0


Tot Ion:163 Resp: 242429

Ion Ratio Lower Upper

163 100

194 3.9 3.2 4.8

164 9.8 8.0 12.0

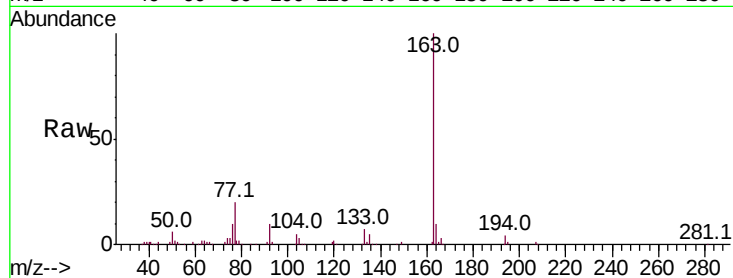

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

