

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM112719\
 Data File : BM023920.D
 Acq On : 27 Nov 2019 19:45
 Operator : JU
 Sample : K5888-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JLLP7

Quant Time: Nov 28 00:21:49 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM112719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 27 17:16:22 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.49	152	410485	20.00	ng/ul	0.00
18) Naphthalene-d8	10.26	136	1637232	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.15	164	979219	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.90	188	1959802	20.00	ng/ul	0.00
78) Chrysene-d12	21.12	240	1900959	20.00	ng/ul	0.00
86) Perylene-d12	23.26	264	2357096	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.04	96	27254	2.95	ng/uL	0.00
5) Phenol-d5	6.68	99	534890	14.87	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.84	67	335310	16.02	ng/ul	0.00
9) 2-Chlorophenol-d4	7.03	132	441266	15.87	ng/ul	0.00
13) 4-Methylphenol-d8	8.21	113	412543	14.53	ng/ul	0.00
19) Nitrobenzene-d5	8.65	128	199618	15.71	ng/ul	0.00
22) 2-Nitrophenol-d4	9.36	143	225256	15.60	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.90	165	397401	14.53	ng/ul	0.00
29) 4-Chloroaniline-d4	10.41	131	512804	17.08	ng/ul	0.00
44) Dimethylphthalate-d6	13.57	166	1235192	16.23	ng/ul	0.00
47) Acenaphthylene-d8	13.84	160	1425258	15.98	ng/ul	0.00
52) 4-Nitrophenol-d4	14.39	143	93678	7.32	ng/ul	0.01
58) Fluorene-d10	15.15	176	1044970	16.32	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.30	200	92993	7.56	ng/ul	0.00
71) Anthracene-d10	17.00	188	1619719	17.30	ng/ul	0.00
79) Pyrene-d10	19.31	212	1743906	17.75	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.12	264	2171818	17.43	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.62	163	566747	7.609	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM112719\
Data File : BM023920.D
Acq On : 27 Nov 2019 19:45
Operator : JU
Sample : K5888-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JLLP7

Quant Time: Nov 28 00:21:49 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM112719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 27 17:16:22 2019
Response via : Initial Calibration

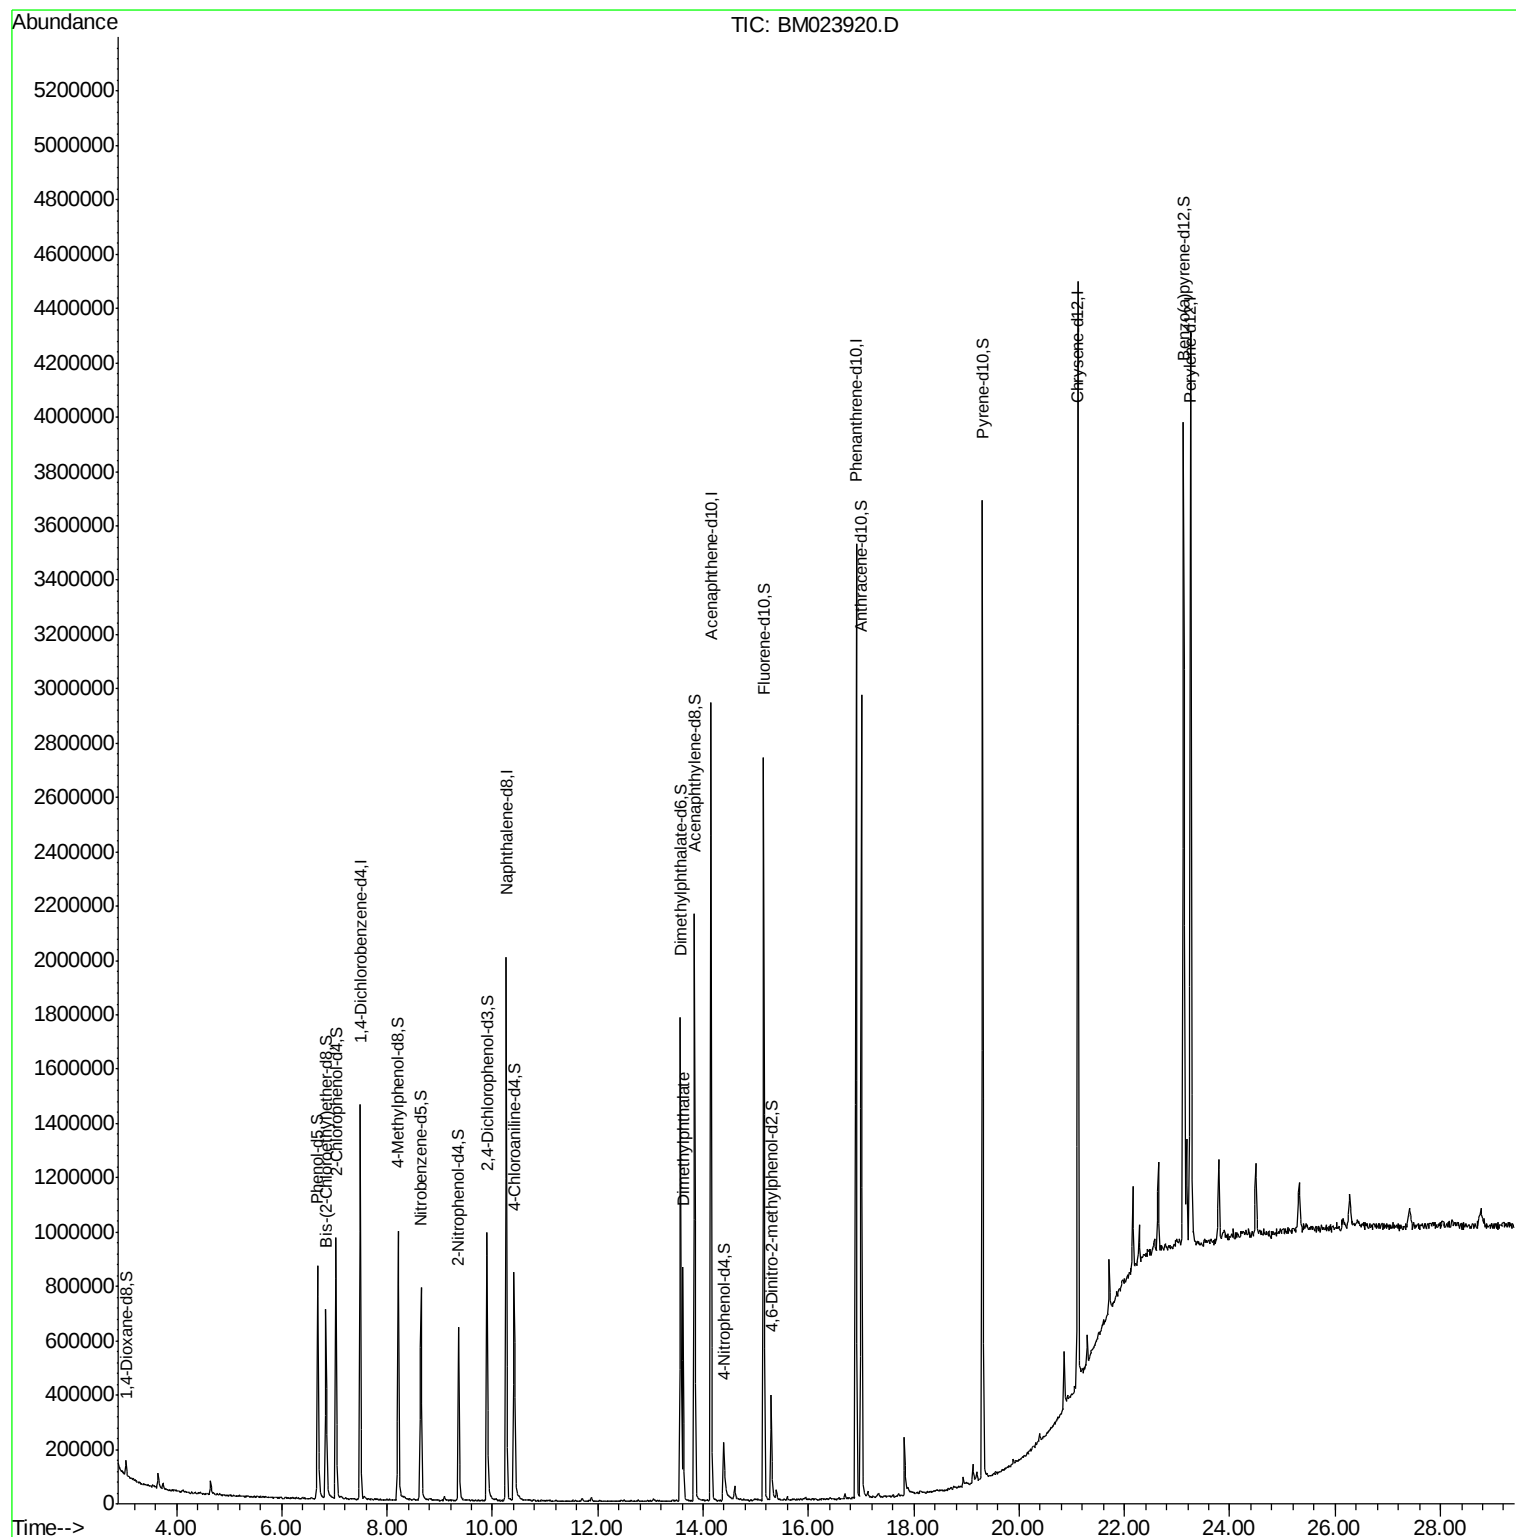

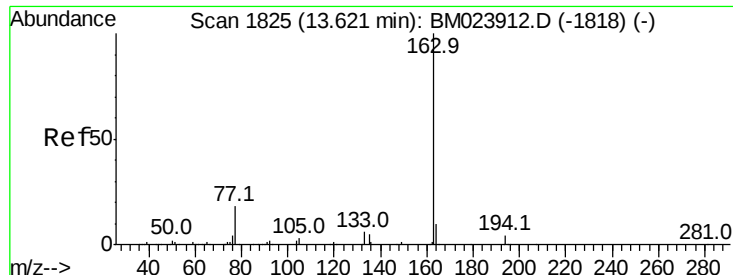

#45

Dimethylphthalate

Concen: 7.609 ng/ul

RT: 13.62 min Scan# 1825

Delta R.T. 0.00 min

Lab File: BM023920.D

Acq: 27 Nov 2019 19:45

Instrument :

BNA_M

ClientSampleId :

JLLP7


Tot Ion:163 Resp: 566747

Ion Ratio Lower Upper

163 100

194 4.2 3.2 4.8

164 10.6 8.0 12.0

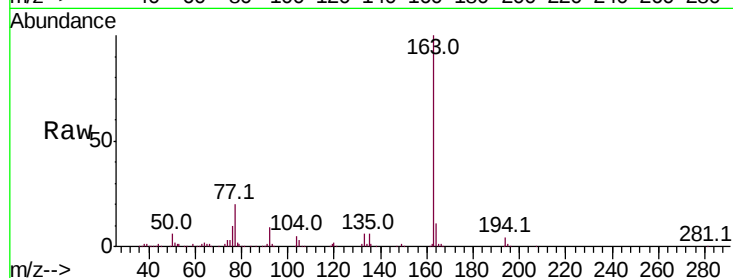

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

