

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM112719\
 Data File : BM023928.D
 Acq On : 28 Nov 2019 00:33
 Operator : JU
 Sample : K5888-10
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JLLR7

Quant Time: Nov 28 03:07:44 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM112719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Nov 28 00:24:52 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.49	152	426826	20.00	ng/ul	0.00
18) Naphthalene-d8	10.26	136	1799407	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.15	164	1105405	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.90	188	2112243	20.00	ng/ul	0.00
78) Chrysene-d12	21.11	240	1712985	20.00	ng/ul	0.00
86) Perylene-d12	23.25	264	2103071	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.04	96	36926	3.85	ng/uL	0.00
5) Phenol-d5	6.68	99	677330	18.11	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.84	67	429922	19.76	ng/ul	0.00
9) 2-Chlorophenol-d4	7.03	132	550565	19.04	ng/ul	0.00
13) 4-Methylphenol-d8	8.20	113	508897	17.24	ng/ul	0.00
19) Nitrobenzene-d5	8.64	128	270446	19.36	ng/ul	0.00
22) 2-Nitrophenol-d4	9.36	143	299710	18.88	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.90	165	536301	17.84	ng/ul	0.00
29) 4-Chloroaniline-d4	10.41	131	639479	19.38	ng/ul	0.00
44) Dimethylphthalate-d6	13.57	166	1738023	20.24	ng/ul	0.00
47) Acenaphthylene-d8	13.84	160	1966484	19.54	ng/ul	0.00
52) 4-Nitrophenol-d4	14.38	143	176574	12.23	ng/ul	0.00
58) Fluorene-d10	15.15	176	1439727	19.92	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.29	200	167287	12.62	ng/ul	0.00
71) Anthracene-d10	17.00	188	2047154	20.29	ng/ul	0.00
79) Pyrene-d10	19.31	212	2073310	23.42	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.12	264	2360532	21.23	ng/ul	-0.01


Target Compounds					Ovalue	
45) Dimethylphthalate	13.62	163	776007	9.230	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM112719\
Data File : BM023928.D
Acq On : 28 Nov 2019 00:33
Operator : JU
Sample : K5888-10
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JLLR7

Quant Time: Nov 28 03:07:44 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM112719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Nov 28 00:24:52 2019
Response via : Initial Calibration

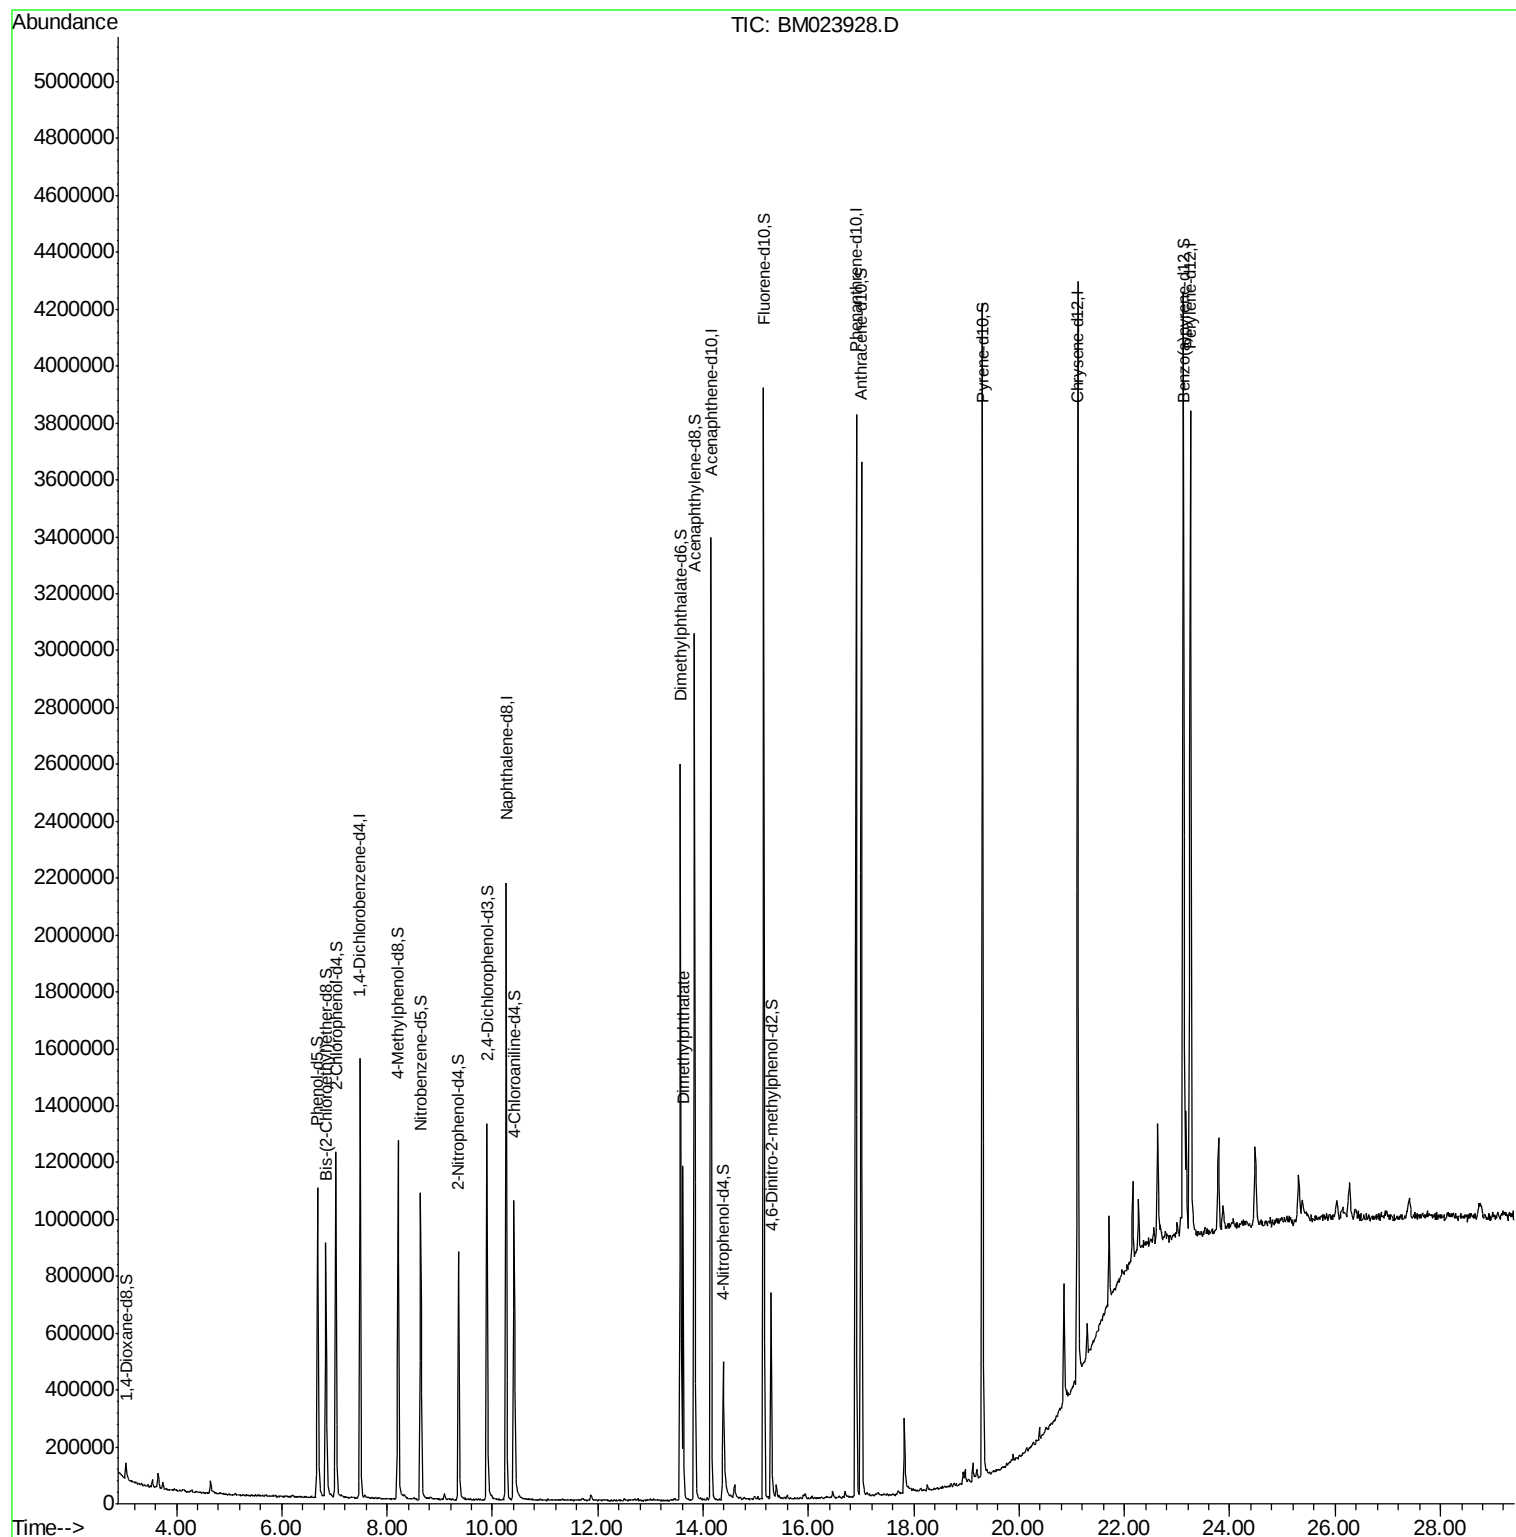

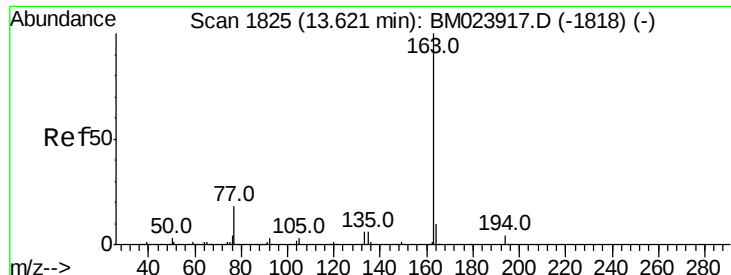

#45

Dimethylphthalate

Concen: 9.230 ng/ul

RT: 13.62 min Scan# 1824

Delta R.T. -0.01 min

Lab File: BM023928.D

Acq: 28 Nov 2019 00:33

Instrument :

BNA_M

ClientSampleId :

JLLR7


Tot Ion:163 Resp: 776007

Ion Ratio Lower Upper

163 100

194 3.9 3.2 4.8

164 10.5 8.0 12.0

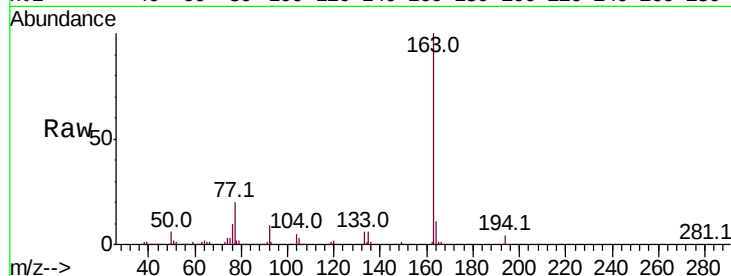

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

