

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM112719\
 Data File : BM023931.D
 Acq On : 28 Nov 2019 02:21
 Operator : JU
 Sample : K5888-13
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JLLS0

Quant Time: Nov 28 03:08:02 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM112719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Nov 28 00:24:52 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.49	152	461946	20.00	ng/ul	0.00
18) Naphthalene-d8	10.26	136	1937739	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.15	164	1181364	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.90	188	2232807	20.00	ng/ul	0.00
78) Chrysene-d12	21.11	240	1850661	20.00	ng/ul	0.00
86) Perylene-d12	23.25	264	2296905	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.04	96	31754	3.06	ng/uL	0.00
5) Phenol-d5	6.68	99	614845	15.19	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.84	67	394391	16.75	ng/ul	0.00
9) 2-Chlorophenol-d4	7.03	132	504131	16.11	ng/ul	0.00
13) 4-Methylphenol-d8	8.20	113	464774	14.55	ng/ul	0.00
19) Nitrobenzene-d5	8.64	128	244440	16.25	ng/ul	0.00
22) 2-Nitrophenol-d4	9.36	143	268170	15.69	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.90	165	484221	14.96	ng/ul	0.00
29) 4-Chloroaniline-d4	10.41	131	585337	16.48	ng/ul	0.00
44) Dimethylphthalate-d6	13.57	166	1566687	17.07	ng/ul	0.00
47) Acenaphthylene-d8	13.84	160	1807801	16.80	ng/ul	0.00
52) 4-Nitrophenol-d4	14.39	143	145478	9.43	ng/ul	0.00
58) Fluorene-d10	15.15	176	1312246	16.99	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.29	200	147603	10.53	ng/ul	0.00
71) Anthracene-d10	17.00	188	1857270	17.42	ng/ul	0.00
79) Pyrene-d10	19.31	212	1891591	19.78	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.11	264	2209601	18.20	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.62	163	602088	6.701	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM112719\
Data File : BM023931.D
Acq On : 28 Nov 2019 02:21
Operator : JU
Sample : K5888-13
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JLLS0

Quant Time: Nov 28 03:08:02 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM112719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Nov 28 00:24:52 2019
Response via : Initial Calibration

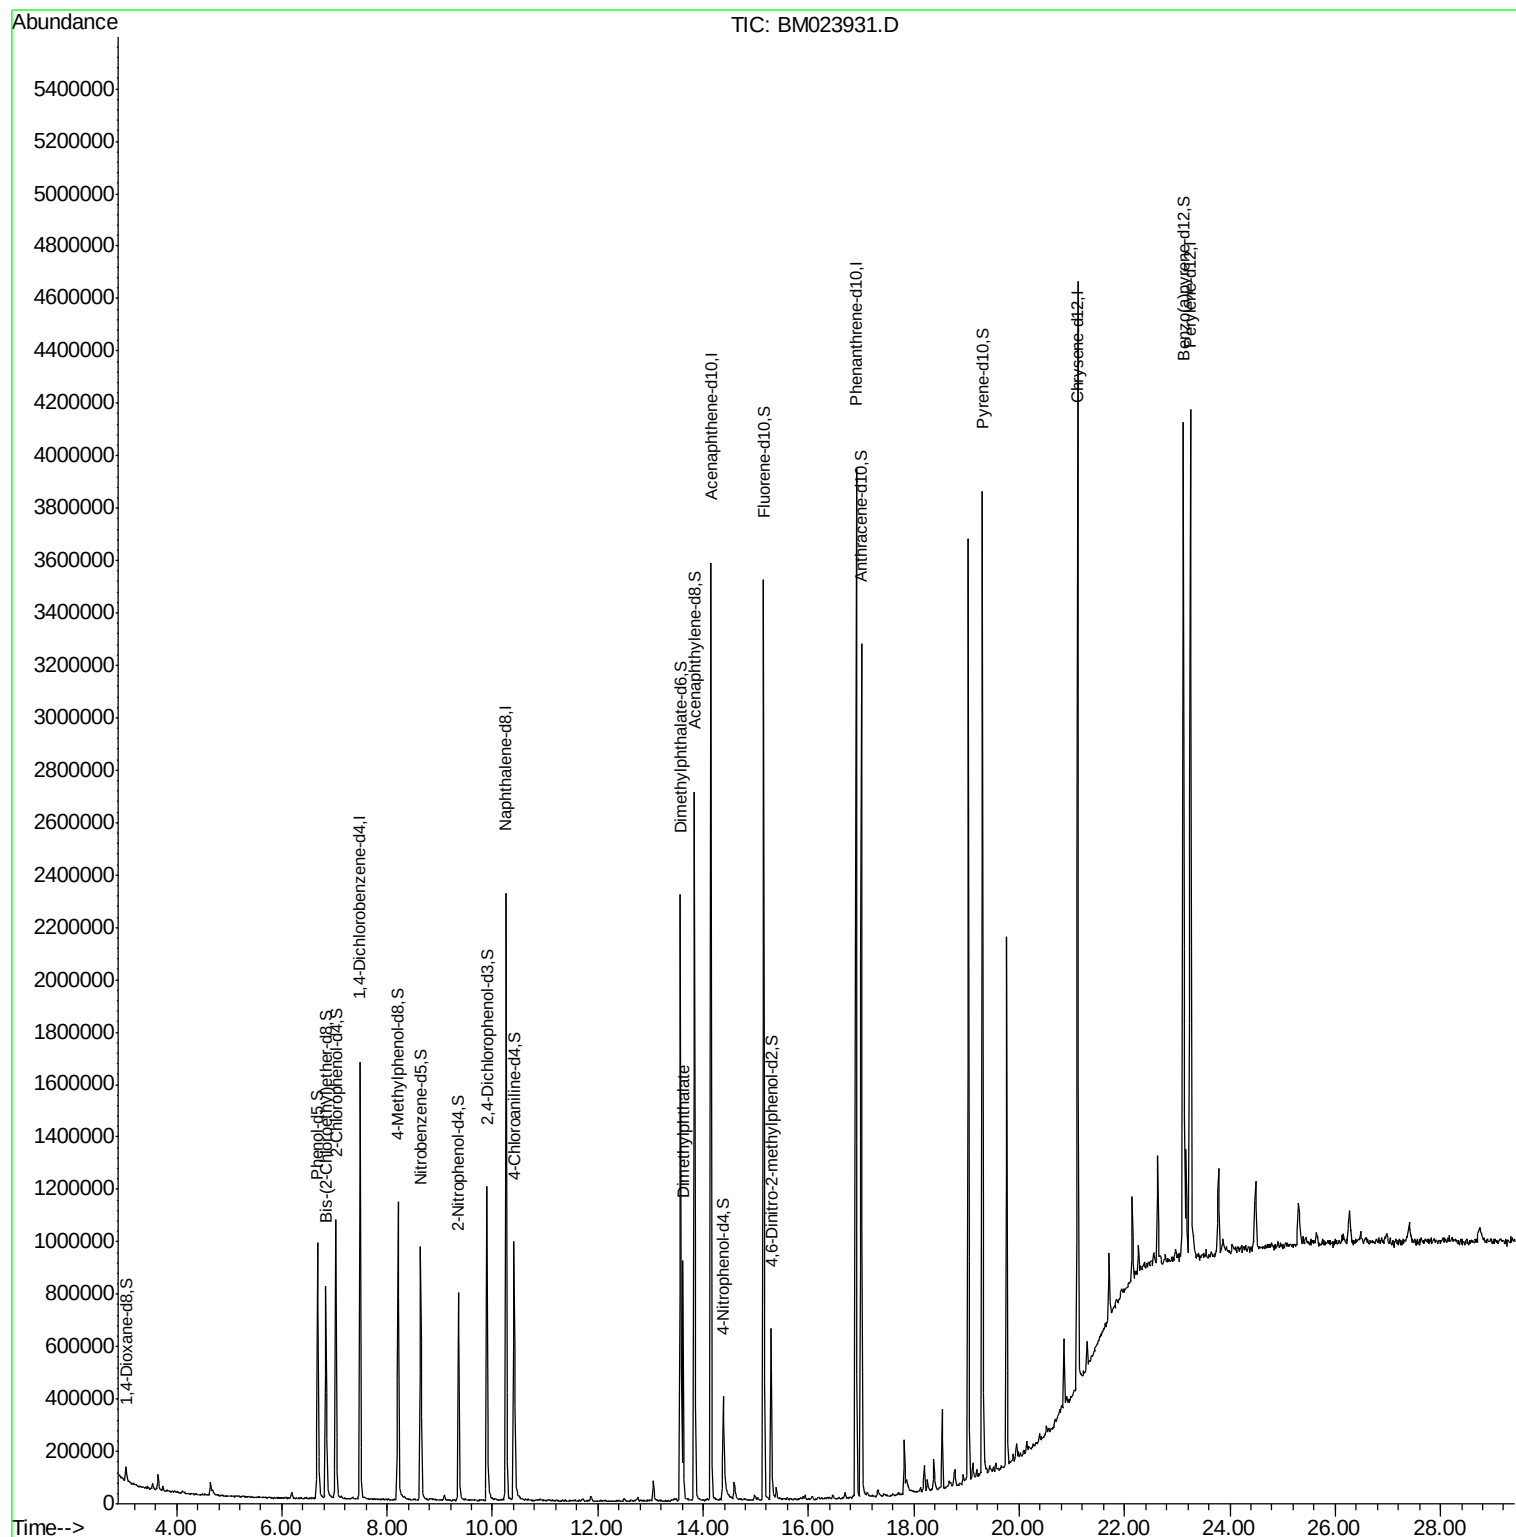

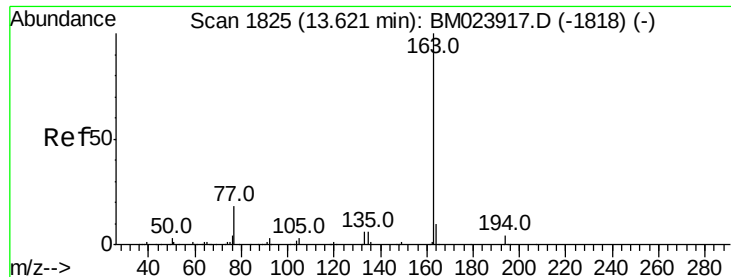

#45

Dimethylphthalate

Concen: 6.701 ng/ul

RT: 13.62 min Scan# 1824

Delta R.T. -0.01 min

Lab File: BM023931.D

Acq: 28 Nov 2019 02:21

Instrument :

BNA_M

ClientSampleId :

JLLS0


Tot Ion:163 Resp: 602088

Ion Ratio Lower Upper

163 100

194 4.0 3.2 4.8

164 10.5 8.0 12.0

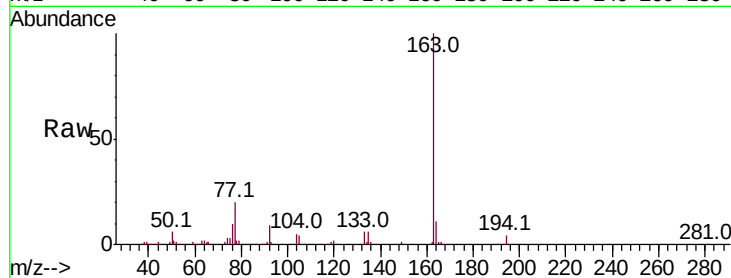

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

