

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM112719\
 Data File : BM023939.D
 Acq On : 28 Nov 2019 07:08
 Operator : JU
 Sample : PB125001BL
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK01

Quant Time: Nov 28 21:35:48 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM112719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 27 17:16:22 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.49	152	394917	20.00	ng/ul	0.00
18) Naphthalene-d8	10.26	136	1639686	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.15	164	1032080	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.90	188	2199359	20.00	ng/ul	0.00
78) Chrysene-d12	21.11	240	2184997	20.00	ng/ul	0.00
86) Perylene-d12	23.25	264	2708277	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.03	96	71260	8.03	ng/uL	0.00
5) Phenol-d5	6.67	99	1280957	37.01	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.83	67	781948	38.84	ng/ul	0.00
9) 2-Chlorophenol-d4	7.02	132	1027500	38.41	ng/ul	0.00
13) 4-Methylphenol-d8	8.20	113	1039016	38.05	ng/ul	0.00
19) Nitrobenzene-d5	8.64	128	504787	39.66	ng/ul	0.00
22) 2-Nitrophenol-d4	9.36	143	573955	39.68	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.89	165	1004622	36.68	ng/ul	0.00
29) 4-Chloroaniline-d4	10.40	131	1417832	47.16	ng/ul	0.00
44) Dimethylphthalate-d6	13.57	166	3307740	41.25	ng/ul	0.00
47) Acenaphthylene-d8	13.84	160	3903835	41.54	ng/ul	0.00
52) 4-Nitrophenol-d4	14.37	143	512533	38.02	ng/ul	0.00
58) Fluorene-d10	15.15	176	2826716	41.89	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.37	200	2137	0.15	ng/ul	0.08
71) Anthracene-d10	17.00	188	4355057	41.46	ng/ul	0.00
79) Pyrene-d10	19.31	212	4648600	41.17	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.12	264	5817499	40.64	ng/ul	0.00

Target Compounds


				Ovalue		
15) N-Nitroso-di-n-propylamine	8.20	70	24506	1.098	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM112719\
Data File : BM023939.D
Acq On : 28 Nov 2019 07:08
Operator : JU
Sample : PB125001BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK01

Quant Time: Nov 28 21:35:48 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM112719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 27 17:16:22 2019
Response via : Initial Calibration

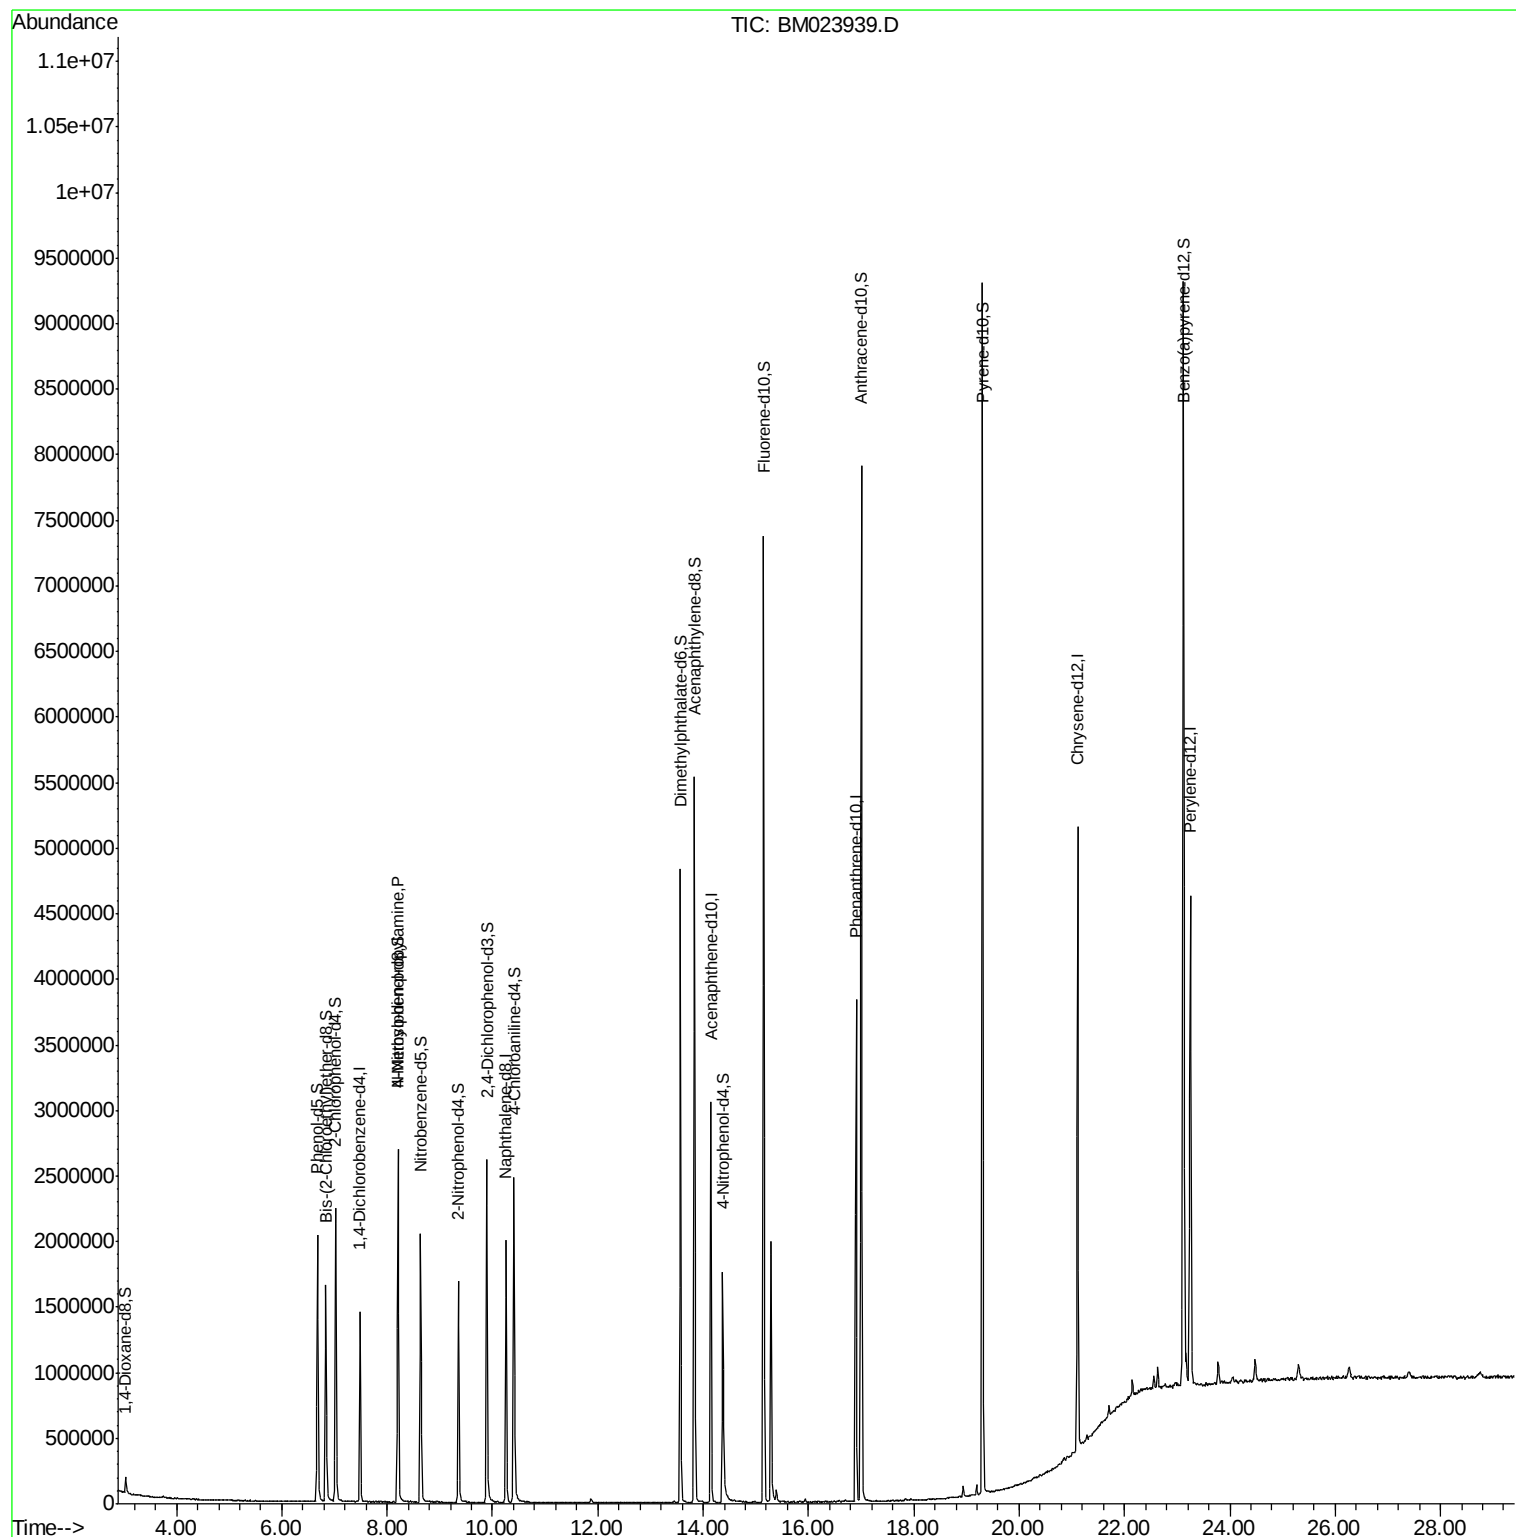

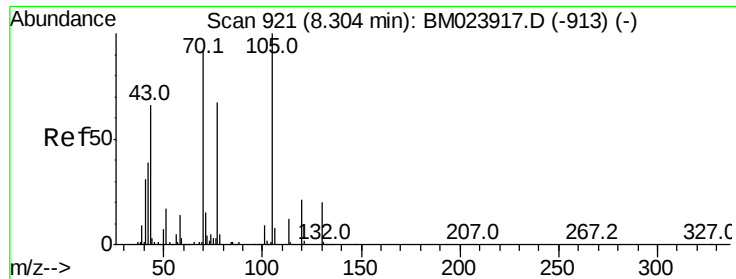

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.098 ng/ul
 RT: 8.20 min Scan# 904
 Delta R.T. -0.10 min
 Lab File: BM023939.D
 Acq: 28 Nov 2019 07:08

Instrument :
 BNA_M
 ClientSampleId :
 SBLK01

Tot Ion: 70 Resp: 24506
 Ion Ratio Lower Upper
 70 100
 42 329.4 34.4 51.6#
 101 0.0 7.3 10.9#
 130 0.0 16.1 24.1#

