

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM112719\
 Data File : BM023946.D
 Acq On : 28 Nov 2019 11:18
 Operator : JU
 Sample : K5915-07
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JLNW2

Quant Time: Nov 28 21:36:28 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM112719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 27 17:16:22 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.49	152	259108	20.00	ng/ul	0.00
18) Naphthalene-d8	10.26	136	1260650	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.15	164	941976	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.90	188	2010956	20.00	ng/ul	0.00
78) Chrysene-d12	21.11	240	1961380	20.00	ng/ul	0.00
86) Perylene-d12	23.25	264	2450906	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.03	96	65270	11.21	ng/uL	0.00
5) Phenol-d5	6.67	99	1192468	52.51	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.83	67	725869	54.96	ng/ul	0.00
9) 2-Chlorophenol-d4	7.02	132	993230	56.59	ng/ul	0.00
13) 4-Methylphenol-d8	8.20	113	974741	54.40	ng/ul	0.00
19) Nitrobenzene-d5	8.64	128	484061	49.47	ng/ul	0.00
22) 2-Nitrophenol-d4	9.36	143	541044	48.65	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.89	165	970054	46.06	ng/ul	0.00
29) 4-Chloroaniline-d4	10.40	131	1277941	55.29	ng/ul	0.00
44) Dimethylphthalate-d6	13.57	166	2902116	39.65	ng/ul	0.00
47) Acenaphthylene-d8	13.83	160	3585060	41.79	ng/ul	0.00
52) 4-Nitrophenol-d4	14.37	143	389604	31.66	ng/ul	0.00
58) Fluorene-d10	15.15	176	2512619	40.79	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.29	200	376036	29.79	ng/ul	0.00
71) Anthracene-d10	17.00	188	3766942	39.22	ng/ul	0.00
79) Pyrene-d10	19.30	212	4034569	39.81	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.12	264	5068643	39.12	ng/ul	0.00

Target Compounds


				Ovalue	
6) Phenol	6.70	94	43017	1.841	ng/ul 92
45) Dimethylphthalate	13.62	163	729810	10.186	ng/ul 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM112719\
Data File : BM023946.D
Acq On : 28 Nov 2019 11:18
Operator : JU
Sample : K5915-07
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JLNLW2

Quant Time: Nov 28 21:36:28 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM112719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 27 17:16:22 2019
Response via : Initial Calibration

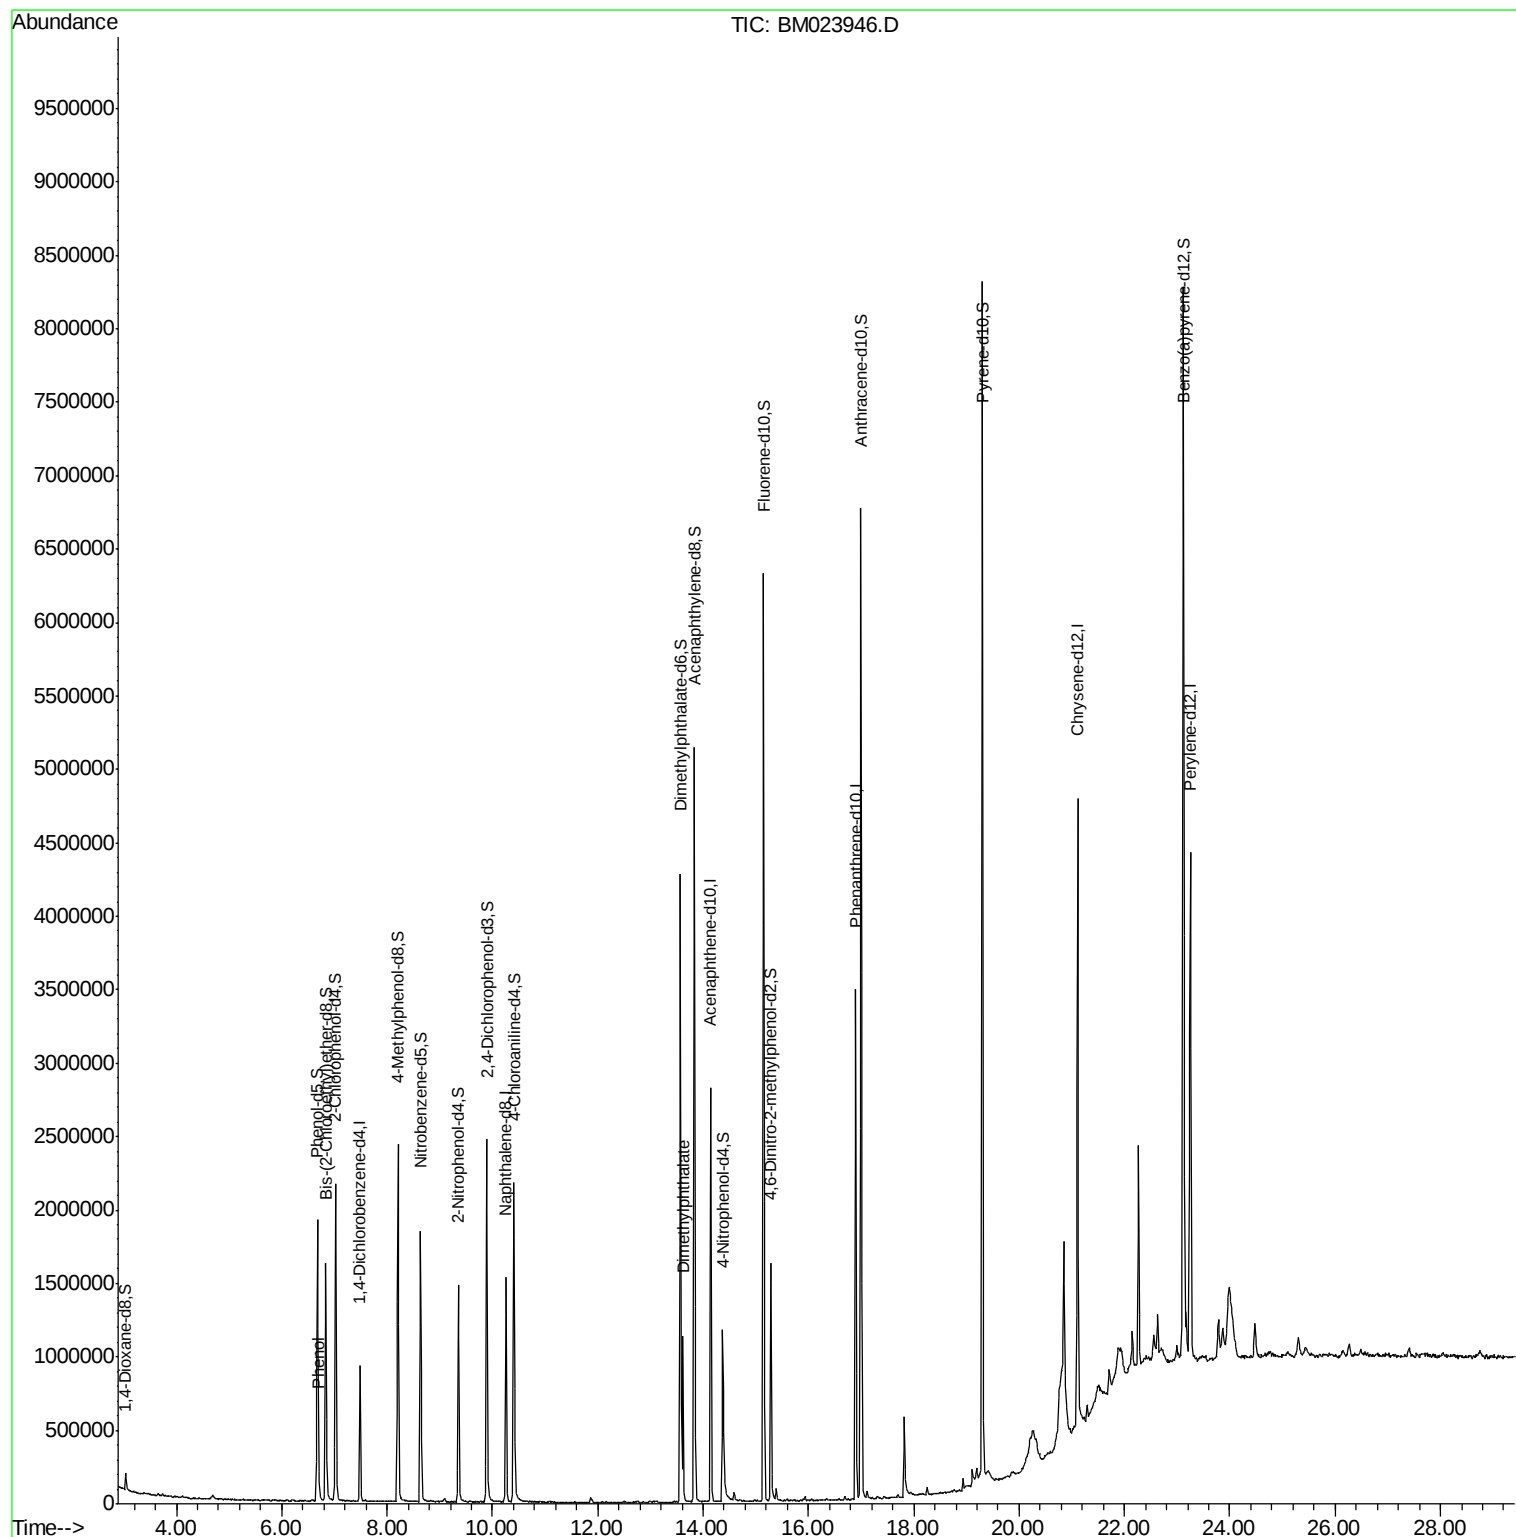

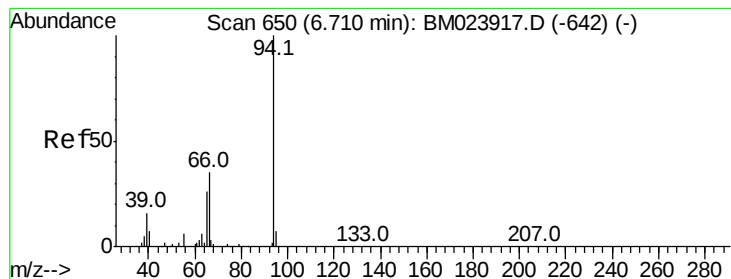

#6

Phenol

Concen: 1.841 ng/ul

RT: 6.70 min Scan# 649

Delta R.T. -0.01 min

Lab File: BM023946.D

Acq: 28 Nov 2019 11:18

Instrument :

BNA_M

ClientSampleId :

JLNW2


Tot Ion: 94 Resp: 43017

Ion Ratio Lower Upper

94 100

65 28.3 20.8 31.2




66 42.0 28.6 43.0

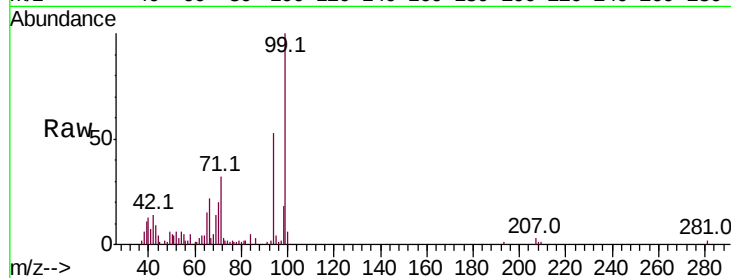

Abundance Ion 94.00 (93.70 to 94.70): BM023917.D (-642) (-)

Ion 65.00 (64.70 to 65.70): BM023917.D (-642) (-)

Ion 66.00 (65.70 to 66.70): BM023917.D (-642) (-)

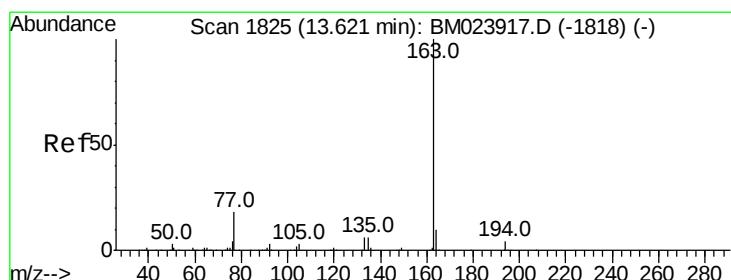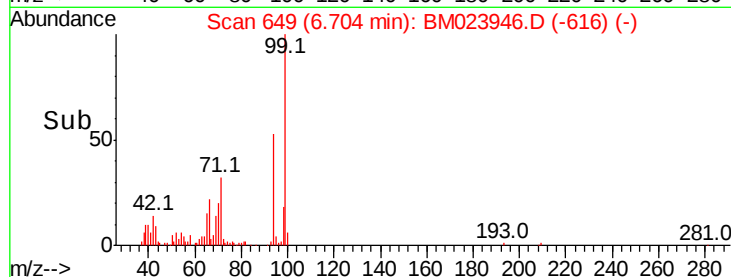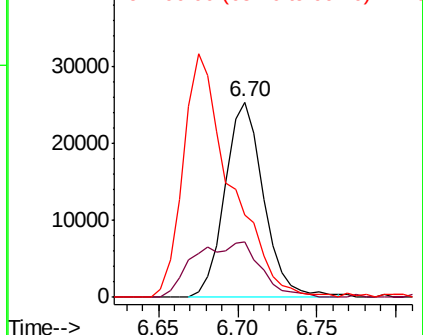

#45

Dimethylphthalate

Concen: 10.186 ng/ul

RT: 13.62 min Scan# 1824

Delta R.T. -0.01 min

Lab File: BM023946.D

Acq: 28 Nov 2019 11:18


Tgt Ion: 163 Resp: 729810

Ion Ratio Lower Upper

163 100

194 4.0 3.2 4.8

164 10.0 8.0 12.0

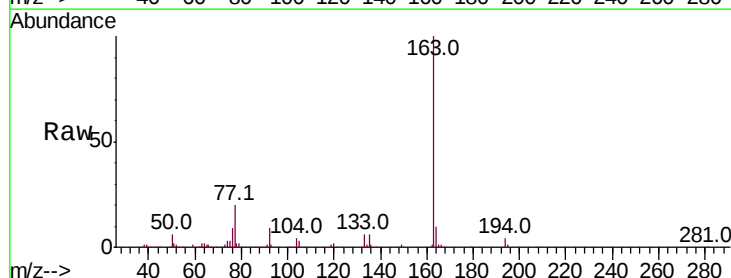

Abundance Ion 163.00 (162.70 to 163.70): BM023917.D (-1818) (-)

Ion 194.00 (193.70 to 194.70): BM023917.D (-1818) (-)

Ion 164.00 (163.70 to 164.70): BM023917.D (-1818) (-)

