

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM112719\
 Data File : BM023921.D
 Acq On : 27 Nov 2019 20:21
 Operator : JU
 Sample : K5888-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JLLP8

Quant Time: Nov 28 00:21:55 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM112719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 27 17:16:22 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.49	152	369434	20.00	ng/ul	0.00
18) Naphthalene-d8	10.26	136	1514472	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.15	164	908854	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.90	188	1785363	20.00	ng/ul	0.00
78) Chrysene-d12	21.11	240	1577408	20.00	ng/ul	0.00
86) Perylene-d12	23.26	264	1935863	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.04	96	34808	4.19	ng/uL	0.00
5) Phenol-d5	6.68	99	670374	20.70	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.84	67	417857	22.19	ng/ul	0.00
9) 2-Chlorophenol-d4	7.03	132	545408	21.79	ng/ul	0.00
13) 4-Methylphenol-d8	8.21	113	499579	19.56	ng/ul	0.00
19) Nitrobenzene-d5	8.64	128	261128	22.21	ng/ul	0.00
22) 2-Nitrophenol-d4	9.36	143	293611	21.98	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.90	165	520620	20.58	ng/ul	0.00
29) 4-Chloroaniline-d4	10.41	131	636341	22.92	ng/ul	0.00
44) Dimethylphthalate-d6	13.57	166	1683826	23.84	ng/ul	0.00
47) Acenaphthylene-d8	13.84	160	1917130	23.16	ng/ul	0.00
52) 4-Nitrophenol-d4	14.38	143	185214	15.60	ng/ul	0.00
58) Fluorene-d10	15.15	176	1407886	23.69	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.29	200	190497	17.00	ng/ul	0.00
71) Anthracene-d10	17.00	188	2096512	24.59	ng/ul	0.00
79) Pyrene-d10	19.31	212	2184699	26.80	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.12	264	2605537	25.46	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.62	163	736268	10.651	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM112719\
Data File : BM023921.D
Acq On : 27 Nov 2019 20:21
Operator : JU
Sample : K5888-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JLLP8

Quant Time: Nov 28 00:21:55 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM112719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 27 17:16:22 2019
Response via : Initial Calibration

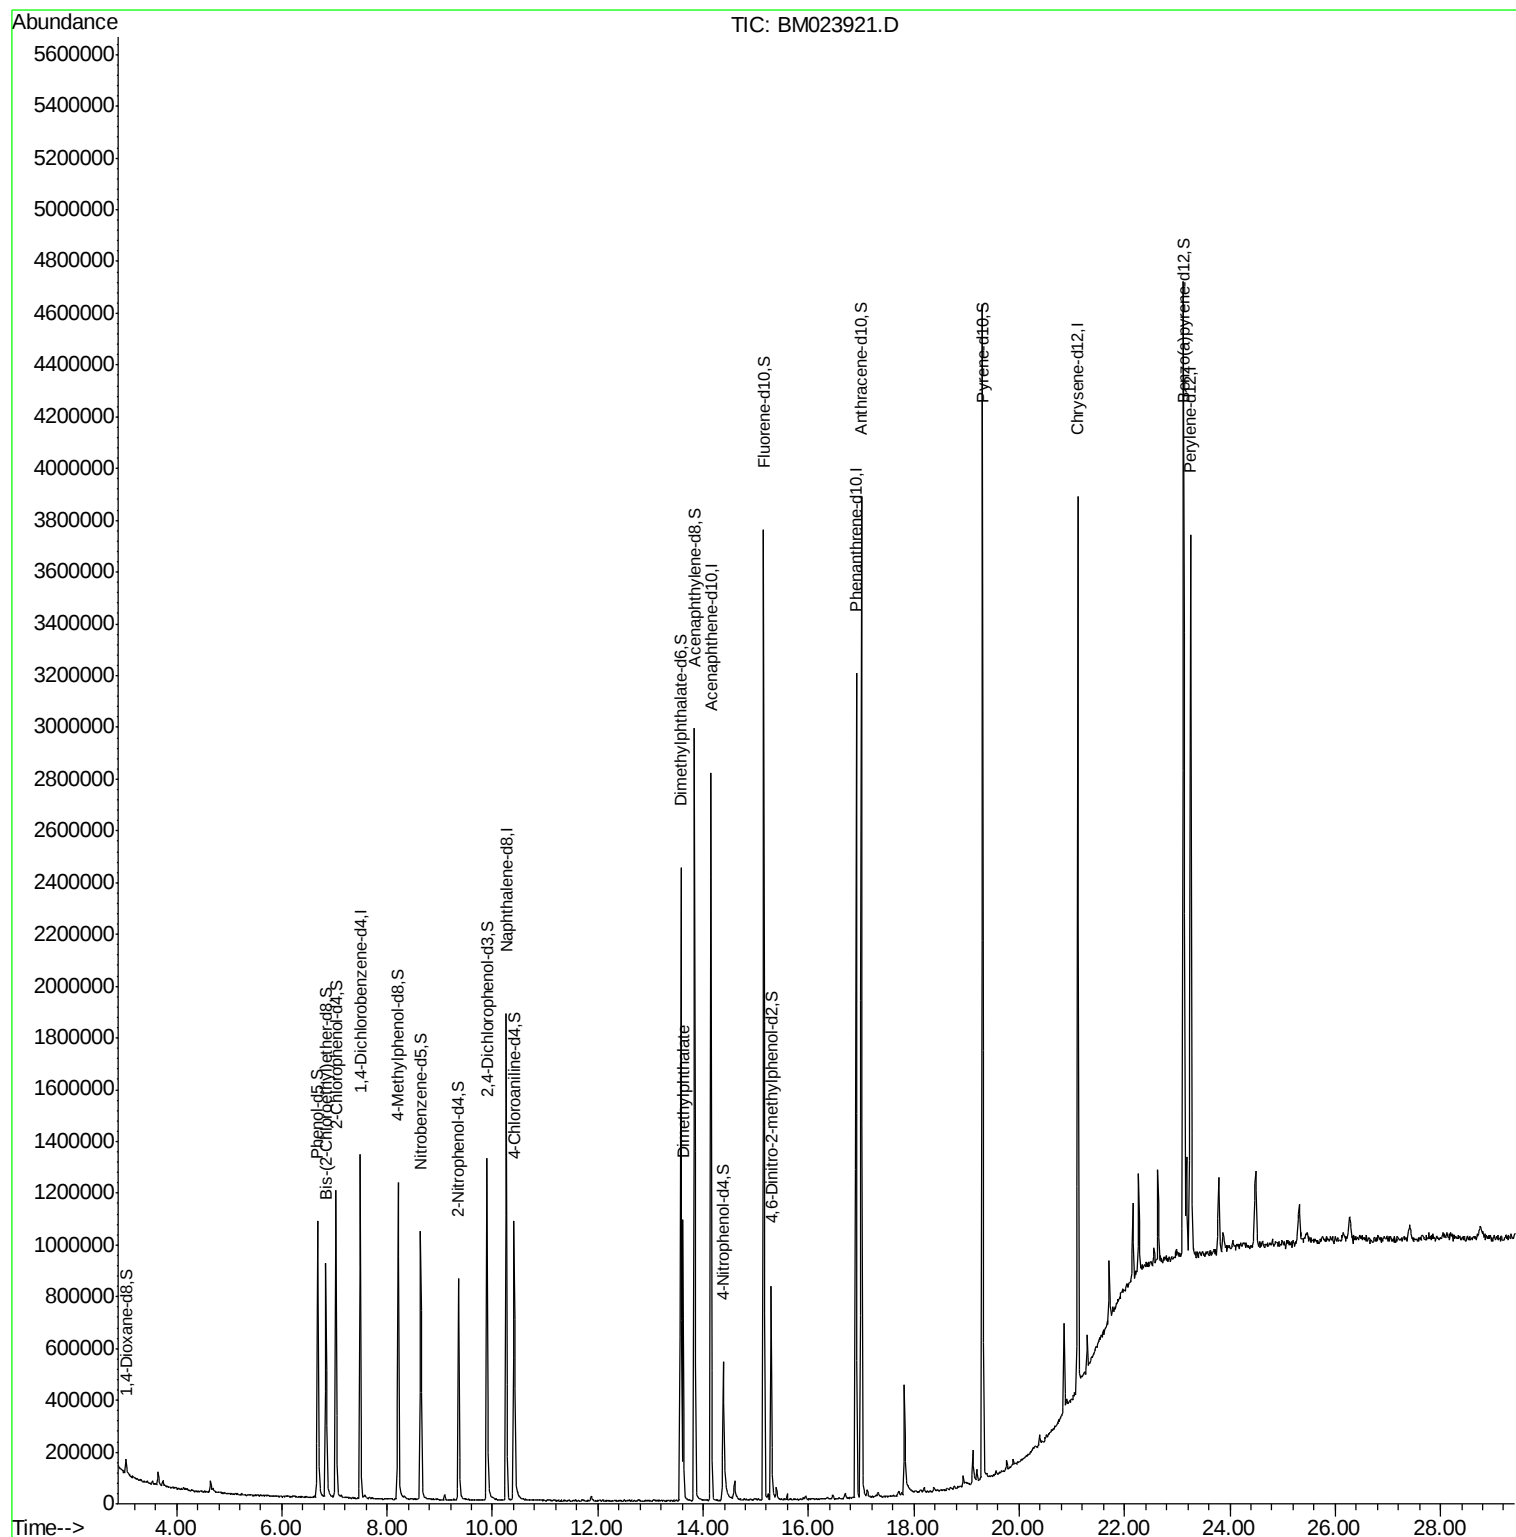

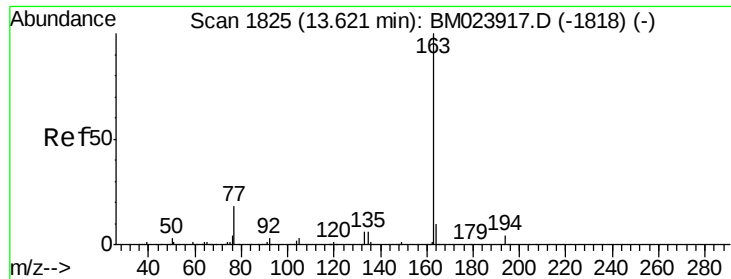

#45

Dimethylphthalate

Concen: 10.651 ng/ul

RT: 13.62 min Scan# 1825

Delta R.T. -0.00 min

Lab File: BM023921.D

Acq: 27 Nov 2019 20:21

Instrument :

BNA_M

ClientSampleId :

JLLP8


Tot Ion:163 Resp: 736268

Ion Ratio Lower Upper

163 100

194 4.6 3.2 4.8

164 9.9 8.0 12.0

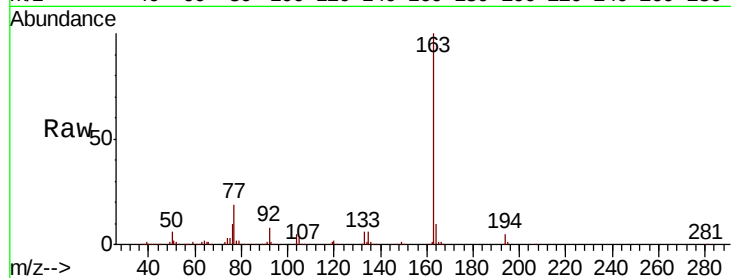

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

