

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM112719\
 Data File : BM023930.D
 Acq On : 28 Nov 2019 01:45
 Operator : JU
 Sample : K5888-12
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JLLR9

Quant Time: Nov 28 03:07:55 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM112719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Nov 28 00:24:52 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.49	152	449955	20.00	ng/ul	0.00
18) Naphthalene-d8	10.26	136	1861775	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.15	164	1133396	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.90	188	2169470	20.00	ng/ul	0.00
78) Chrysene-d12	21.11	240	1839185	20.00	ng/ul	0.00
86) Perylene-d12	23.25	264	2252646	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.04	96	27890	2.76	ng/uL	0.00
5) Phenol-d5	6.68	99	571686	14.50	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.84	67	361703	15.77	ng/ul	0.00
9) 2-Chlorophenol-d4	7.03	132	467719	15.34	ng/ul	0.00
13) 4-Methylphenol-d8	8.20	113	410478	13.19	ng/ul	0.00
19) Nitrobenzene-d5	8.64	128	229269	15.87	ng/ul	0.00
22) 2-Nitrophenol-d4	9.36	143	252434	15.37	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.89	165	451598	14.52	ng/ul	0.00
29) 4-Chloroaniline-d4	10.41	131	594311	17.41	ng/ul	0.00
44) Dimethylphthalate-d6	13.57	166	1506246	17.10	ng/ul	0.00
47) Acenaphthylene-d8	13.84	160	1688685	16.36	ng/ul	0.00
52) 4-Nitrophenol-d4	14.38	143	187968	12.70	ng/ul	0.00
58) Fluorene-d10	15.15	176	1259314	16.99	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.29	200	206341	15.15	ng/ul	0.00
71) Anthracene-d10	17.00	188	2117551	20.44	ng/ul	0.00
79) Pyrene-d10	19.30	212	2270596	23.89	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.12	264	2690988	22.60	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.62	163	631671	7.327	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM112719\
Data File : BM023930.D
Acq On : 28 Nov 2019 01:45
Operator : JU
Sample : K5888-12
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JLLR9

Quant Time: Nov 28 03:07:55 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM112719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Nov 28 00:24:52 2019
Response via : Initial Calibration

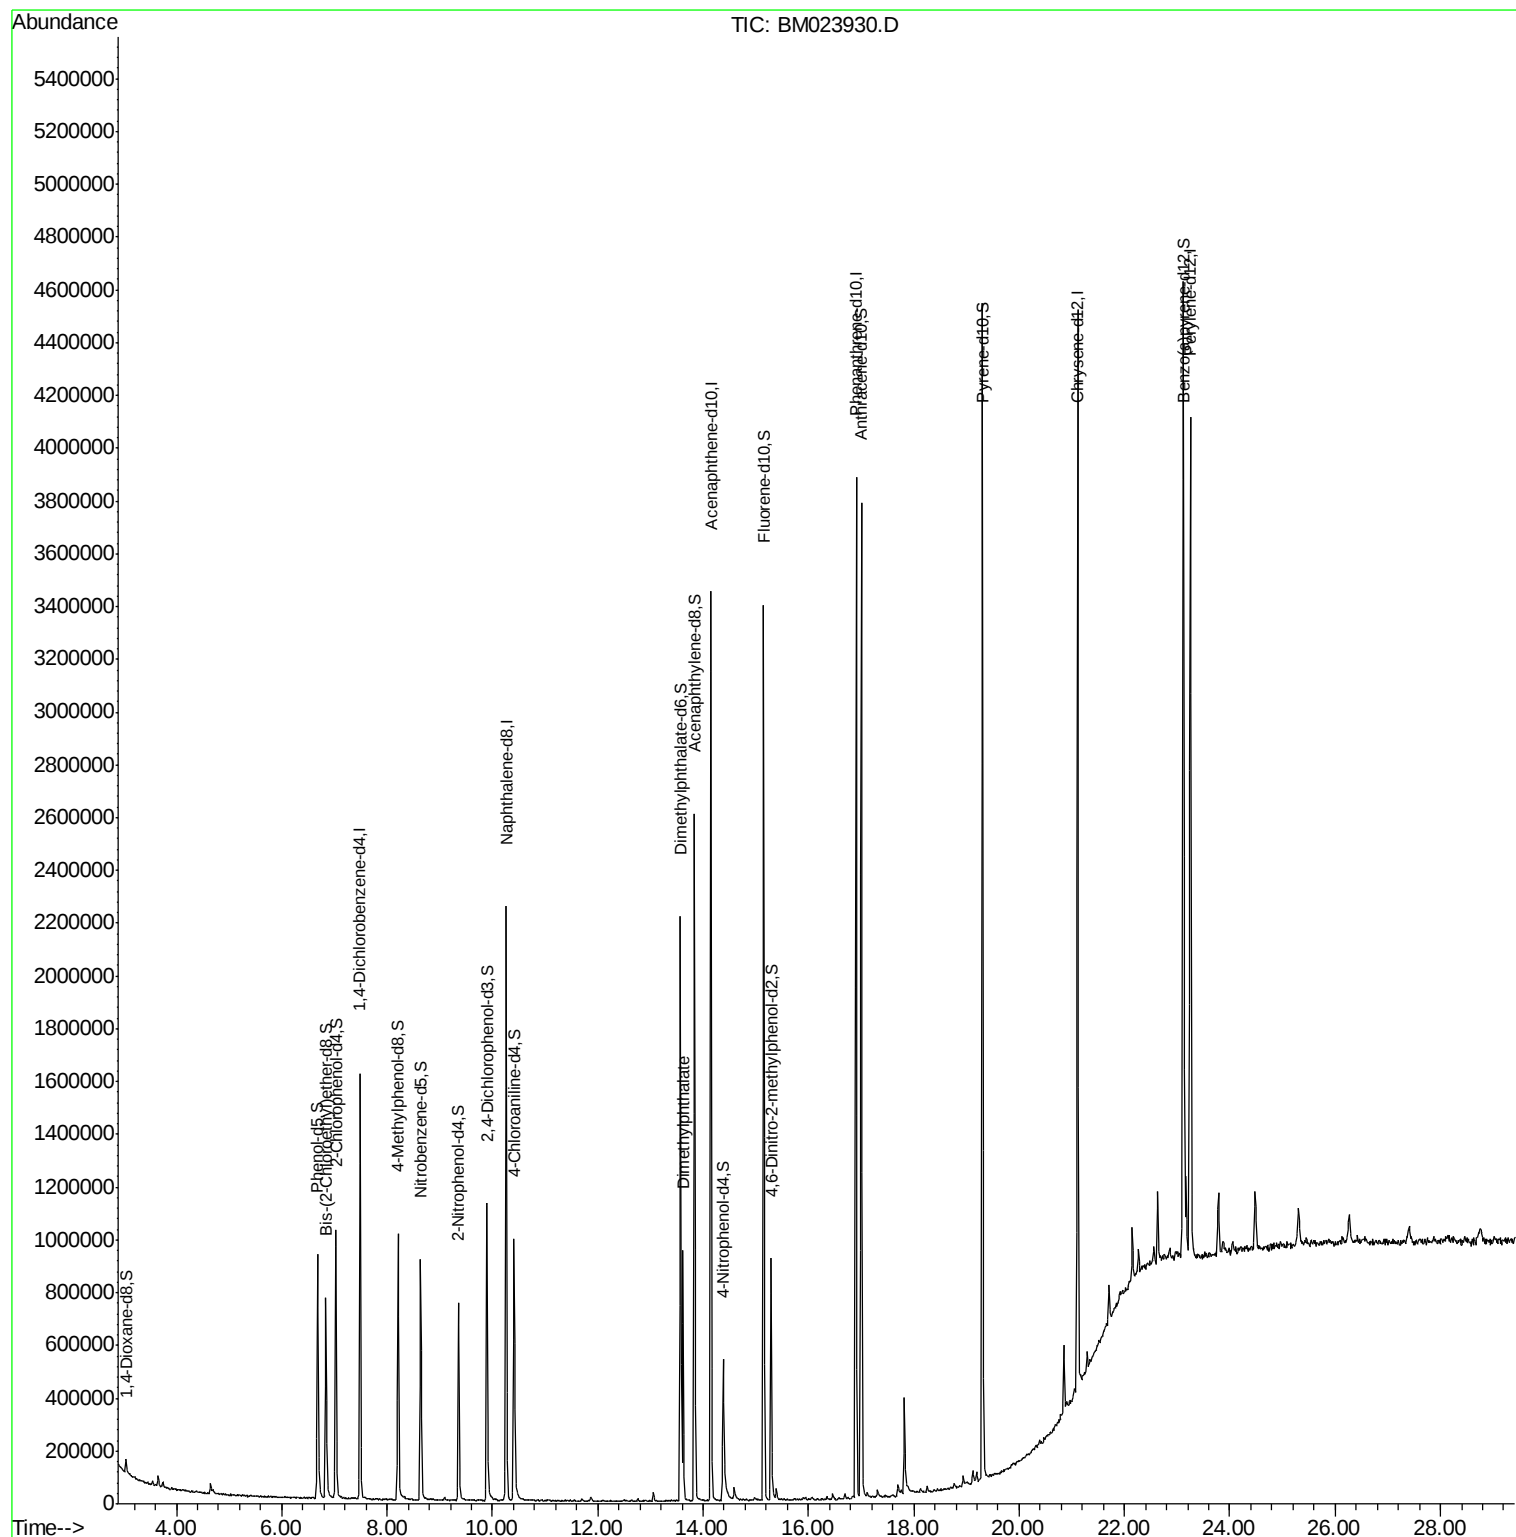

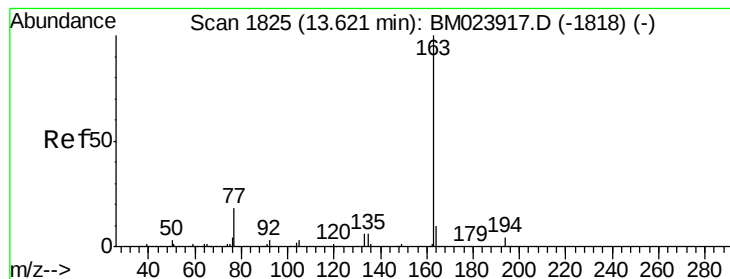

#45

Dimethylphthalate

Concen: 7.327 ng/ul

RT: 13.62 min Scan# 1824

Delta R.T. -0.01 min

Lab File: BM023930.D

Acq: 28 Nov 2019 01:45

Instrument :

BNA_M

ClientSampleId :

JLLR9


Tot Ion:163 Resp: 631671

Ion Ratio Lower Upper

163 100

194 3.9 3.2 4.8

164 9.9 8.0 12.0

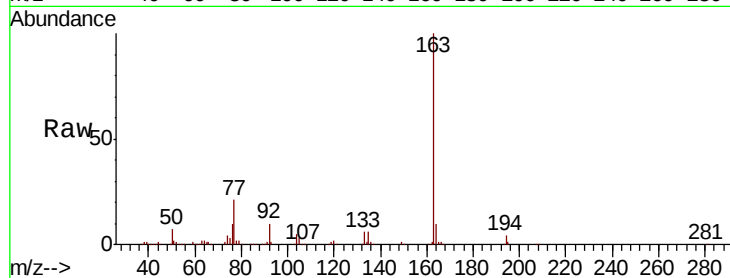

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

