

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM112719\
 Data File : BM023950.D
 Acq On : 28 Nov 2019 13:41
 Operator : JU
 Sample : K5915-11
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JLNx0

Quant Time: Nov 28 21:36:50 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM112719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 27 17:16:22 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.49	152	400418	20.00	ng/ul	0.00
18) Naphthalene-d8	10.26	136	1608013	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.15	164	957370	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.90	188	1981936	20.00	ng/ul	0.00
78) Chrysene-d12	21.11	240	1976524	20.00	ng/ul	0.00
86) Perylene-d12	23.25	264	2466667	20.00	ng/ul	-0.01

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.03	96	36005	4.00	ng/uL	0.00
5) Phenol-d5	6.67	99	722227	20.58	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.83	67	453037	22.20	ng/ul	0.00
9) 2-Chlorophenol-d4	7.02	132	587048	21.64	ng/ul	0.00
13) 4-Methylphenol-d8	8.20	113	562645	20.32	ng/ul	0.00
19) Nitrobenzene-d5	8.64	128	277178	22.21	ng/ul	0.00
22) 2-Nitrophenol-d4	9.36	143	309081	21.79	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.89	165	566449	21.09	ng/ul	0.00
29) 4-Chloroaniline-d4	10.40	131	676719	22.95	ng/ul	0.00
44) Dimethylphthalate-d6	13.57	166	1775250	23.86	ng/ul	0.00
47) Acenaphthylene-d8	13.83	160	2115428	24.26	ng/ul	0.00
52) 4-Nitrophenol-d4	14.38	143	210234	16.81	ng/ul	0.00
58) Fluorene-d10	15.14	176	1542609	24.64	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.29	200	204717	16.45	ng/ul	0.00
71) Anthracene-d10	17.00	188	2309308	24.40	ng/ul	0.00
79) Pyrene-d10	19.30	212	2590728	25.37	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.11	264	3301890	25.32	ng/ul	-0.01


Target Compounds					Ovalue	
6) Phenol	6.70	94	42358	1.173	ng/ul#	90
45) Dimethylphthalate	13.62	163	609312	8.368	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM112719\
Data File : BM023950.D
Acq On : 28 Nov 2019 13:41
Operator : JU
Sample : K5915-11
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JLNX0

Quant Time: Nov 28 21:36:50 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM112719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 27 17:16:22 2019
Response via : Initial Calibration

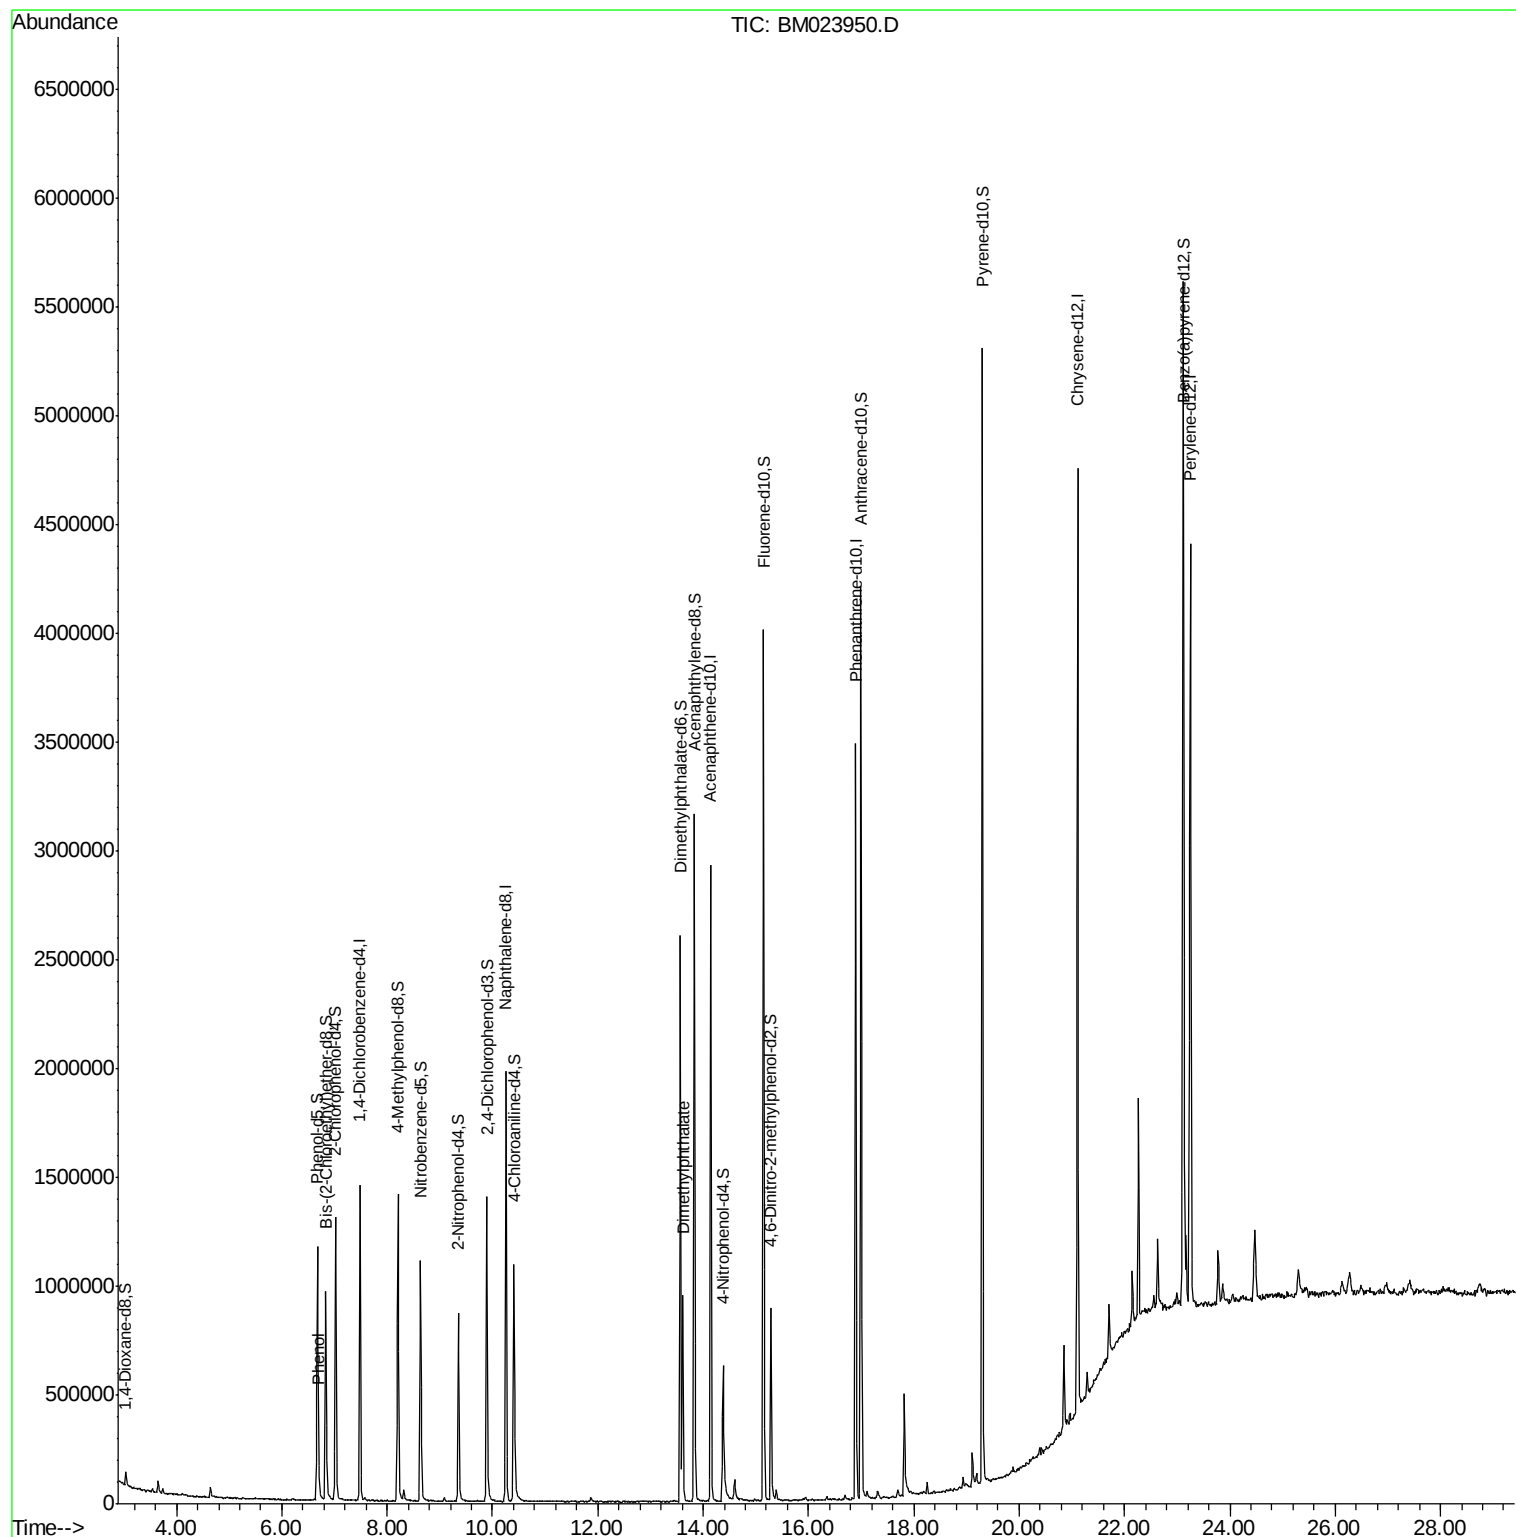

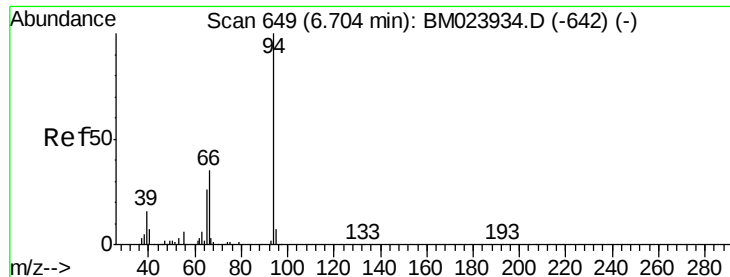





#6

Phenol

Concen: 1.173 ng/ul
 RT: 6.70 min Scan# 649
 Delta R.T. -0.01 min
 Lab File: BM023950.D
 Acq: 28 Nov 2019 13:41

Instrument :
 BNA_M
 ClientSampleId :
 JLNK0

Tot Ion: 94 Resp: 42358
 Ion Ratio Lower Upper
 94 100
 65 28.7 20.8 31.2
 66 44.2 28.6 43.0#

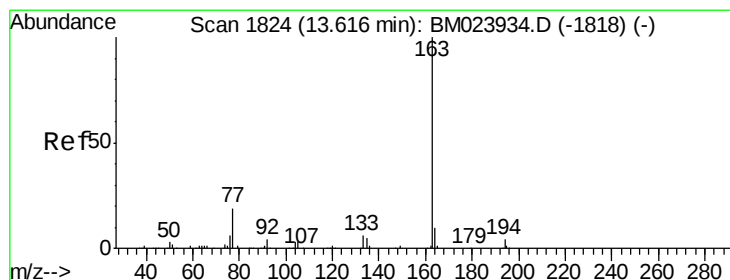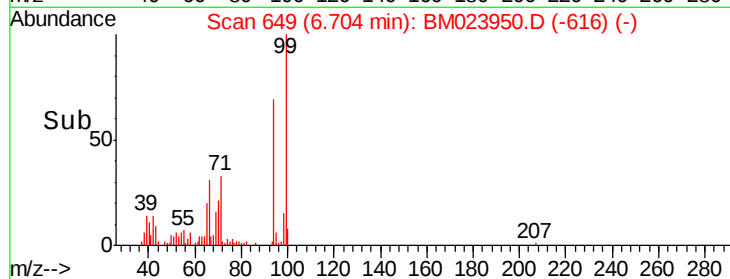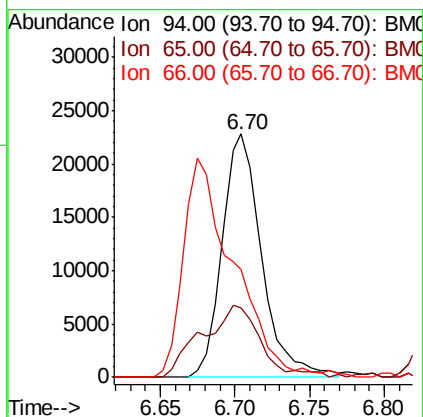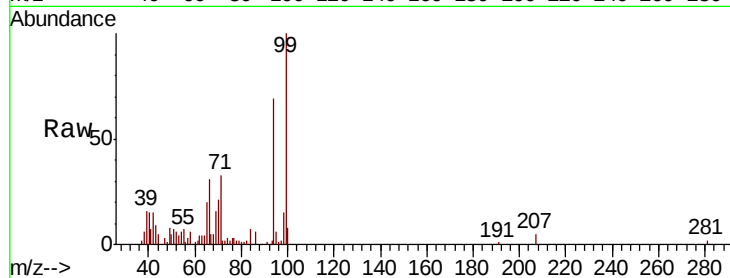

#45

Dimethylphthalate

Concen: 8.368 ng/ul
 RT: 13.62 min Scan# 1824
 Delta R.T. -0.01 min
 Lab File: BM023950.D
 Acq: 28 Nov 2019 13:41

Tgt Ion: 163 Resp: 609312
 Ion Ratio Lower Upper
 163 100
 194 4.1 3.2 4.8
 164 10.5 8.0 12.0

