

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112723\
 Data File : BM043050.D
 Acq On : 27 Nov 2023 14:59
 Operator : MA/JU
 Sample : 05264-16
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCKS7

Quant Time: Nov 27 23:41:05 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 27 02:36:19 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.809	152	984	0.400	ng/ul	#-0.07
4) Naphthalene-d8	10.605	136	3338	0.400	ng/ul	#-0.04
9) Acenaphthene-d10	14.455	164	1944	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.305	188	313833	0.400	ng/ul	# 0.07
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.42
23) Perylene-d12	23.753	264	5703	0.400	ng/ul	#-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.160	96	3489	2.311	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.233	152	1127	0.252	ng/ul	-0.02
18) Fluoranthene-d10	19.242	212	3314	0.000	ng/ul	-0.02
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.193	88	49	0.030	ng/ul#	79
26) Benzo(a)pyrene	23.589	252	1234	0.059	ng/ul#	63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112723\
Data File : BM043050.D
Acq On : 27 Nov 2023 14:59
Operator : MA/JU
Sample : 05264-16
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKS7

Quant Time: Nov 27 23:41:05 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 27 02:36:19 2023
Response via : Initial Calibration




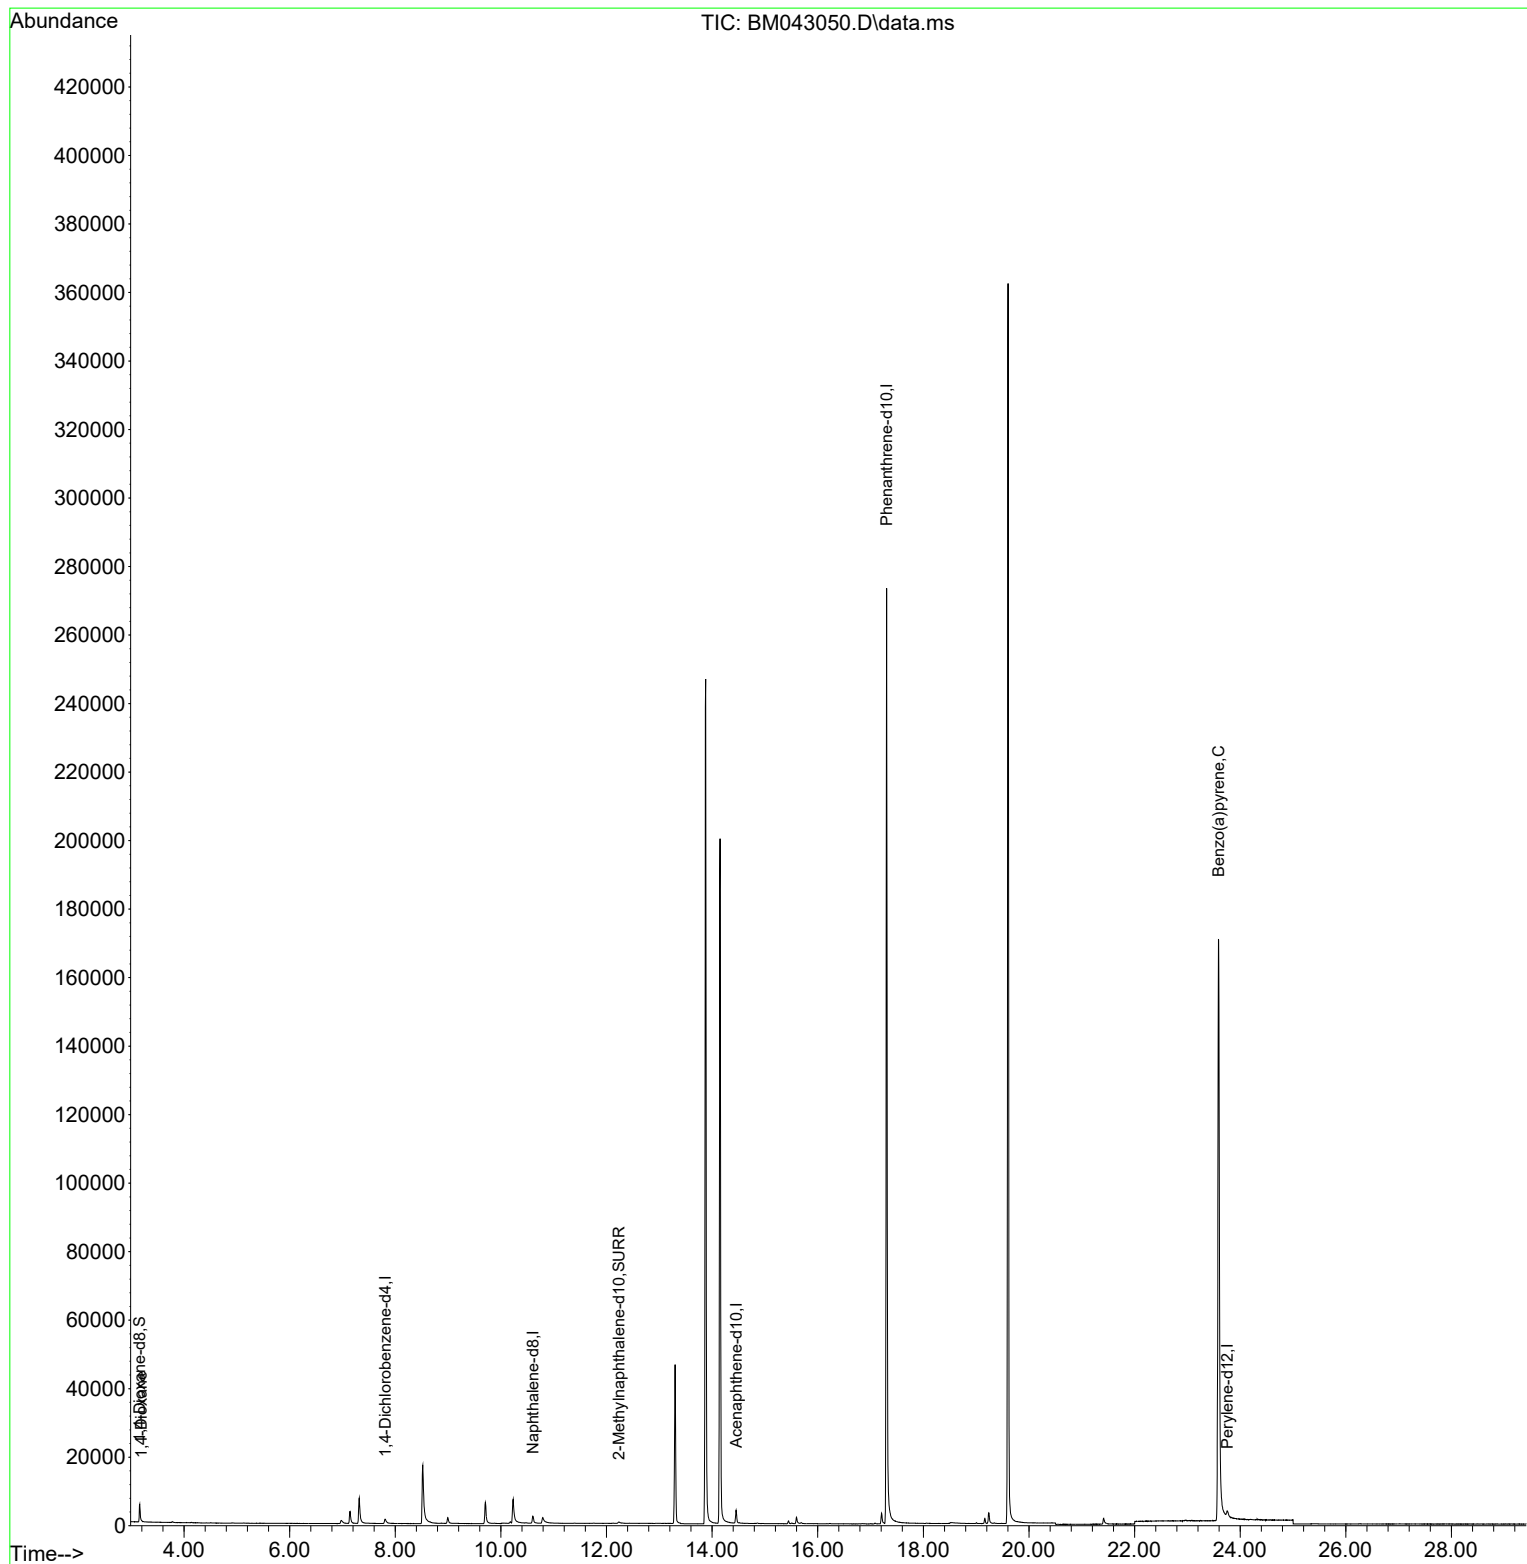


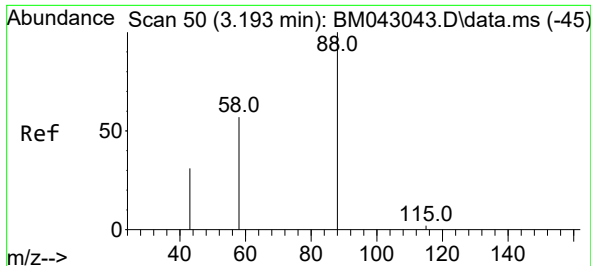

#2
1,4-Dioxane
Concen: 0.030 ng/ul
RT: 3.193 min Scan# 50
Delta R.T. -0.012 min
Lab File: BM043050.D
Acq: 27 Nov 2023 14:59

Instrument :
BNA_M
ClientSampleId :
DCKS7

Tgt Ion: 88 Resp: 49
Ion Ratio Lower Upper
88 100
43 26.5 22.8 34.2
58 13.4 26.8 40.2#

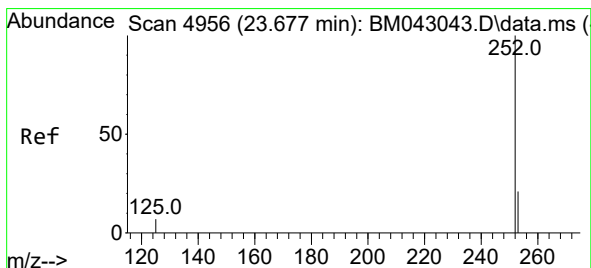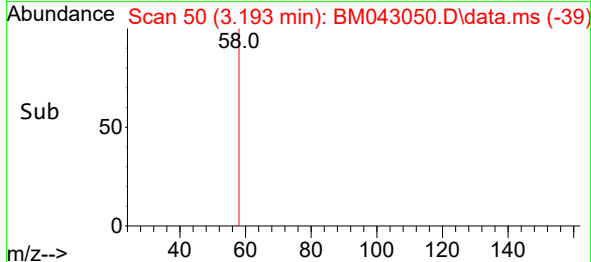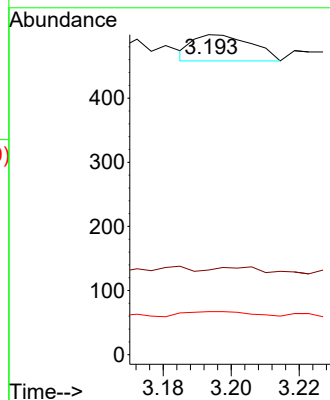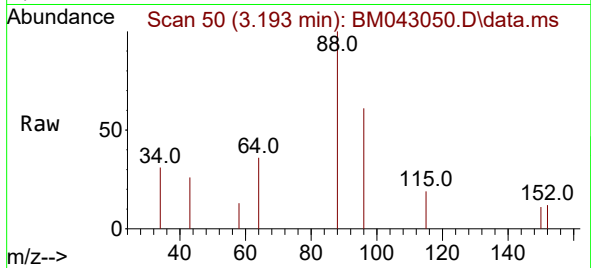

#26
Benzo(a)pyrene
Concen: 0.059 ng/ul
RT: 23.589 min Scan# 4926
Delta R.T. -0.096 min
Lab File: BM043050.D
Acq: 27 Nov 2023 14:59

Tgt Ion: 252 Resp: 1234
Ion Ratio Lower Upper
252 100
253 66.8 36.6 55.0#
125 42.3 16.2 24.4#

