

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112723\
 Data File : BM043052.D
 Acq On : 27 Nov 2023 16:59
 Operator : MA/JU
 Sample : PB157100BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK100

Quant Time: Nov 28 00:22:46 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 27 02:36:19 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.805	152	1002	0.400	ng/ul	#-0.08
4) Naphthalene-d8	10.606	136	3567	0.400	ng/ul	#-0.04
9) Acenaphthene-d10	14.451	164	2036	0.400	ng/ul	-0.02
13) Phenanthrene-d10	17.302	188	333268	0.400	ng/ul	# 0.06
17) Chrysene-d12	21.429	240	2454	0.400	ng/ul	0.00
23) Perylene-d12	0.000	264	0	0.000	ng/ul	-23.78
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.155	96	5842	3.800	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.245	152	1125	0.236	ng/ul	0.00
18) Fluoranthene-d10	19.244	212	2774	0.310	ng/ul	-0.02
Target Compounds						
20) Pyrene	19.601	202	659	0.045	ng/ul#	Qvalue 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112723\
Data File : BM043052.D
Acq On : 27 Nov 2023 16:59
Operator : MA/JU
Sample : PB157100BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK100

Quant Time: Nov 28 00:22:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 27 02:36:19 2023
Response via : Initial Calibration

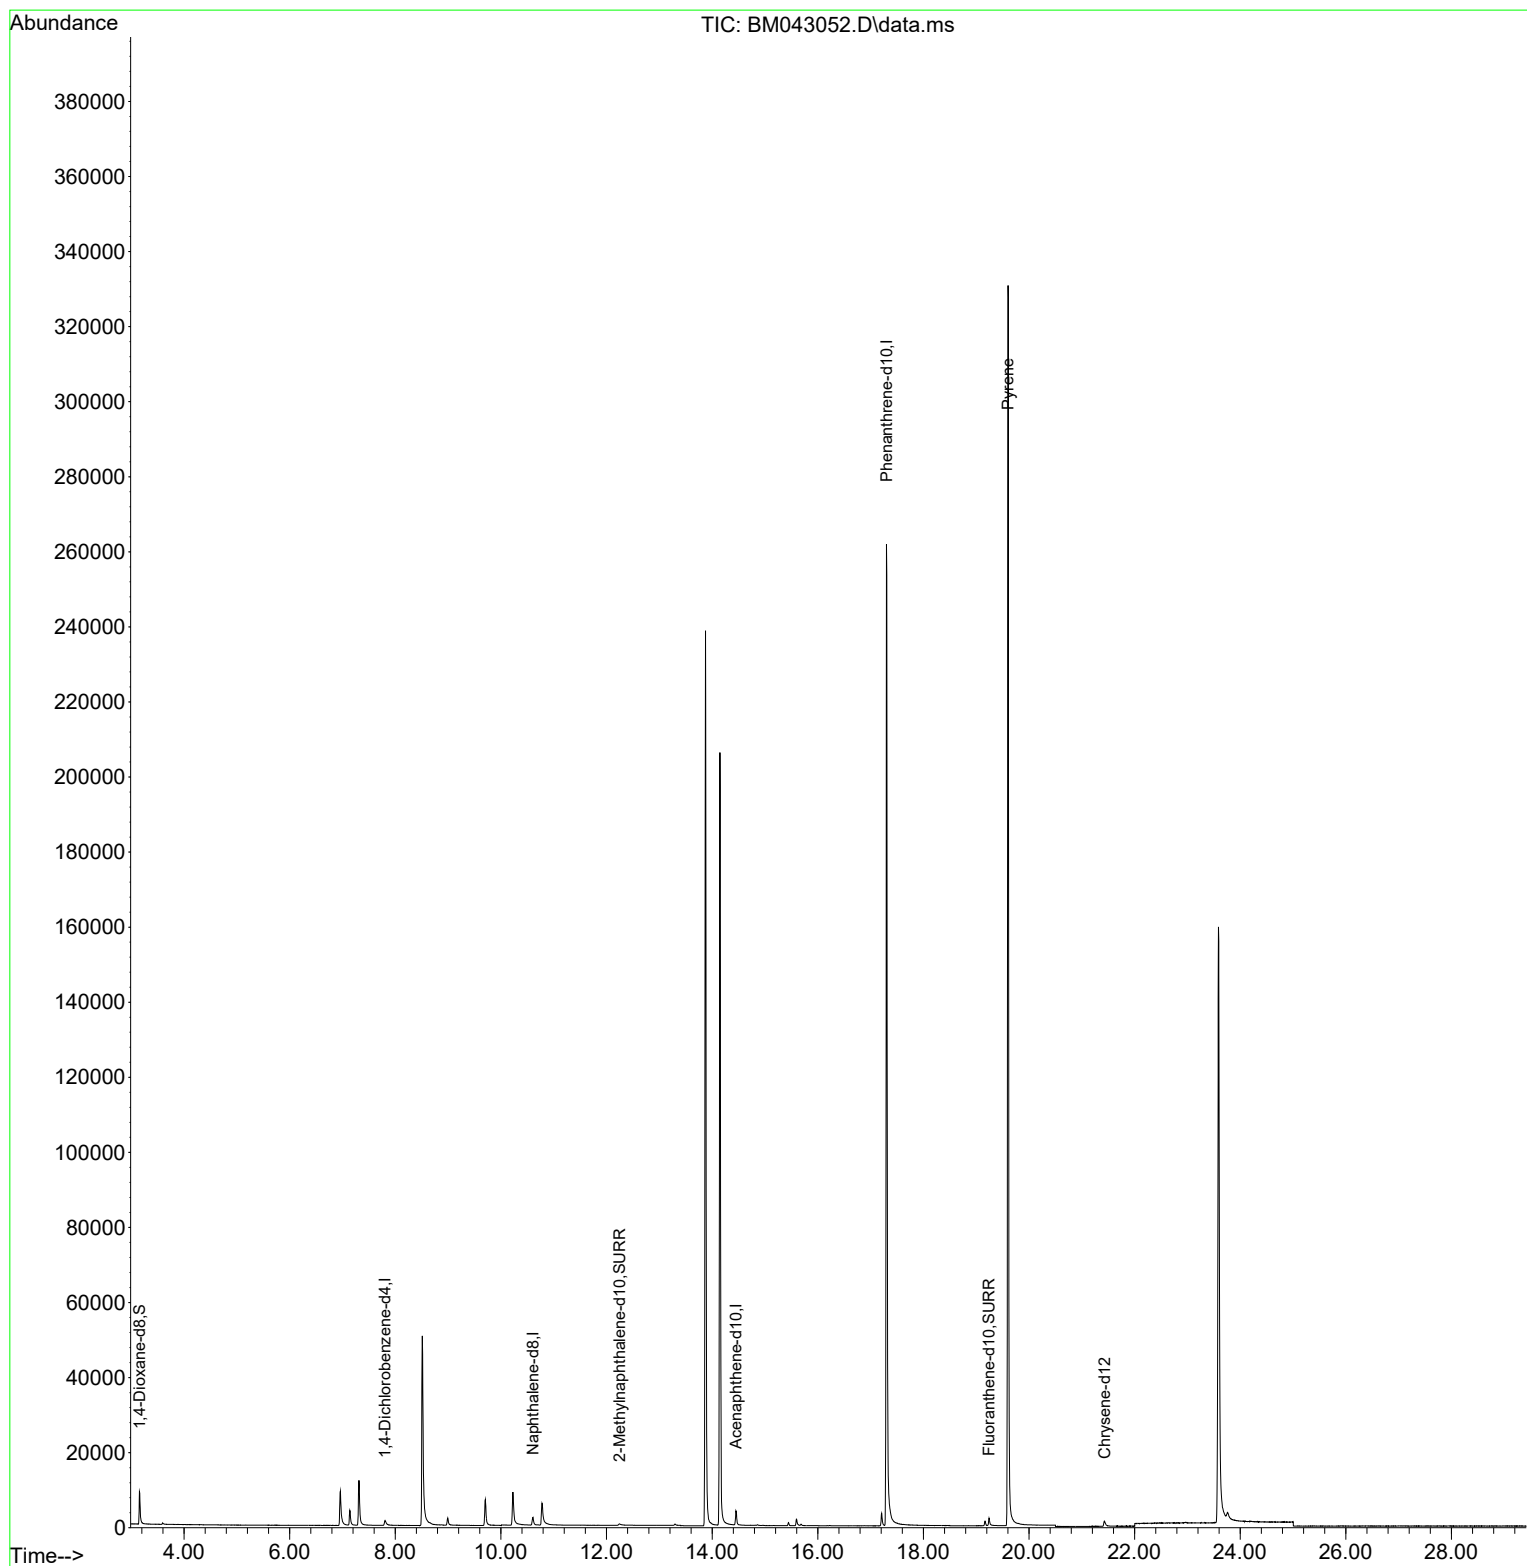

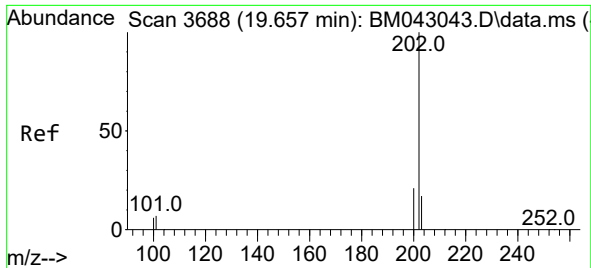

#20
 Pyrene
 Concen: 0.045 ng/ul
 RT: 19.601 min Scan# 30
 Delta R.T. -0.059 min
 Lab File: BM043052.D
 Acq: 27 Nov 2023 16:59

Instrument :
 BNA_M
 ClientSampleId :
 SBLK100

Tgt Ion:202 Resp: 659
 Ion Ratio Lower Upper
 202 100
 101 188.4 8.7 13.1#
 100 1501.1 7.8 11.8#

