

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM112723\  
 Data File : BM043058.D  
 Acq On : 27 Nov 2023 20:37  
 Operator : MA/JU  
 Sample : PB157100BS  
 Misc :  
 ALS Vial : 16 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 SLCS100

Quant Time: Nov 28 00:23:34 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-SIM-BM112423.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Mon Nov 27 02:36:19 2023  
 Response via : Initial Calibration


| Compound                    | R.T.   | QIon | Response | Conc  | Units  | Dev(Min) |
|-----------------------------|--------|------|----------|-------|--------|----------|
| Internal Standards          |        |      |          |       |        |          |
| 1) 1,4-Dichlorobenzene-d4   | 7.876  | 152  | 656      | 0.400 | ng/ul  | 0.00     |
| 4) Naphthalene-d8           | 10.638 | 136  | 2525     | 0.400 | ng/ul  | -0.01    |
| 9) Acenaphthene-d10         | 14.459 | 164  | 1510     | 0.400 | ng/ul  | 0.00     |
| 13) Phenanthrene-d10        | 17.229 | 188  | 3128     | 0.400 | ng/ul  | 0.00     |
| 17) Chrysene-d12            | 21.415 | 240  | 1672     | 0.400 | ng/ul  | 0.00     |
| 23) Perylene-d12            | 23.771 | 264  | 2006     | 0.400 | ng/ul  | 0.00     |
| System Monitoring Compounds |        |      |          |       |        |          |
| 3) 1,4-Dioxane-d8           | 3.164  | 96   | 736      | 0.731 | ng/ul  | 0.00     |
| 6) 2-Methylnaphthalene-d10  | 12.239 | 152  | 1096     | 0.324 | ng/ul  | -0.01    |
| 18) Fluoranthene-d10        | 19.257 | 212  | 2160     | 0.355 | ng/ul  | 0.00     |
| Target Compounds            |        |      |          |       |        |          |
|                             |        |      |          |       | Qvalue |          |
| 2) 1,4-Dioxane              | 3.198  | 88   | 2029     | 1.877 | ng/ul# | 86       |
| 5) Naphthalene              | 10.693 | 128  | 1978     | 0.288 | ng/ul  | 98       |
| 7) 2-Methylnaphthalene      | 12.321 | 142  | 1190     | 0.294 | ng/ul  | 100      |
| 8) 1-Methylnaphthalene      | 12.519 | 142  | 1273     | 0.282 | ng/ul  | 98       |
| 10) Acenaphthylene          | 14.196 | 152  | 2238     | 0.290 | ng/ul  | 98       |
| 11) Acenaphthene            | 14.524 | 153  | 1732     | 0.297 | ng/ul  | 96       |
| 12) Fluorene                | 15.533 | 166  | 1800     | 0.300 | ng/ul  | 96       |
| 14) Pentachlorophenol       | 16.891 | 266  | 478      | 0.565 | ng/ul  | 94       |
| 15) Phenanthrene            | 17.271 | 178  | 2577     | 0.289 | ng/ul  | 99       |
| 16) Anthracene              | 17.385 | 178  | 2451     | 0.290 | ng/ul  | 98       |
| 19) Fluoranthene            | 19.289 | 202  | 3122     | 0.329 | ng/ul  | 99       |
| 20) Pyrene                  | 19.656 | 202  | 3286     | 0.326 | ng/ul  | 99       |
| 21) Benzo(a)anthracene      | 21.409 | 228  | 1763     | 0.325 | ng/ul  | 98       |
| 22) Chrysene                | 21.453 | 228  | 3122     | 0.309 | ng/ul  | 100      |
| 24) Benzo(b)fluoranthene    | 23.046 | 252  | 2272     | 0.336 | ng/ul  | 98       |
| 25) Benzo(k)fluoranthene    | 23.095 | 252  | 3180     | 0.341 | ng/ul  | 96       |
| 26) Benzo(a)pyrene          | 23.674 | 252  | 2407     | 0.326 | ng/ul  | 97       |
| 27) Indeno(1,2,3-cd)pyrene  | 26.235 | 276  | 3310     | 0.331 | ng/ul# | 100      |
| 28) Dibenzo(a,h)anthracene  | 26.252 | 278  | 2603     | 0.337 | ng/ul  | 100      |
| 29) Benzo(g,h,i)perylene    | 26.997 | 276  | 3255     | 0.335 | ng/ul  | 99       |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM112723\  
Data File : BM043058.D  
Acq On : 27 Nov 2023 20:37  
Operator : MA/JU  
Sample : PB157100BS  
Misc :  
ALS Vial : 16 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
SLCS100

Quant Time: Nov 28 00:23:34 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-SIM-BM112423.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Nov 27 02:36:19 2023  
Response via : Initial Calibration




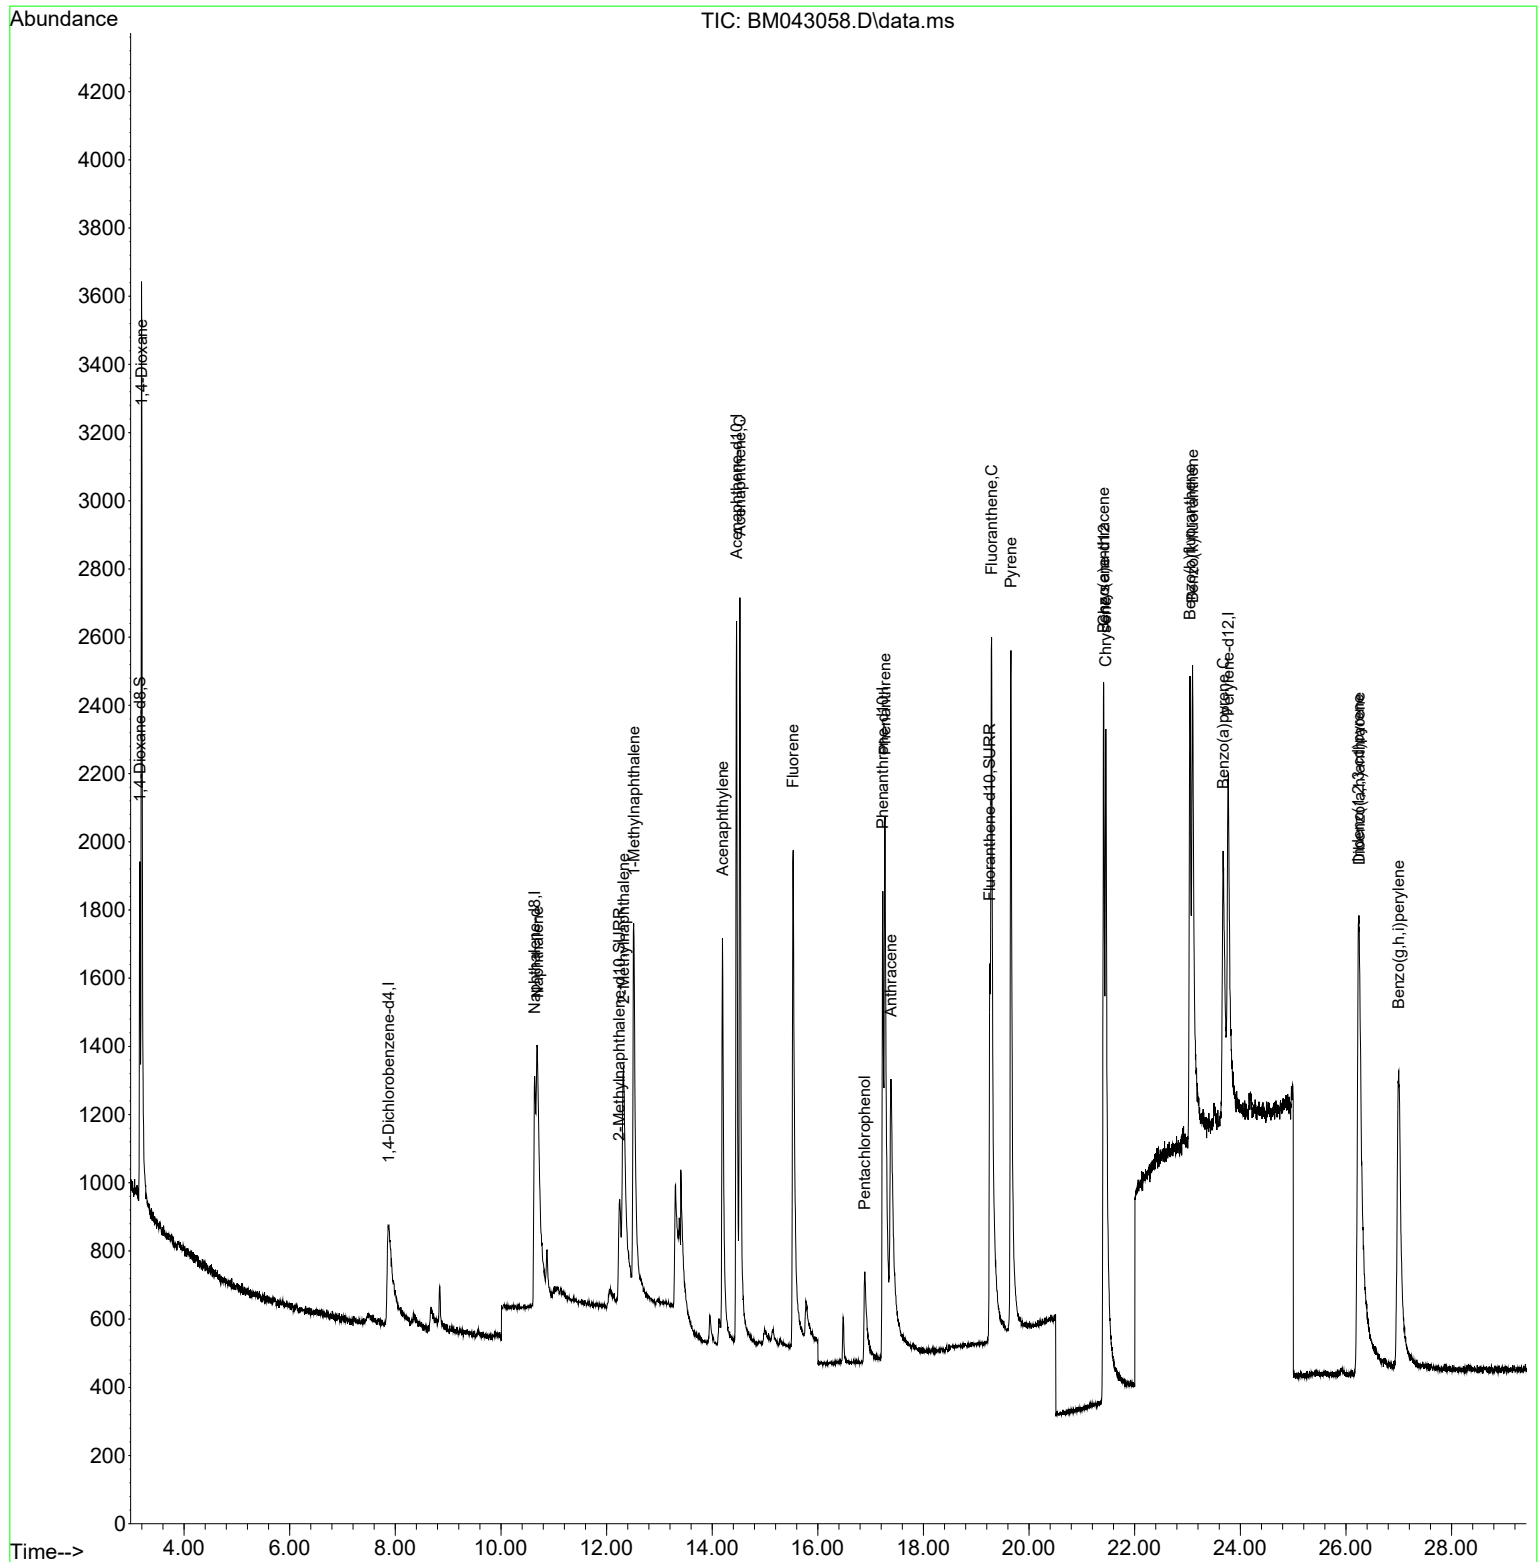


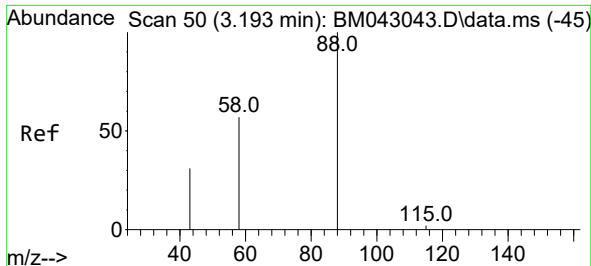

#2  
1,4-Dioxane  
Concen: 1.877 ng/ul  
RT: 3.198 min Scan# 51  
Delta R.T. -0.008 min  
Lab File: BM043058.D  
Acq: 27 Nov 2023 20:37




Instrument :  
BNA\_M  
ClientSampleId :  
SLCS100


Tgt Ion: 88 Resp: 2029  
Ion Ratio Lower Upper  
88 100  
43 28.5 22.8 34.2  
58 48.4 26.8 40.2#

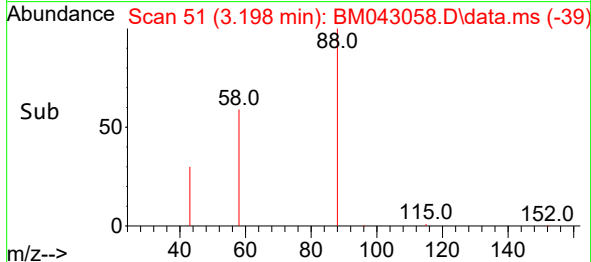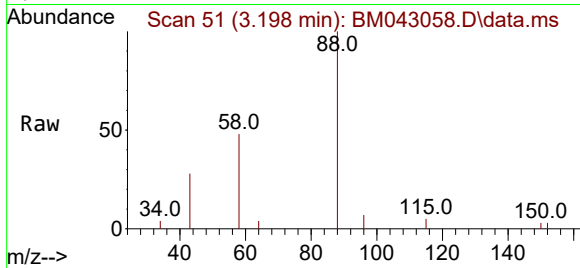

#5  
Naphthalene  
Concen: 0.288 ng/ul  
RT: 10.693 min Scan# 1793  
Delta R.T. -0.005 min  
Lab File: BM043058.D  
Acq: 27 Nov 2023 20:37

Tgt Ion: 128 Resp: 1978  
Ion Ratio Lower Upper  
128 100  
129 19.2 16.0 24.0  
127 21.9 16.5 24.7


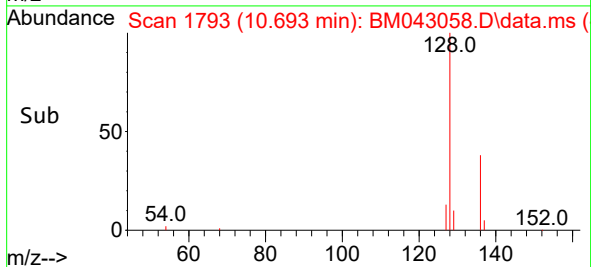

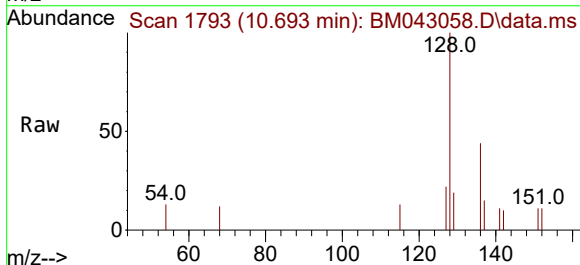




#7  
2-Methylnaphthalene  
Concen: 0.294 ng/ul  
RT: 12.321 min Scan# 2087  
Delta R.T. -0.011 min  
Lab File: BM043058.D  
Acq: 27 Nov 2023 20:37




Instrument :  
BNA\_M  
ClientSampleId :  
SLCS100


Tgt Ion:142 Resp: 1190  
Ion Ratio Lower Upper  
142 100  
141 95.1 76.1 114.1

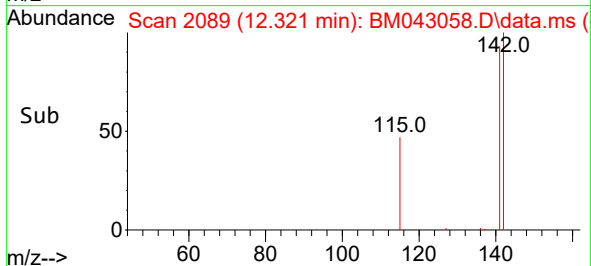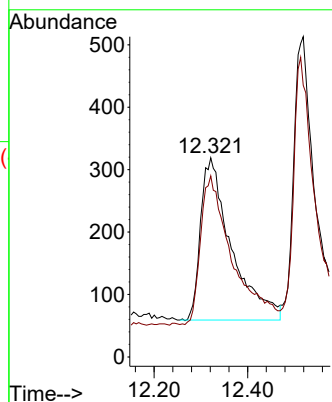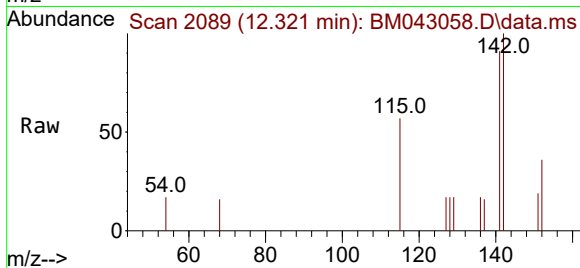

#8  
1-Methylnaphthalene  
Concen: 0.282 ng/ul  
RT: 12.519 min Scan# 2125  
Delta R.T. 0.000 min  
Lab File: BM043058.D  
Acq: 27 Nov 2023 20:37

Tgt Ion:142 Resp: 1273  
Ion Ratio Lower Upper  
142 100  
141 94.7 73.8 110.8


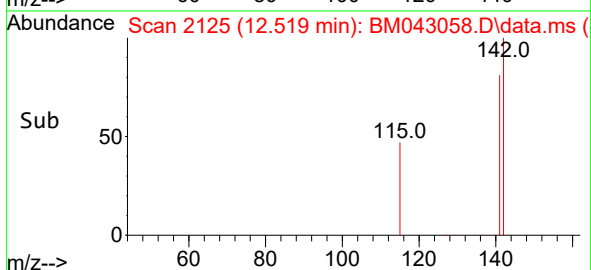

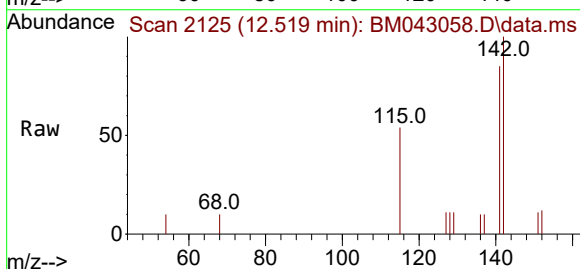


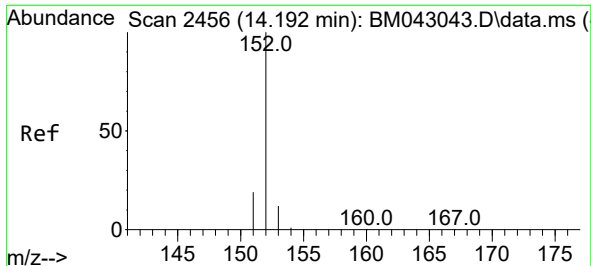

#10  
Acenaphthylene  
Concen: 0.290 ng/ul  
RT: 14.196 min Scan# 2456  
Delta R.T. -0.009 min  
Lab File: BM043058.D  
Acq: 27 Nov 2023 20:37




Instrument :  
BNA\_M  
ClientSampleId :  
SLCS100


Tgt Ion:152 Resp: 2238  
Ion Ratio Lower Upper  
152 100  
151 25.6 19.4 29.0  
153 18.4 14.6 21.8

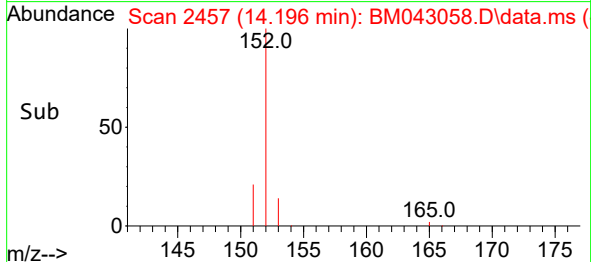

#11  
Acenaphthene  
Concen: 0.297 ng/ul  
RT: 14.524 min Scan# 2528  
Delta R.T. -0.009 min  
Lab File: BM043058.D  
Acq: 27 Nov 2023 20:37

Tgt Ion:153 Resp: 1732  
Ion Ratio Lower Upper  
153 100  
152 53.4 43.9 65.9  
154 82.8 70.6 105.8


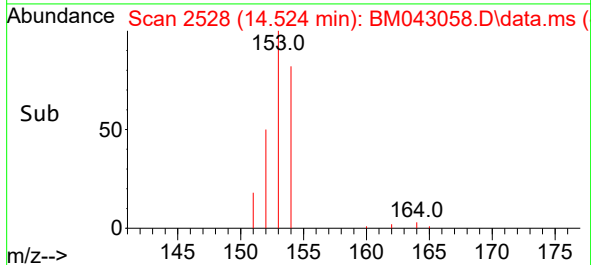

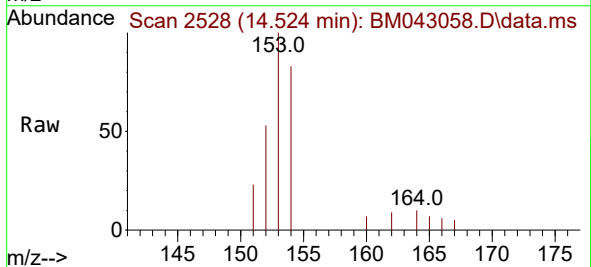


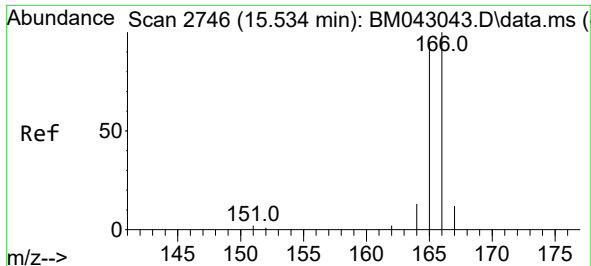

#12  
 Fluorene  
 Concen: 0.300 ng/ul  
 RT: 15.533 min Scan# 21  
 Delta R.T. -0.004 min  
 Lab File: BM043058.D  
 Acq: 27 Nov 2023 20:37




Instrument :  
 BNA\_M  
 ClientSampleId :  
 SLCS100


Tgt Ion:166 Resp: 1800  
 Ion Ratio Lower Upper  
 166 100  
 165 104.1 79.9 119.9  
 167 19.8 14.2 21.4

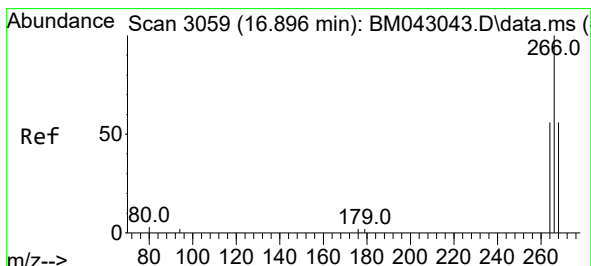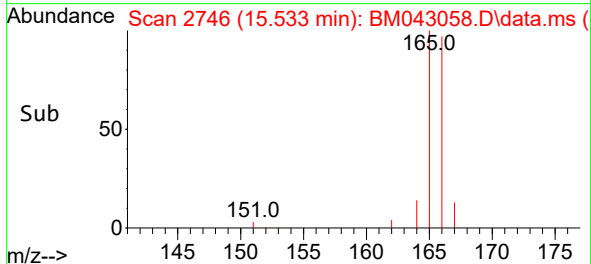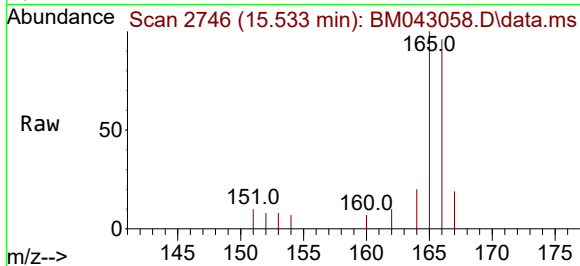

#14  
 Pentachlorophenol  
 Concen: 0.565 ng/ul  
 RT: 16.891 min Scan# 3058  
 Delta R.T. -0.021 min  
 Lab File: BM043058.D  
 Acq: 27 Nov 2023 20:37

Tgt Ion:266 Resp: 478  
 Ion Ratio Lower Upper  
 266 100  
 264 55.0 48.8 73.2  
 268 60.9 51.8 77.6


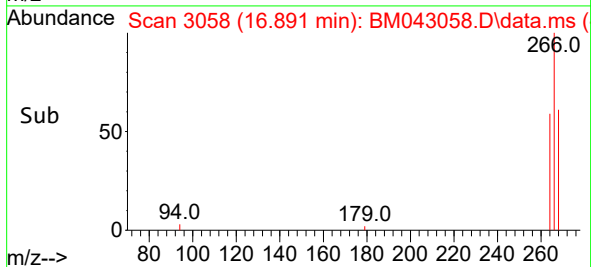

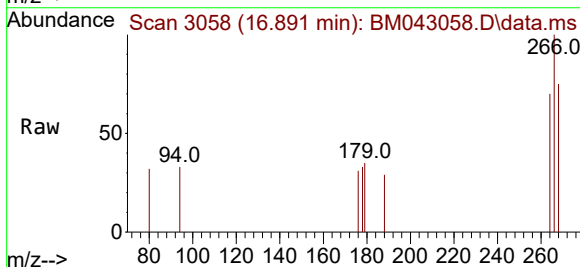


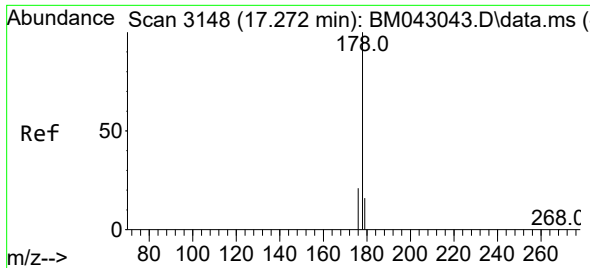

#15  
Phenanthrene  
Concen: 0.289 ng/ul  
RT: 17.271 min Scan# 3148  
Delta R.T. -0.008 min  
Lab File: BM043058.D  
Acq: 27 Nov 2023 20:37




Instrument :  
BNA\_M  
ClientSampleId :  
SLCS100


|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 178   | Resp: | 2577  |
| Ion      | Ratio | Lower | Upper |
| 178      | 100   |       |       |
| 179      | 19.7  | 15.7  | 23.5  |
| 176      | 24.3  | 18.9  | 28.3  |

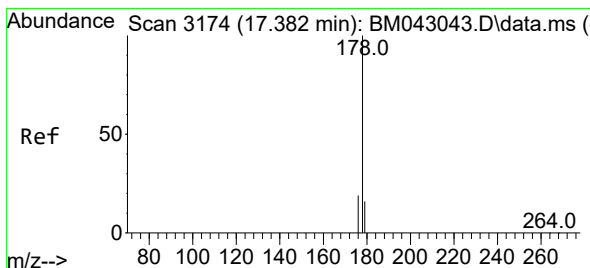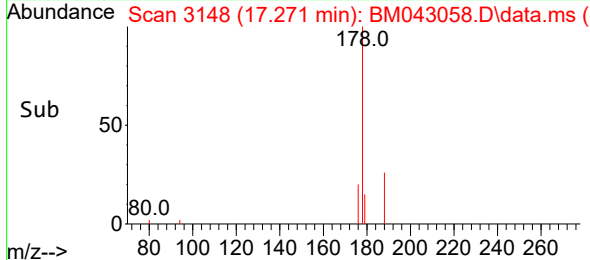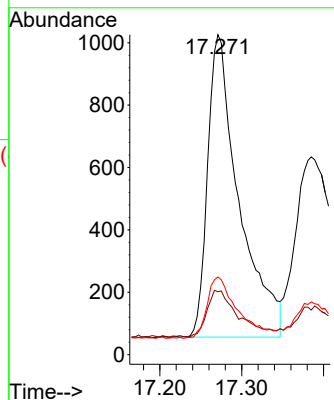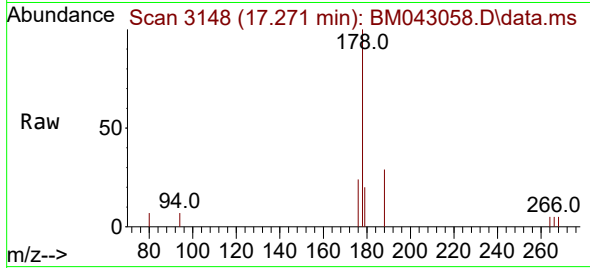

#16  
Anthracene  
Concen: 0.290 ng/ul  
RT: 17.385 min Scan# 3175  
Delta R.T. -0.008 min  
Lab File: BM043058.D  
Acq: 27 Nov 2023 20:37

|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 178   | Resp: | 2451  |
| Ion      | Ratio | Lower | Upper |
| 178      | 100   |       |       |
| 179      | 22.6  | 17.3  | 25.9  |
| 176      | 26.7  | 20.5  | 30.7  |


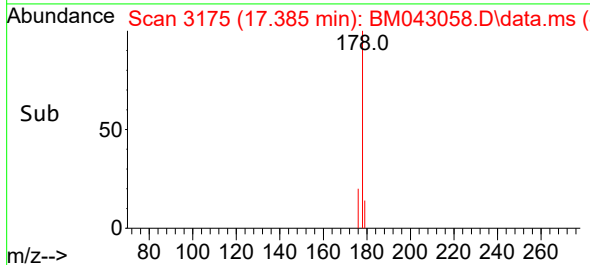
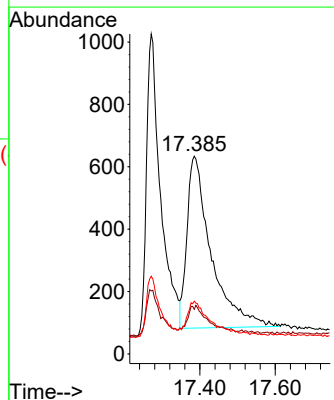
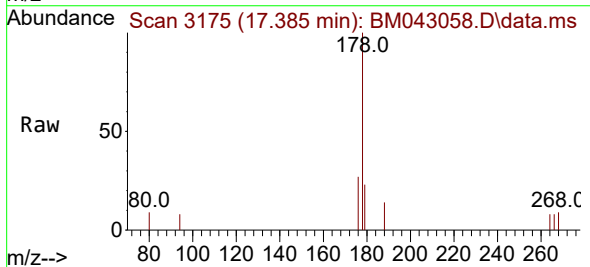


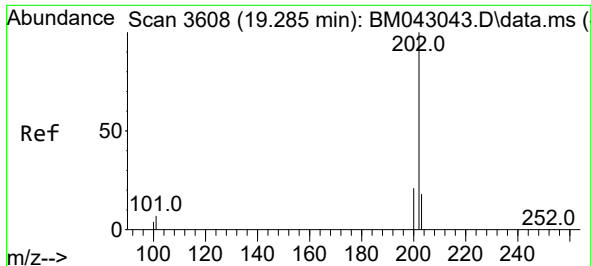

#19  
Fluoranthene  
Concen: 0.329 ng/ul  
RT: 19.289 min Scan# 3609  
Delta R.T. -0.004 min  
Lab File: BM043058.D  
Acq: 27 Nov 2023 20:37




Instrument :  
BNA\_M  
ClientSampleId :  
SLCS100

Tgt Ion:202 Resp: 3122  
Ion Ratio Lower Upper  
202 100  
101 10.1 7.8 11.8  
100 9.5 7.1 10.7

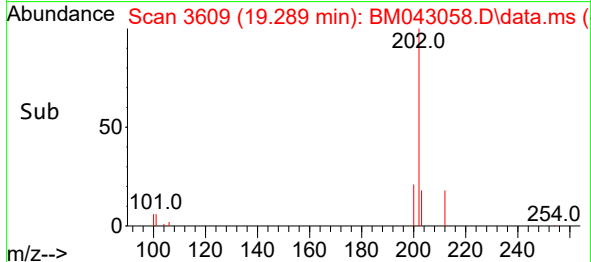


#20  
Pyrene  
Concen: 0.326 ng/ul  
RT: 19.656 min Scan# 3688  
Delta R.T. -0.004 min  
Lab File: BM043058.D  
Acq: 27 Nov 2023 20:37

Tgt Ion:202 Resp: 3286  
Ion Ratio Lower Upper  
202 100  
101 10.7 8.7 13.1  
100 10.3 7.8 11.8

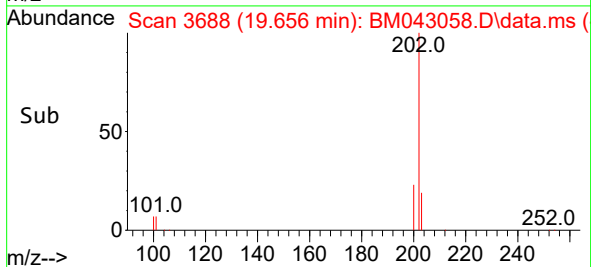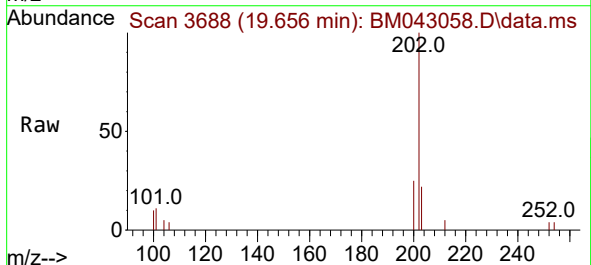





#21

Benzo(a)anthracene

Concen: 0.325 ng/ul

RT: 21.409 min Scan# 4181

Delta R.T. -0.003 min

Lab File: BM043058.D

Acq: 27 Nov 2023 20:37

Instrument :

BNA\_M

ClientSampleId :

SLCS100





Tgt Ion:228 Resp: 1763

Ion Ratio Lower Upper

228 100

229 24.6 19.4 29.0

226 33.0 24.9 37.3

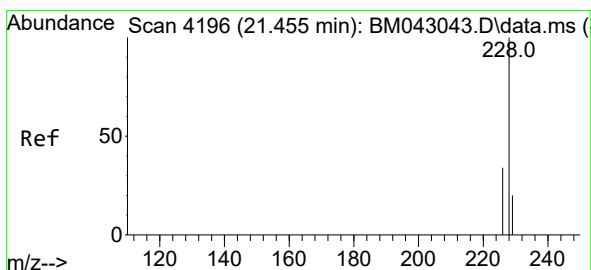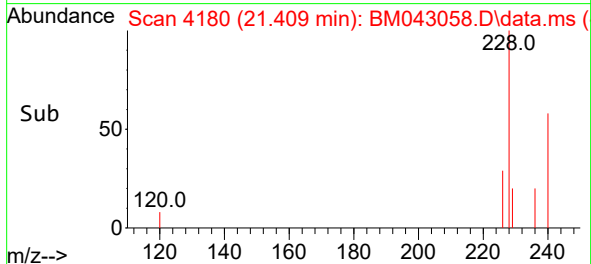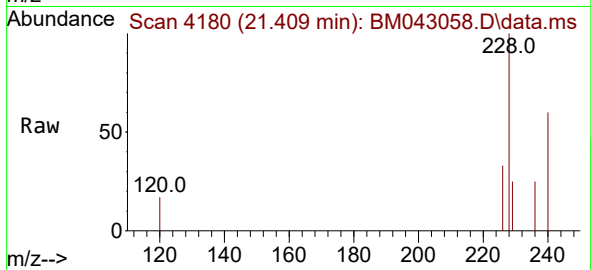

#22

Chrysene

Concen: 0.309 ng/ul

RT: 21.453 min Scan# 4195

Delta R.T. -0.006 min

Lab File: BM043058.D

Acq: 27 Nov 2023 20:37




Tgt Ion:228 Resp: 3122


Ion Ratio Lower Upper

228 100

226 34.3 27.2 40.8

229 22.6 18.0 27.0




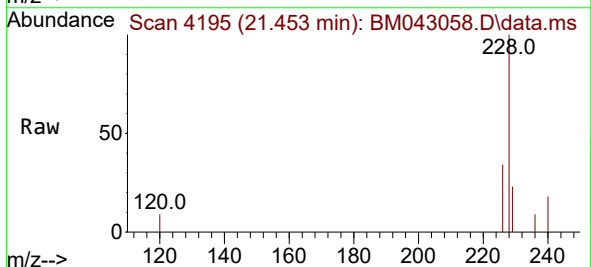


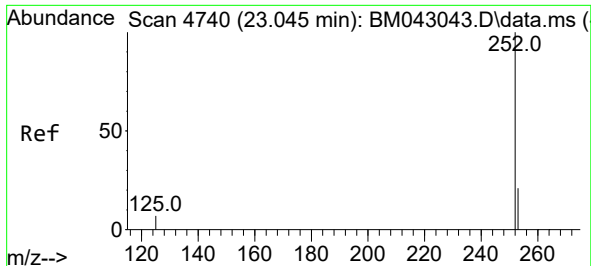

#24  
Benzo(b)fluoranthene  
Concen: 0.336 ng/ul  
RT: 23.046 min Scan# 4740  
Delta R.T. -0.006 min  
Lab File: BM043058.D  
Acq: 27 Nov 2023 20:37




Instrument :  
BNA\_M  
ClientSampleId :  
SLCS100


Tgt Ion:252 Resp: 2272  
Ion Ratio Lower Upper  
252 100  
253 34.4 0.0 71.8  
125 14.5 0.0 29.0

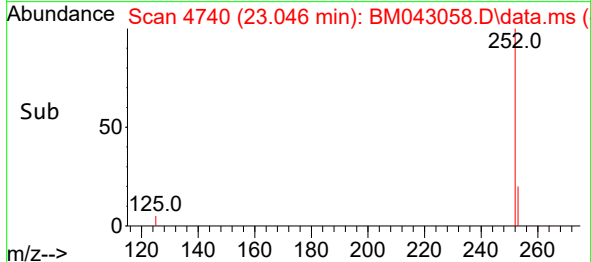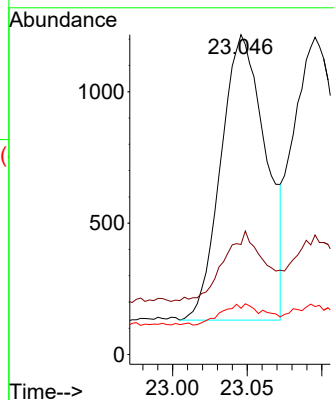

#25  
Benzo(k)fluoranthene  
Concen: 0.341 ng/ul  
RT: 23.095 min Scan# 4757  
Delta R.T. -0.003 min  
Lab File: BM043058.D  
Acq: 27 Nov 2023 20:37

Tgt Ion:252 Resp: 3180  
Ion Ratio Lower Upper  
252 100  
253 37.7 28.2 42.2  
125 15.2 11.0 16.6


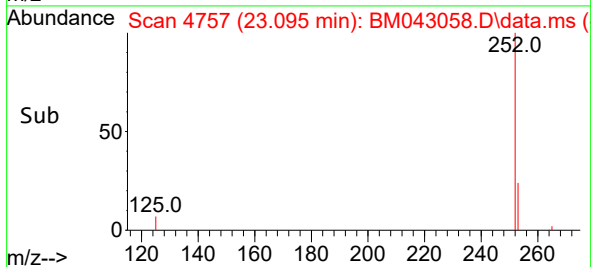
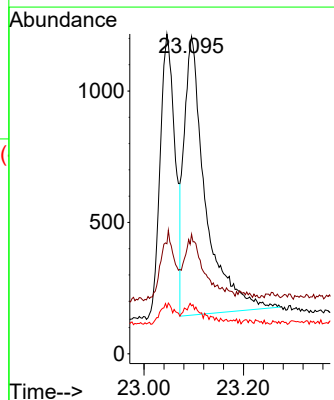
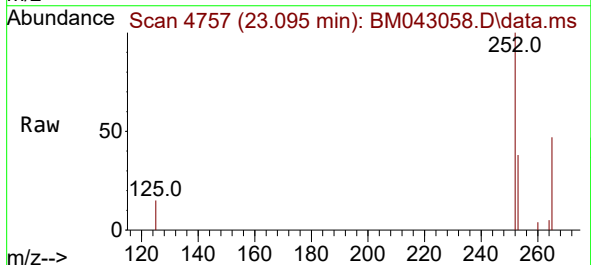


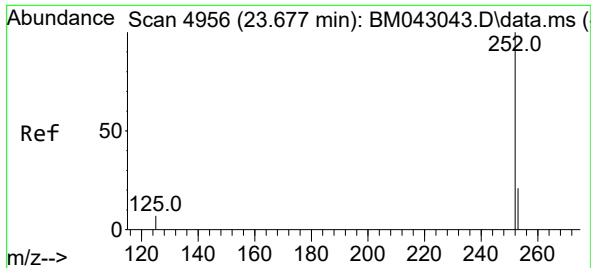

#26  
Benzo(a)pyrene  
Concen: 0.326 ng/ul  
RT: 23.674 min Scan# 4955  
Delta R.T. -0.011 min  
Lab File: BM043058.D  
Acq: 27 Nov 2023 20:37




Instrument :  
BNA\_M  
ClientSampleId :  
SLCS100


Tgt Ion:252 Resp: 2407  
Ion Ratio Lower Upper  
252 100  
253 46.7 36.6 55.0  
125 23.0 16.2 24.4

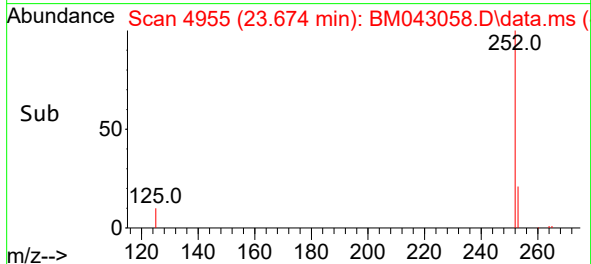

#27  
Indeno(1,2,3-cd)pyrene  
Concen: 0.331 ng/ul  
RT: 26.235 min Scan# 5777  
Delta R.T. -0.003 min  
Lab File: BM043058.D  
Acq: 27 Nov 2023 20:37

Tgt Ion:276 Resp: 3310  
Ion Ratio Lower Upper  
276 100  
138 17.6 0.0 0.0#  
227 0.2 0.2 0.2#


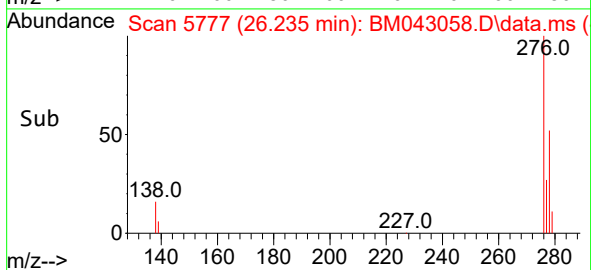

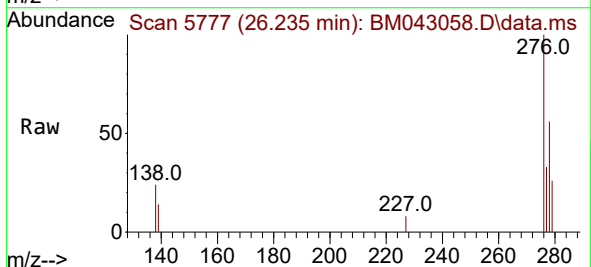


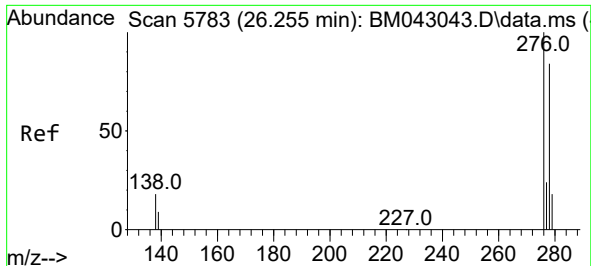

#28  
 Dibenzo(a,h)anthracene  
 Concen: 0.337 ng/ul  
 RT: 26.252 min Scan# 51  
 Delta R.T. -0.023 min  
 Lab File: BM043058.D  
 Acq: 27 Nov 2023 20:37

Instrument :  
 BNA\_M  
 ClientSampleId :  
 SLCS100

|           |       |       |      |
|-----------|-------|-------|------|
| Tgt Ion:  | 278   | Resp: | 2603 |
| Ion Ratio | Lower | Upper |      |
| 278       | 100   |       |      |
| 139       | 22.7  | 18.1  | 27.1 |
| 279       | 42.9  | 34.4  | 51.6 |

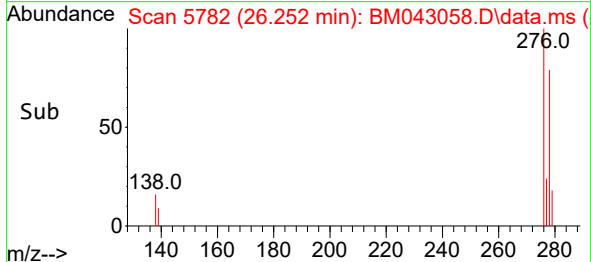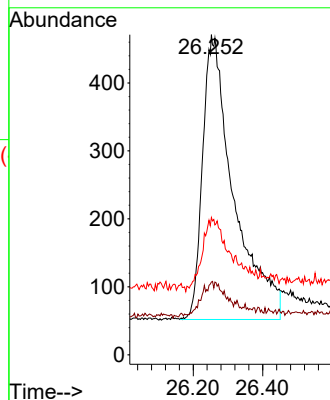

#29  
 Benzo(g,h,i)perylene  
 Concen: 0.335 ng/ul  
 RT: 26.997 min Scan# 6004  
 Delta R.T. -0.013 min  
 Lab File: BM043058.D  
 Acq: 27 Nov 2023 20:37

|           |       |       |      |
|-----------|-------|-------|------|
| Tgt Ion:  | 276   | Resp: | 3255 |
| Ion Ratio | Lower | Upper |      |
| 276       | 100   |       |      |
| 138       | 22.6  | 17.8  | 26.8 |
| 277       | 29.3  | 23.8  | 35.8 |

