

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112822\
 Data File : BM037753.D
 Acq On : 28 Nov 2022 11:03
 Operator : CG/JU
 Sample : PB149209BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK209

Quant Time: Nov 28 22:27:21 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Nov 28 22:24:47 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.110	152	218375	20.000	ng/ul	0.00
20) Naphthalene-d8	10.928	136	1015636	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.733	164	637226	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.468	188	1268388	20.000	ng/ul	0.00
79) Chrysene-d12	21.633	240	1047616	20.000	ng/ul	0.00
88) Perylene-d12	24.127	264	865131	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.434	96	26085	4.954	ng/uL	0.00
4) Pyridine-d5	3.875	84	250515	14.616	ng/ul	0.00
7) Phenol-d5	7.257	99	490561	22.517	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.428	67	341456	23.495	ng/ul	0.00
11) 2-Chlorophenol-d4	7.634	132	368893	24.368	ng/ul	0.00
15) 4-Methylphenol-d8	8.816	113	390588	22.530	ng/ul	0.00
21) Nitrobenzene-d5	9.281	128	200411	25.171	ng/ul	0.00
24) 2-Nitrophenol-d4	10.004	143	202167	25.769	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.545	165	337785	23.527	ng/ul	0.00
31) 4-Chloroaniline-d4	11.063	131	411563	17.275	ng/ul	0.00
46) Dimethylphthalate-d6	14.139	166	1153837	25.563	ng/ul	0.00
49) Acenaphthylene-d8	14.427	160	1324914	24.869	ng/ul	0.00
54) 4-Nitrophenol-d4	14.916	143	198116	19.927	ng/ul	0.00
60) Fluorene-d10	15.721	176	984374	24.902	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.827	200	133211	19.523	ng/ul	0.00
73) Anthracene-d10	17.568	188	1535675	25.890	ng/ul	0.00
81) Pyrene-d10	19.851	212	1588641	29.841	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.962	264	1136202	25.515	ng/ul	0.00
Target Compounds						
48) 2,6-Dinitrotoluene	14.139	165	10118	1.092	ng/ul#	32


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112822\
Data File : BM037753.D
Acq On : 28 Nov 2022 11:03
Operator : CG/JU
Sample : PB149209BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK209


Quant Time: Nov 28 22:27:21 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Nov 28 22:24:47 2022
Response via : Initial Calibration

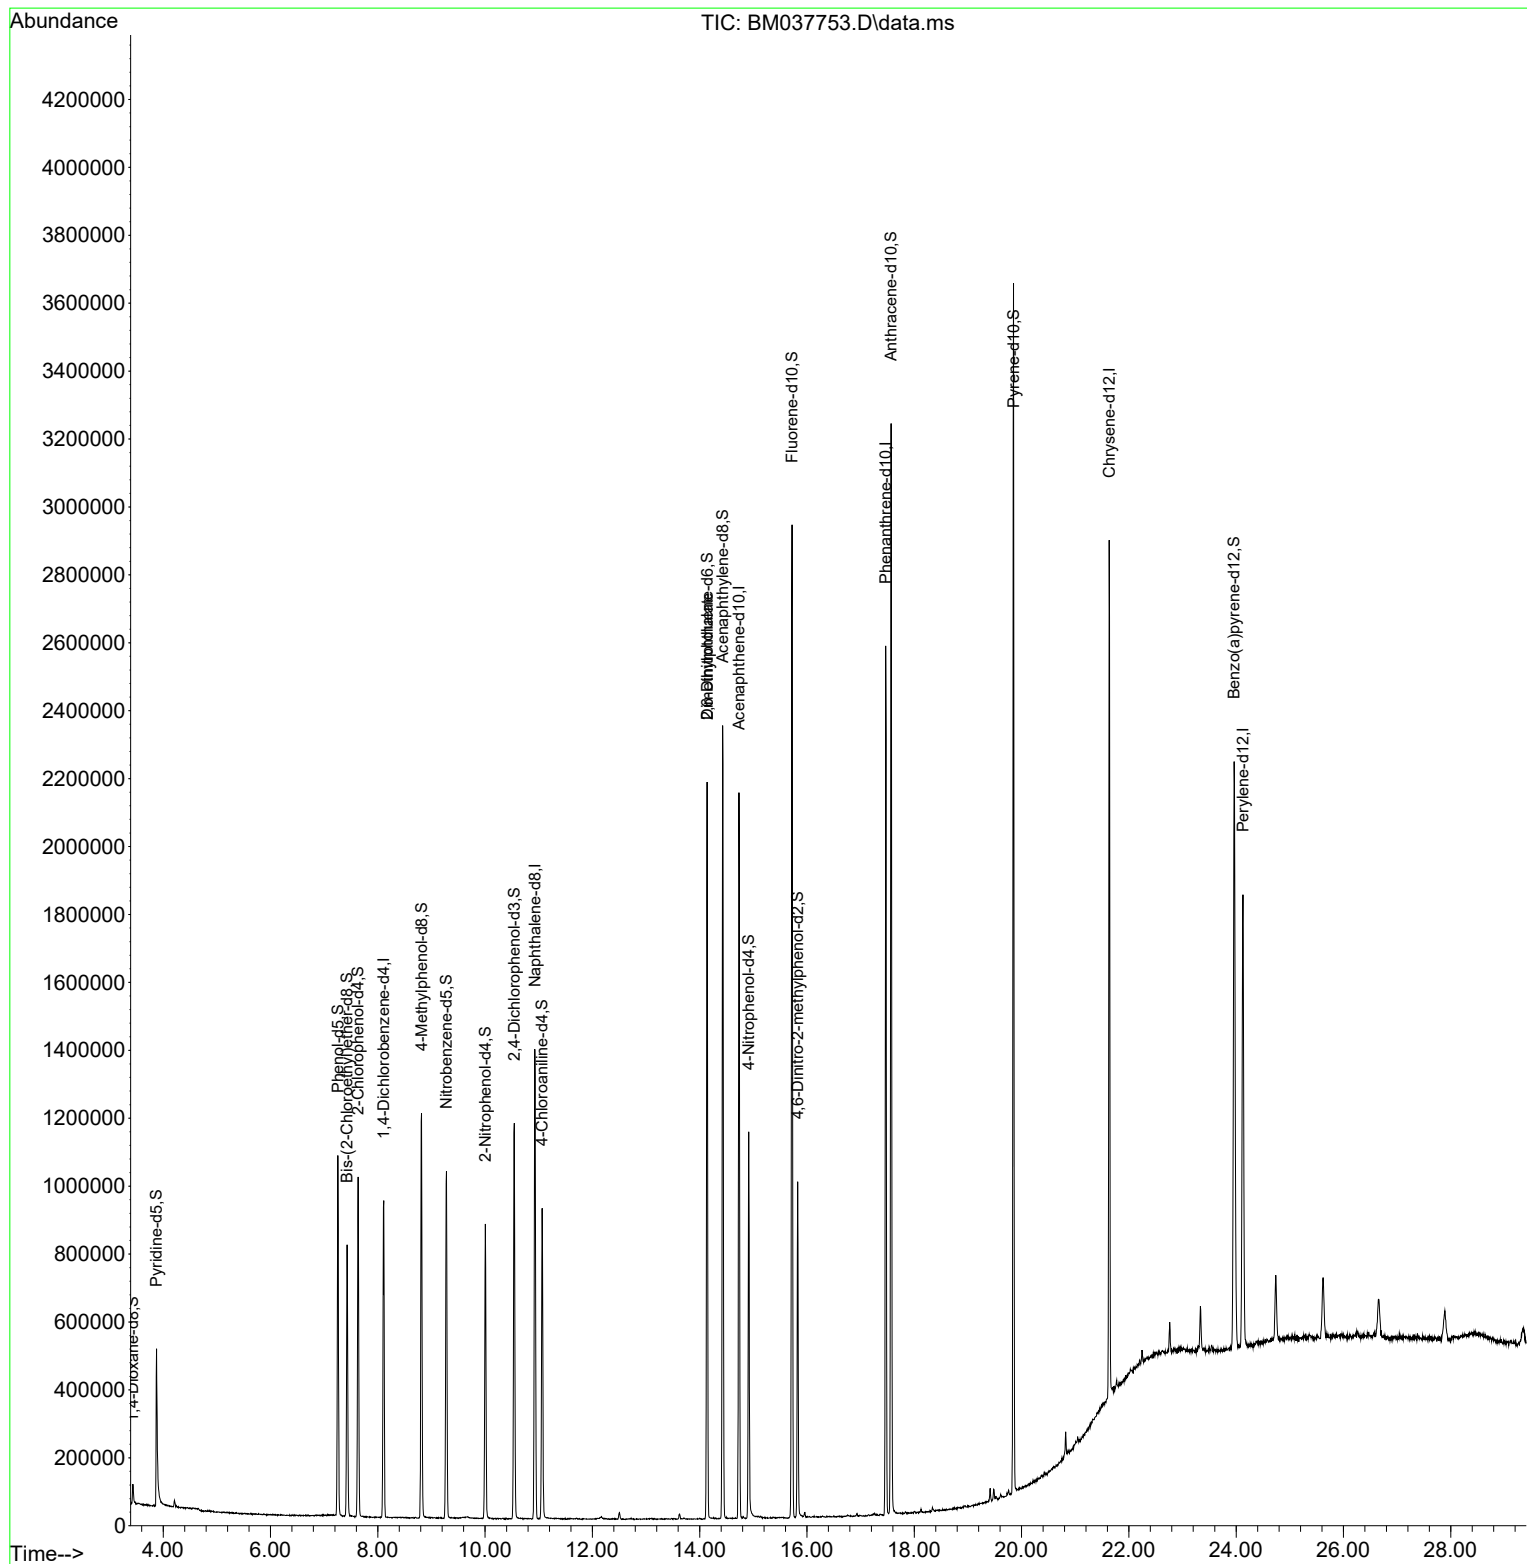

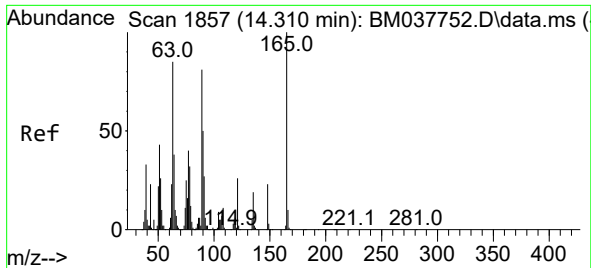

#48
 2,6-Dinitrotoluene
 Concen: 1.092 ng/ul
 RT: 14.139 min Scan# 11
 Delta R.T. -0.170 min
 Lab File: BM037753.D
 Acq: 28 Nov 2022 11:03

Instrument :
 BNA_M
 ClientSampleId :
 SBLK209

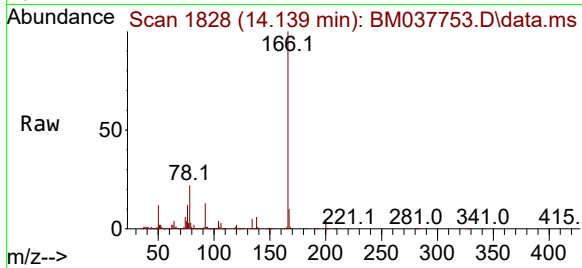

Tgt Ion:165 Resp: 10118
 Ion Ratio Lower Upper
 165 100
 89 3.6 56.4 84.6#
 121 37.4 18.9 28.3#

