

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112822\
 Data File : BM037761.D
 Acq On : 28 Nov 2022 16:01
 Operator : CG/JU
 Sample : N5710-16
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0L02

Quant Time: Nov 28 22:29:11 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Nov 28 22:24:47 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.110	152	221069	20.000	ng/ul	0.00
20) Naphthalene-d8	10.928	136	1040796	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.733	164	693803	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.468	188	1429807	20.000	ng/ul	0.00
79) Chrysene-d12	21.633	240	1292059	20.000	ng/ul	0.00
88) Perylene-d12	24.127	264	1111763	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.434	96	30422	5.707	ng/uL	0.00
4) Pyridine-d5	3.875	84	184490	10.633	ng/ul	0.00
7) Phenol-d5	7.257	99	684732	31.047	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.428	67	461186	31.347	ng/ul	0.00
11) 2-Chlorophenol-d4	7.634	132	520735	33.979	ng/ul	0.00
15) 4-Methylphenol-d8	8.816	113	571764	32.578	ng/ul	0.00
21) Nitrobenzene-d5	9.281	128	292766	35.881	ng/ul	0.00
24) 2-Nitrophenol-d4	10.004	143	315134	39.197	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.545	165	532825	36.215	ng/ul	0.00
31) 4-Chloroaniline-d4	11.063	131	518141	21.223	ng/ul	0.00
46) Dimethylphthalate-d6	14.139	166	1755486	35.722	ng/ul	0.00
49) Acenaphthylene-d8	14.433	160	2090585	36.041	ng/ul	0.00
54) 4-Nitrophenol-d4	14.916	143	322682	29.809	ng/ul	0.00
60) Fluorene-d10	15.722	176	1582357	36.765	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.827	200	218268	28.378	ng/ul	0.00
73) Anthracene-d10	17.568	188	2467211	36.900	ng/ul	0.00
81) Pyrene-d10	19.851	212	2714741	41.346	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.968	264	2120077	37.048	ng/ul	0.00


Target Compounds					Qvalue
17) N-Nitroso-di-n-propyla...	8.816	70	17643	1.042 ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112822\
Data File : BM037761.D
Acq On : 28 Nov 2022 16:01
Operator : CG/JU
Sample : N5710-16
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COL02

Quant Time: Nov 28 22:29:11 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Nov 28 22:24:47 2022
Response via : Initial Calibration

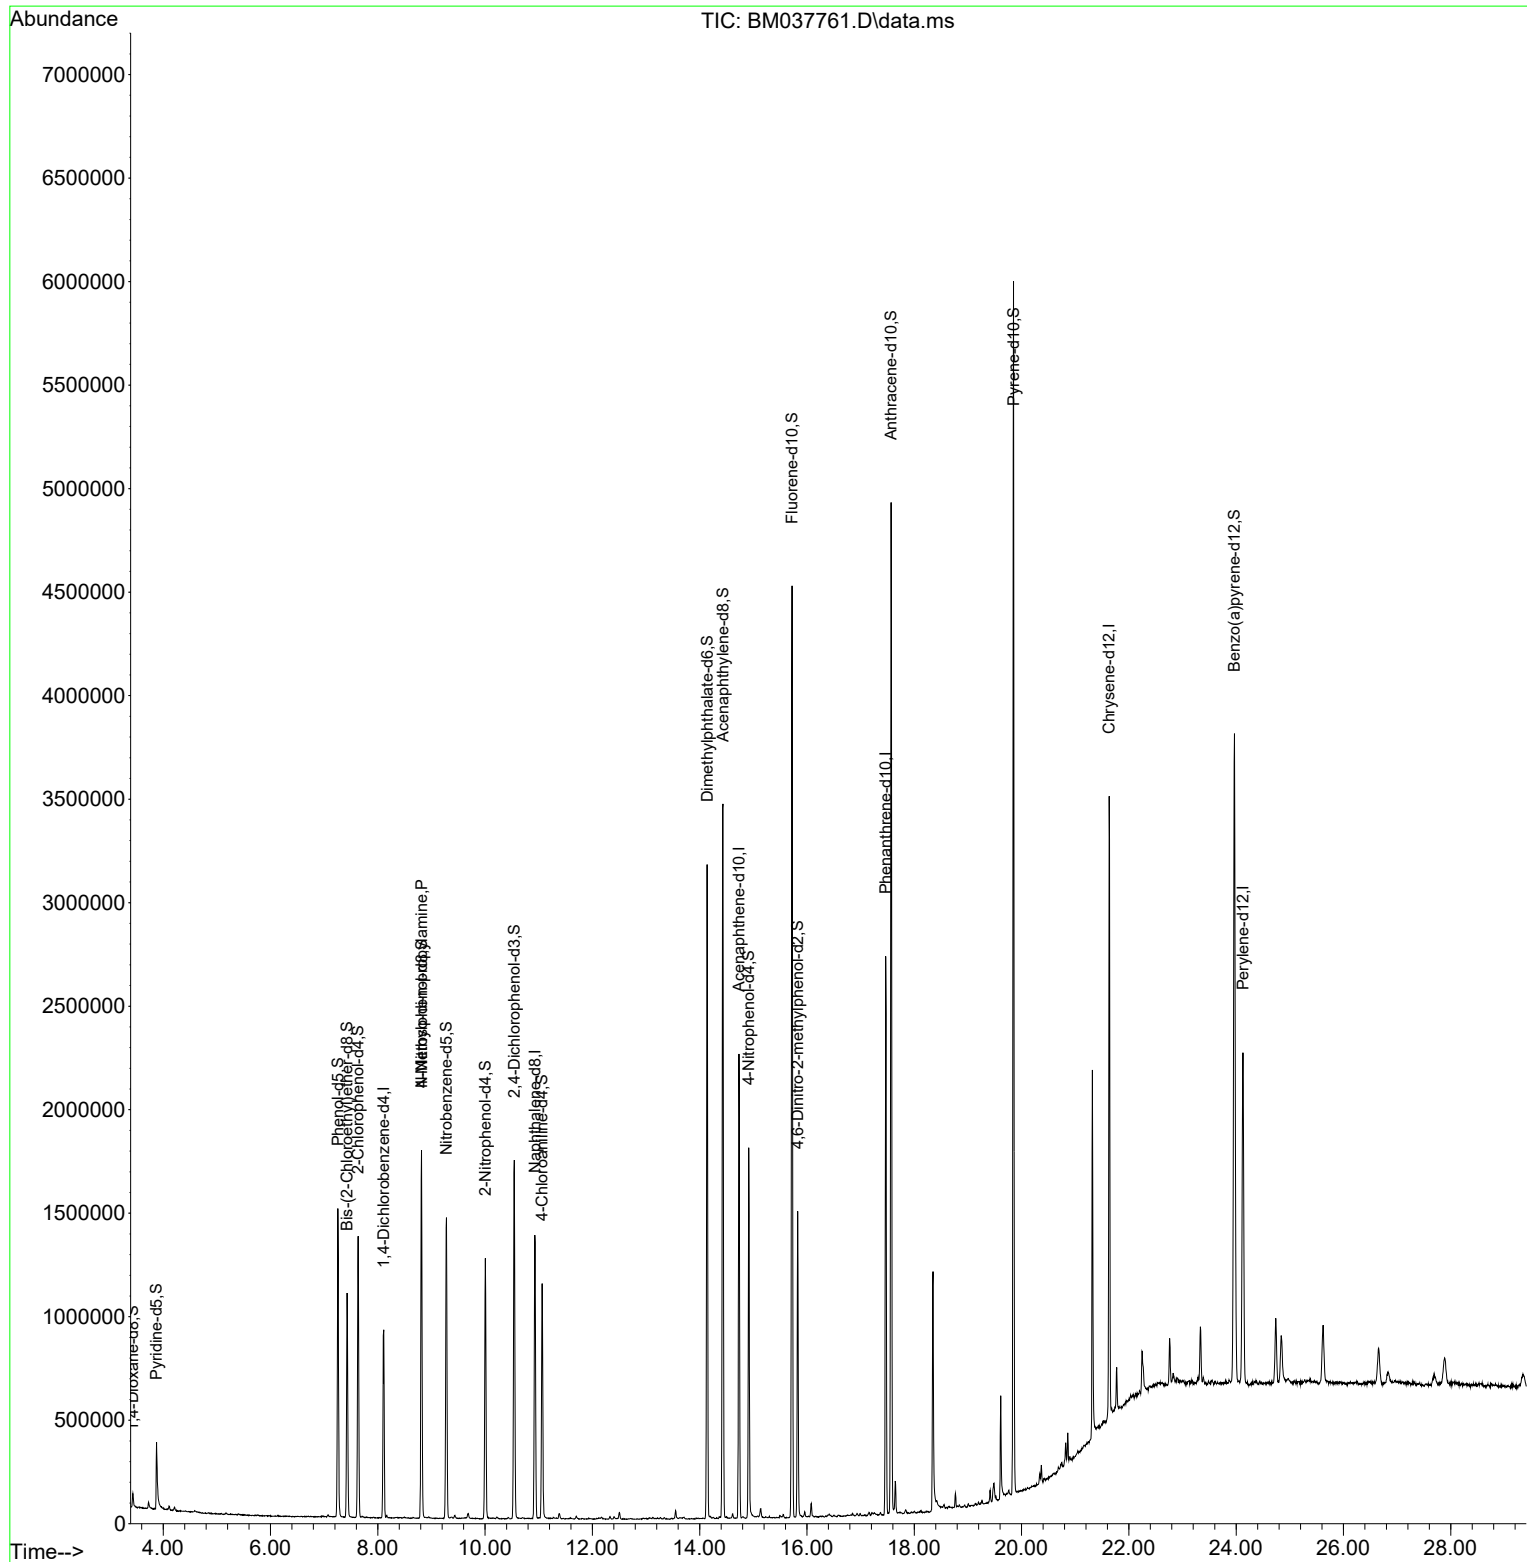

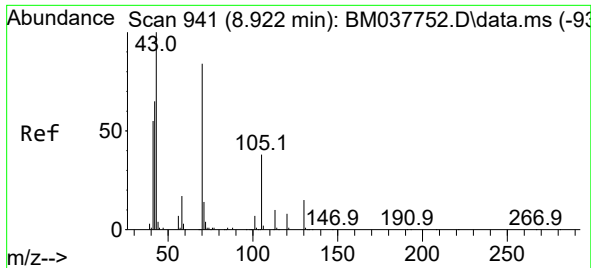

#17
 N-Nitroso-di-n-propylamine
 Concen: 1.042 ng/ul
 RT: 8.816 min Scan# 91
 Delta R.T. -0.106 min
 Lab File: BM037761.D
 Acq: 28 Nov 2022 16:01

Instrument :
 BNA_M
 ClientSampleId :
 C0L02

Tgt Ion: 70 Resp: 17643
 Ion Ratio Lower Upper
 70 100
 42 453.2 57.1 85.7#
 101 0.0 7.0 10.6#
 130 0.0 14.8 22.2#

