

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112822\
 Data File : BM037769.D
 Acq On : 28 Nov 2022 21:34
 Operator : CG/JU
 Sample : PB149209BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK209

Quant Time: Nov 28 22:30:33 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Nov 28 22:24:47 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.104	152	239297	20.000	ng/ul	0.00
20) Naphthalene-d8	10.927	136	1110334	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.733	164	697623	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.468	188	1413763	20.000	ng/ul	0.00
79) Chrysene-d12	21.633	240	1219301	20.000	ng/ul	0.00
88) Perylene-d12	24.127	264	979569	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.434	96	25656	4.446	ng/uL	0.00
4) Pyridine-d5	3.875	84	255281	13.592	ng/ul	0.00
7) Phenol-d5	7.257	99	537428	22.511	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.428	67	363301	22.813	ng/ul	0.00
11) 2-Chlorophenol-d4	7.634	132	402086	24.238	ng/ul	0.00
15) 4-Methylphenol-d8	8.810	113	426503	22.450	ng/ul	0.00
21) Nitrobenzene-d5	9.275	128	221078	25.398	ng/ul	0.00
24) 2-Nitrophenol-d4	10.004	143	229807	26.793	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.539	165	382728	24.384	ng/ul	0.00
31) 4-Chloroaniline-d4	11.063	131	459512	17.643	ng/ul	0.00
46) Dimethylphthalate-d6	14.139	166	1265225	25.604	ng/ul	0.00
49) Acenaphthylene-d8	14.427	160	1470390	25.210	ng/ul	0.00
54) 4-Nitrophenol-d4	14.915	143	230187	21.148	ng/ul	0.00
60) Fluorene-d10	15.721	176	1098460	25.382	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.827	200	144634	19.018	ng/ul	0.00
73) Anthracene-d10	17.568	188	1703028	25.760	ng/ul	0.00
81) Pyrene-d10	19.845	212	1832680	29.578	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.962	264	1306789	25.917	ng/ul	0.00
Target Compounds						
48) 2,6-Dinitrotoluene	14.139	165	10883	1.073	ng/ul#	36


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112822\
Data File : BM037769.D
Acq On : 28 Nov 2022 21:34
Operator : CG/JU
Sample : PB149209BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK209

Quant Time: Nov 28 22:30:33 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Nov 28 22:24:47 2022
Response via : Initial Calibration

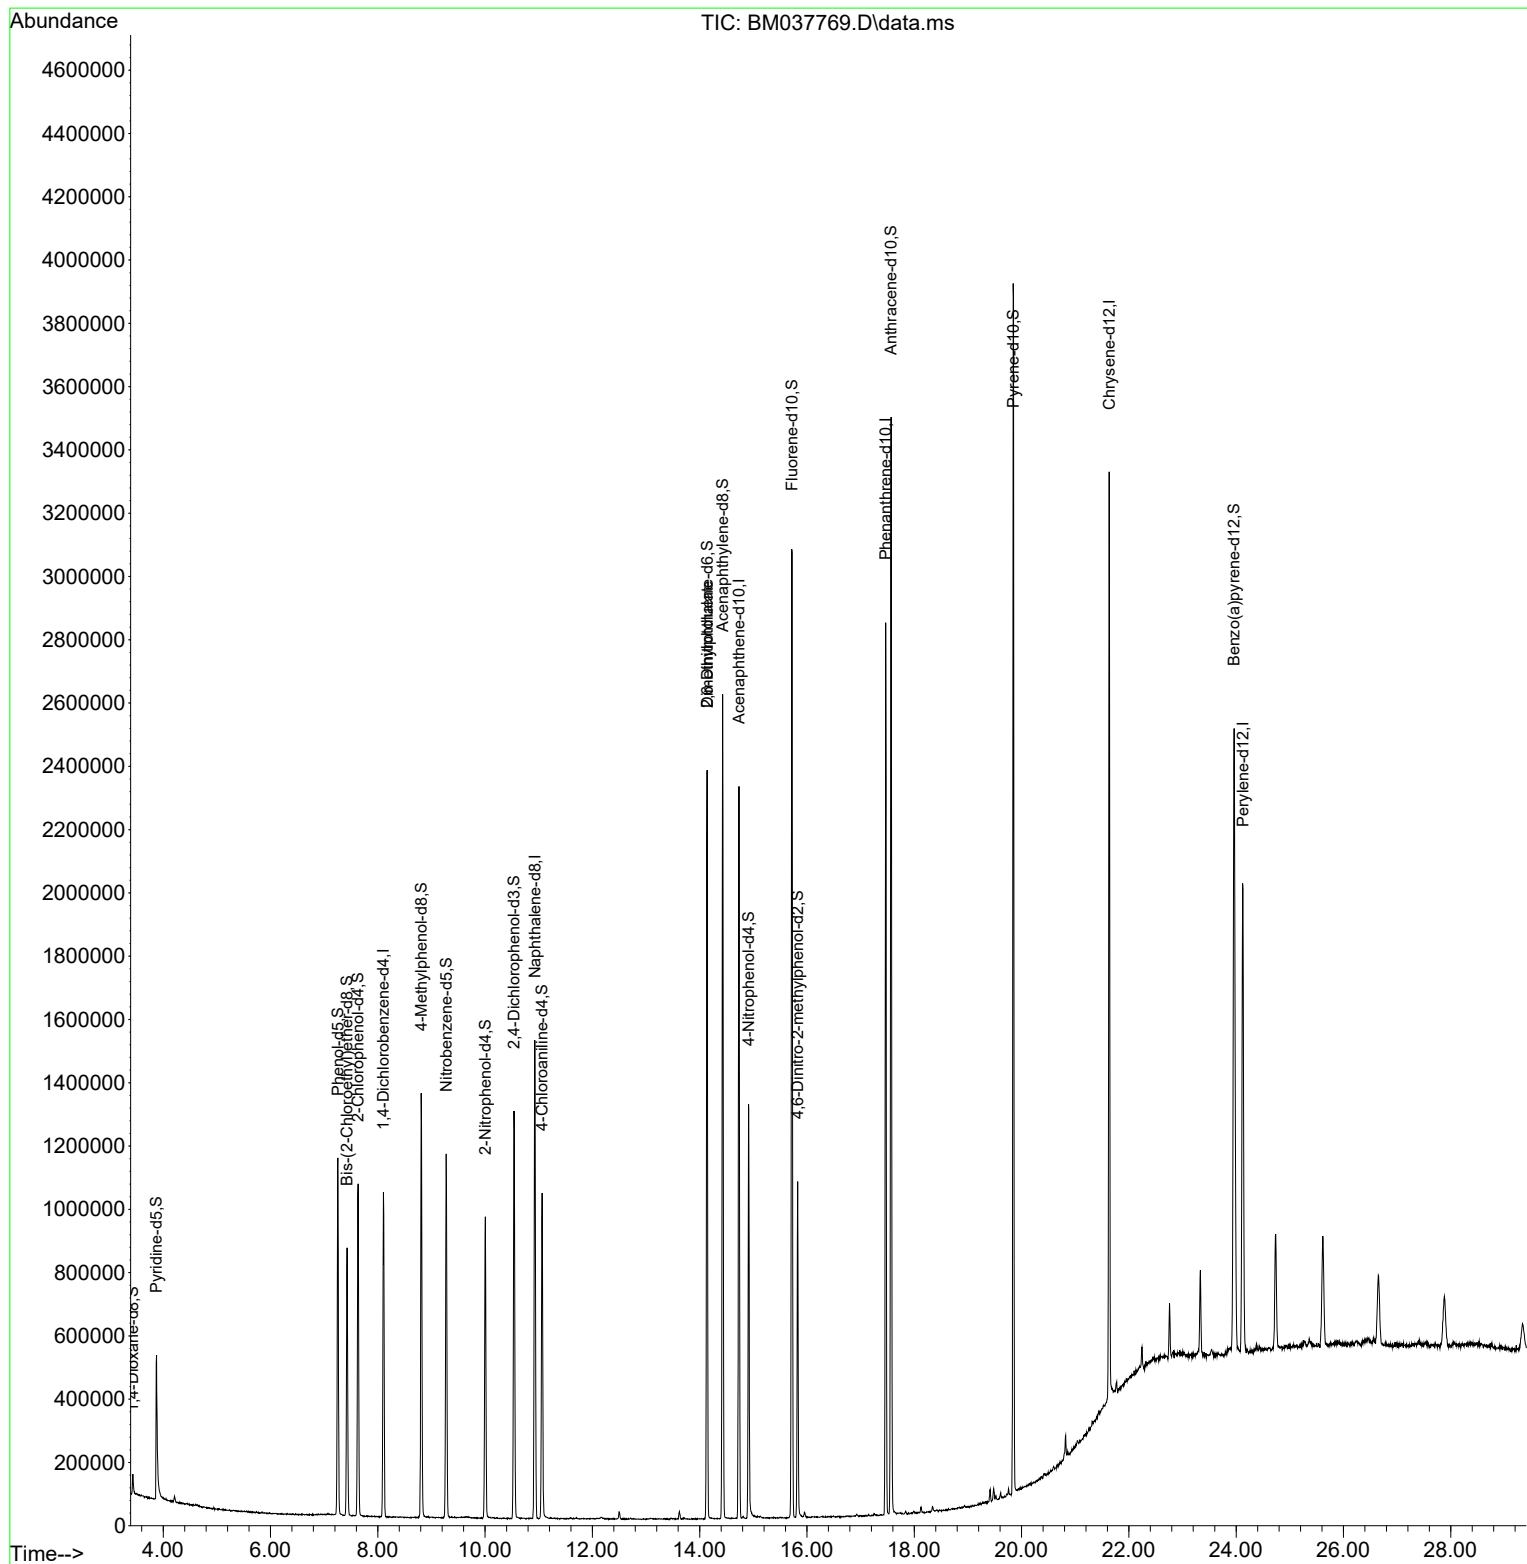

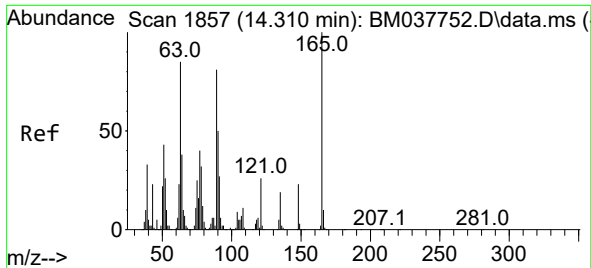

#48
 2,6-Dinitrotoluene
 Concen: 1.073 ng/ul
 RT: 14.139 min Scan# 11
 Delta R.T. -0.171 min
 Lab File: BM037769.D
 Acq: 28 Nov 2022 21:34

Instrument :
 BNA_M
 ClientSampleId :
 SBLK209

Tgt Ion:165 Resp: 10883
 Ion Ratio Lower Upper
 165 100
 89 3.9 56.4 84.6#
 121 29.9 18.9 28.3#

