

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112822\
 Data File : BM037777.D
 Acq On : 29 Nov 2022 02:27
 Operator : CG/JU
 Sample : N5710-02
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0KY1

Quant Time: Nov 29 03:33:00 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Nov 28 22:24:47 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.104	152	218532	20.000	ng/u1	0.00
20) Naphthalene-d8	10.928	136	1031386	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.733	164	622677	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.468	188	1237759	20.000	ng/u1	0.00
79) Chrysene-d12	21.627	240	1159438	20.000	ng/u1	-0.01
88) Perylene-d12	24.121	264	987924	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.434	96	21463	4.073	ng/uL	0.00
4) Pyridine-d5	3.875	84	154070	8.983	ng/u1	0.00
7) Phenol-d5	7.251	99	170729	7.831	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.422	67	452762	31.132	ng/u1	0.00
11) 2-Chlorophenol-d4	7.628	132	398152	26.282	ng/u1	0.00
15) 4-Methylphenol-d8	8.810	113	286786	16.530	ng/u1	0.00
21) Nitrobenzene-d5	9.275	128	264342	32.693	ng/u1	0.00
24) 2-Nitrophenol-d4	10.004	143	260163	32.655	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.539	165	408438	28.014	ng/u1	0.00
31) 4-Chloroaniline-d4	11.063	131	629051	26.001	ng/u1	0.00
46) Dimethylphthalate-d6	14.139	166	1458219	33.062	ng/u1	0.00
49) Acenaphthylene-d8	14.427	160	1720784	33.054	ng/u1	0.00
54) 4-Nitrophenol-d4	14.910	143	62425	6.426	ng/u1	0.00
60) Fluorene-d10	15.716	176	1278949	33.110	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.827	200	171979	25.829	ng/u1	0.00
73) Anthracene-d10	17.568	188	2095065	36.195	ng/u1	0.00
81) Pyrene-d10	19.845	212	2327954	39.511	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.956	264	1808528	35.565	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.469	88	140804	24.305	ng/uL	Qvalue 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112822\
Data File : BM037777.D
Acq On : 29 Nov 2022 02:27
Operator : CG/JU
Sample : N5710-02
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0KY1

Quant Time: Nov 29 03:33:00 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Nov 28 22:24:47 2022
Response via : Initial Calibration

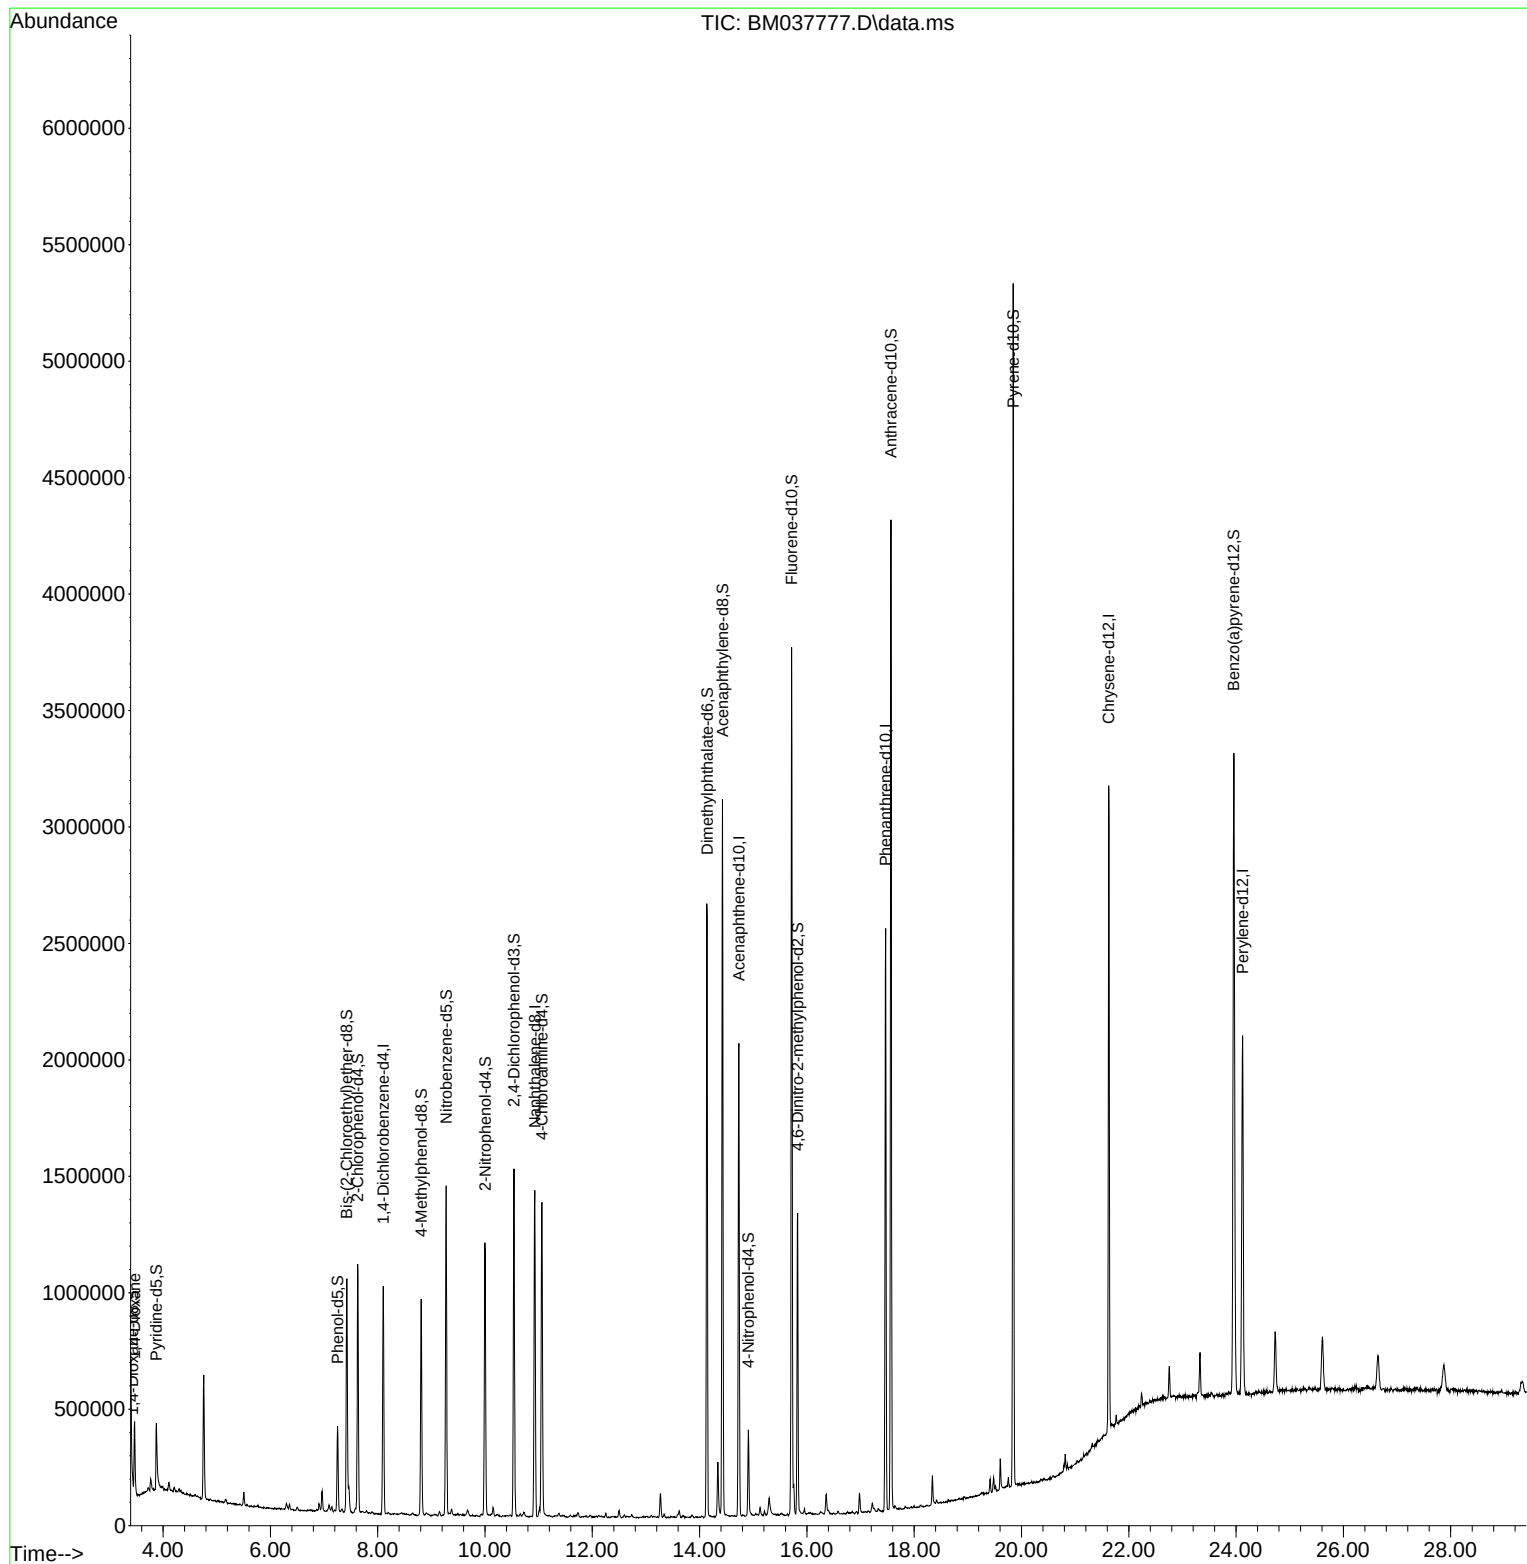

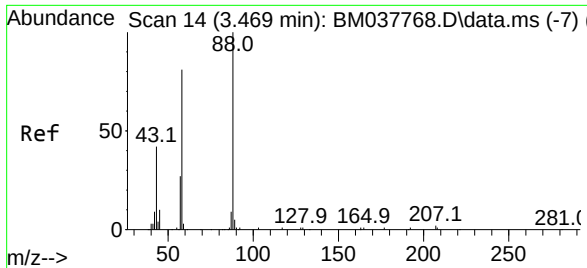

#2
 1,4-Dioxane
 Concen: 24.305 ng/uL
 RT: 3.469 min Scan# 14
 Delta R.T. 0.000 min
 Lab File: BM037777.D
 Acq: 29 Nov 2022 02:27

Instrument :
 BNA_M
 ClientSampleId :
 C0KY1

Tgt Ion: 88 Resp: 140804
 Ion Ratio Lower Upper
 88 100
 43 46.1 42.8 64.2
 58 83.2 62.6 94.0

