

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112822\
 Data File : BM037770.D
 Acq On : 28 Nov 2022 22:11
 Operator : CG/JU
 Sample : PB149202BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK202

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037770.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.434	4	8	15	rBV2	58697	87487	1.62%	0.138%
2	3.869	79	82	101	rBV	800856	1304730	24.11%	2.061%
3	4.204	137	139	149	rVB2	18898	30554	0.56%	0.048%
4	7.257	649	658	668	rBV	1173542	1838074	33.97%	2.904%
5	7.428	680	687	695	rBV	858045	1316272	24.33%	2.079%
6	7.634	715	722	737	rVB	1073600	1708904	31.58%	2.700%
7	8.104	796	802	811	rVB	947171	1466759	27.11%	2.317%
8	8.810	911	922	932	rBV	1375599	2168965	40.08%	3.426%
9	9.275	993	1001	1009	rBV	1173680	1890068	34.93%	2.986%
10	10.004	1117	1125	1137	rBV	980099	1579436	29.19%	2.495%
11	10.539	1209	1216	1224	rBV	1323910	2159543	39.91%	3.411%
12	10.927	1274	1282	1296	rVB	1410780	2286779	42.26%	3.612%
13	11.063	1297	1305	1323	rBV	1353763	2268649	41.93%	3.584%
14	11.604	1392	1397	1401	rVB8	2715	5463	0.10%	0.009%
15	12.498	1545	1549	1556	rVB2	22934	38770	0.72%	0.061%
16	13.621	1735	1740	1745	rBV3	16867	26961	0.50%	0.043%
17	13.710	1751	1755	1757	rBV4	4592	5683	0.11%	0.009%
18	14.139	1821	1828	1837	rBV	2318842	3168587	58.56%	5.006%
19	14.427	1869	1877	1886	rBV	2643530	3732024	68.97%	5.896%
20	14.733	1921	1929	1937	rBV	2120501	3034711	56.08%	4.794%
21	14.804	1939	1941	1948	rVB6	5682	8582	0.16%	0.014%
22	14.910	1953	1959	1974	rBV	1340059	1999495	36.95%	3.159%
23	15.139	1994	1998	2001	rVB5	8073	10560	0.20%	0.017%
24	15.715	2085	2096	2104	rBV	3159537	4536858	83.85%	7.167%
25	15.827	2108	2115	2127	rVV	1057407	1399492	25.86%	2.211%
26	15.957	2132	2137	2141	rVB3	18620	29634	0.55%	0.047%
27	16.492	2226	2228	2232	rBV5	4963	7881	0.15%	0.012%
28	16.921	2299	2301	2305	rVB4	7449	9213	0.17%	0.015%
29	17.145	2336	2339	2346	rVB9	3948	8683	0.16%	0.014%
30	17.215	2346	2351	2353	rBV6	5138	8574	0.16%	0.014%
31	17.251	2354	2357	2362	rVB7	4144	7875	0.15%	0.012%
32	17.468	2387	2394	2404	rBV	2594251	3502646	64.73%	5.533%
33	17.568	2404	2411	2420	rBV	3594591	4963629	91.73%	7.841%
34	17.845	2454	2458	2459	rBV4	6372	7280	0.13%	0.012%
35	18.339	2540	2542	2548	rVB7	7808	10349	0.19%	0.016%
36	19.415	2721	2725	2729	rBV3	44238	55273	1.02%	0.087%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112822\
Data File : BM037770.D
Acq On : 28 Nov 2022 22:11
Operator : CG/JU
Sample : PB149202BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK202

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Title : SVOA CALIBRATION

37	19.480	2732	2736	2740	rBV3	39762	56328	1.04%	0.089%
38	19.756	2780	2783	2787	rVB4	15341	20114	0.37%	0.032%
39	19.845	2792	2798	2805	rBV	3928925	5410918	100.00%	8.548%
40	20.815	2961	2963	2967	rVB	52680	56784	1.05%	0.090%
41	21.633	3096	3102	3108	rBV	2760089	3598499	66.50%	5.685%
42	23.956	3490	3497	3510	rVB2	2148060	4577389	84.60%	7.231%
43	24.121	3519	3525	3535	rVB2	1432635	2897476	53.55%	4.577%


Sum of corrected areas: 63301951

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112822\
Data File : BM037770.D
Acq On : 28 Nov 2022 22:11
Operator : CG/JU
Sample : PB149202BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK202

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

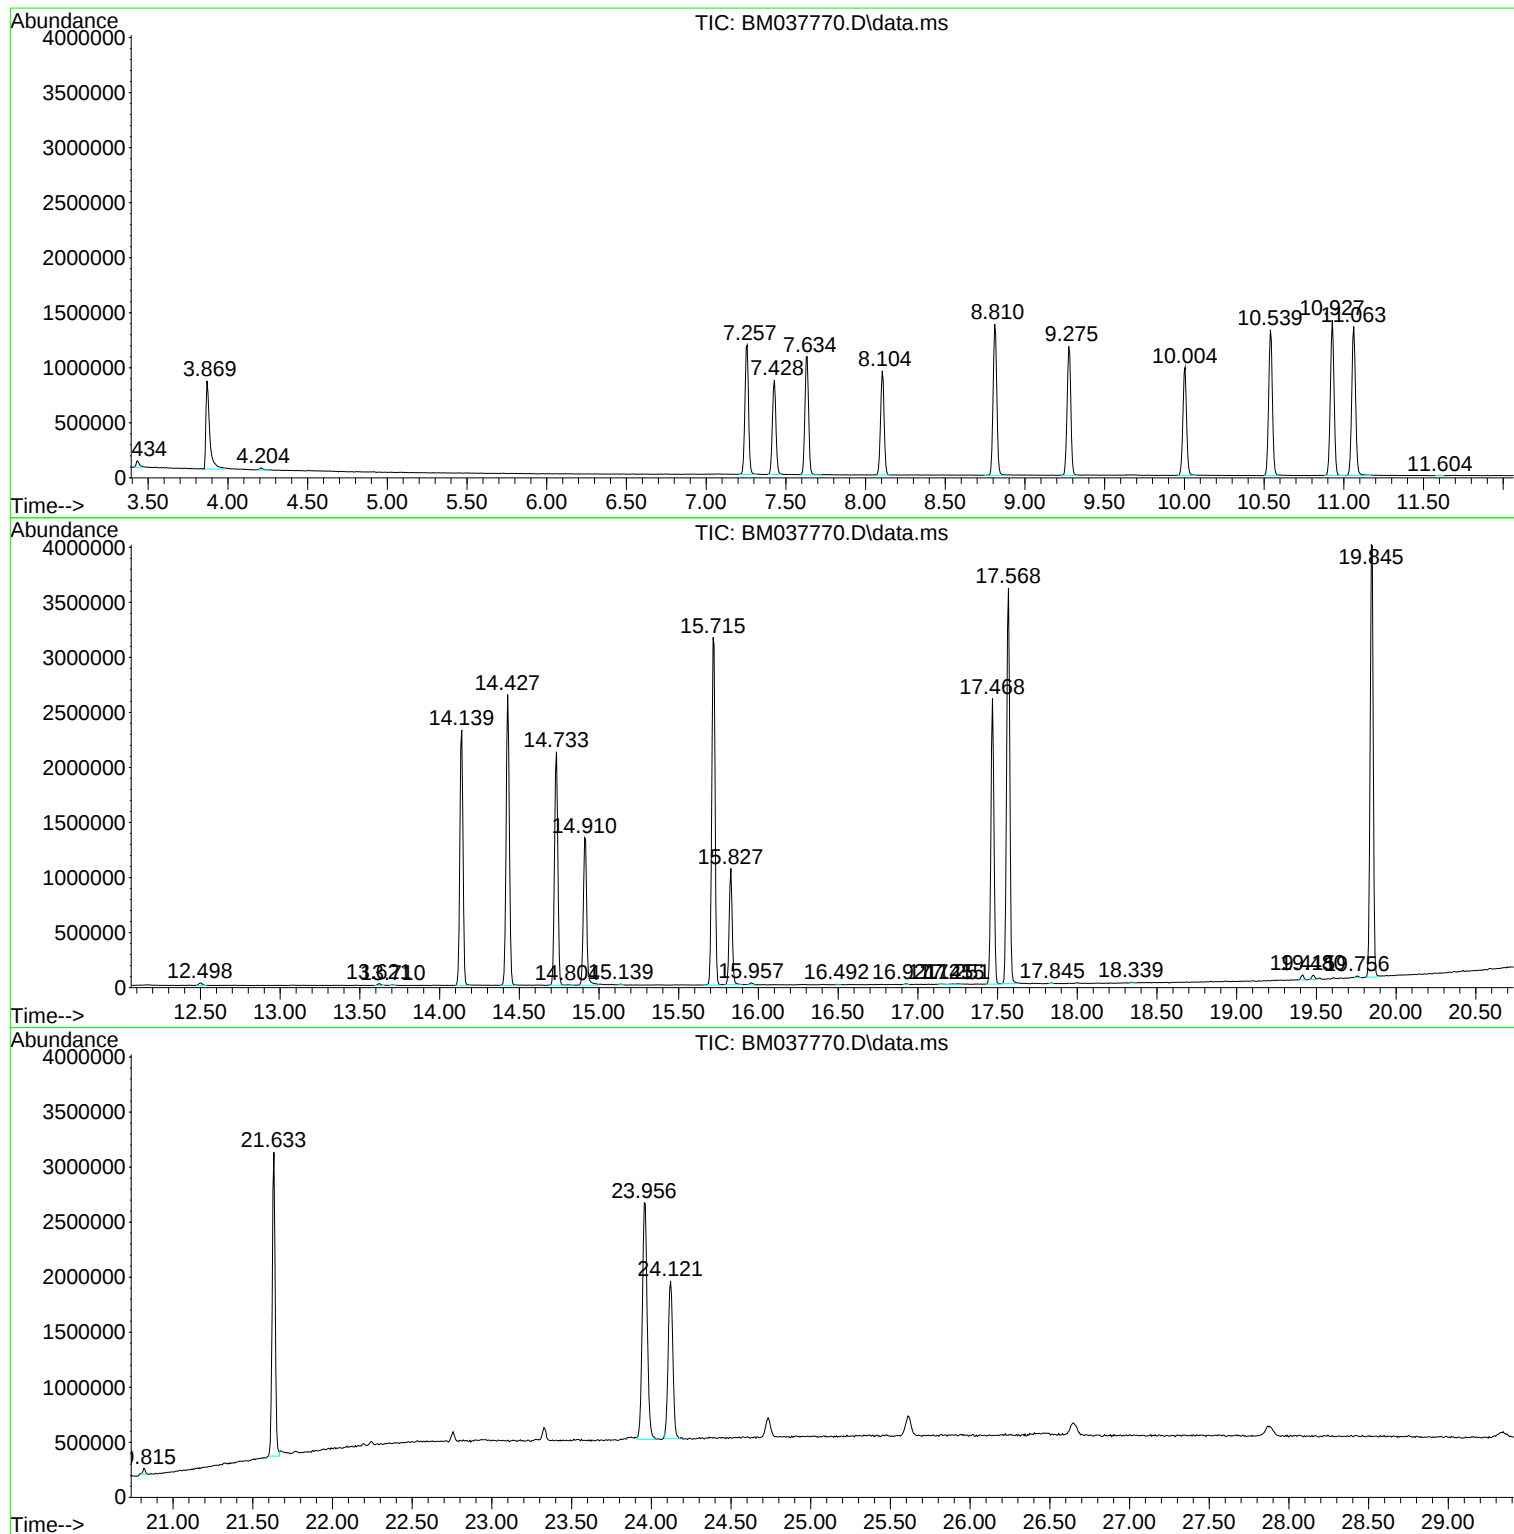

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112822\
Data File : BM037770.D
Acq On : 28 Nov 2022 22:11
Operator : CG/JU
Sample : PB149202BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK202

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112822\
Data File : BM037770.D
Acq On : 28 Nov 2022 22:11
Operator : CG/JU
Sample : PB149202BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK202

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc