

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112822\
 Data File : BM037773.D
 Acq On : 29 Nov 2022 00:01
 Operator : CG/JU
 Sample : N5684-02
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH1H2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037773.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.881	81	84	99	rVB	77596	161440	2.80%	0.267%
2	4.204	137	139	144	rVB3	16097	22664	0.39%	0.037%
3	4.757	227	233	245	rVB	1079869	1618031	28.03%	2.675%
4	7.251	651	657	666	rVB	287146	445583	7.72%	0.737%
5	7.428	680	687	695	rVB	855534	1346273	23.32%	2.226%
6	7.628	714	721	732	rBV	860635	1365947	23.66%	2.259%
7	7.722	732	737	738	rBV5	5036	6882	0.12%	0.011%
8	8.104	794	802	810	rBV	922772	1428678	24.75%	2.362%
9	8.810	915	922	931	rBV	759041	1175781	20.37%	1.944%
10	9.275	993	1001	1011	rBV	1211740	1934767	33.52%	3.199%
11	9.375	1014	1018	1020	rVV4	6196	8518	0.15%	0.014%
12	9.433	1023	1028	1033	rBV9	5672	10661	0.18%	0.018%
13	9.681	1064	1070	1074	rVB4	13227	17319	0.30%	0.029%
14	9.998	1116	1124	1132	rBV	918564	1494242	25.89%	2.471%
15	10.210	1156	1160	1164	rBV7	4017	6173	0.11%	0.010%
16	10.539	1208	1216	1225	rBV	1221409	1986739	34.42%	3.285%
17	10.928	1274	1282	1289	rBV	1364440	2222861	38.51%	3.676%
18	11.063	1298	1305	1316	rBV	1046674	1782914	30.89%	2.948%
19	12.163	1486	1492	1493	rBV4	6468	7649	0.13%	0.013%
20	12.322	1514	1519	1525	rBV5	13459	20866	0.36%	0.035%
21	12.504	1545	1550	1556	rBV3	21469	35524	0.62%	0.059%
22	13.127	1652	1656	1659	rBV6	6391	7373	0.13%	0.012%
23	13.474	1709	1715	1720	rBV9	3466	6816	0.12%	0.011%
24	13.551	1720	1728	1733	rVV	23272	37288	0.65%	0.062%
25	13.621	1736	1740	1748	rVV3	18002	30191	0.52%	0.050%
26	13.704	1748	1754	1760	rVB8	6619	15337	0.27%	0.025%
27	14.045	1808	1812	1815	rBV6	3555	6590	0.11%	0.011%
28	14.139	1819	1828	1836	rBV	2368403	3240715	56.14%	5.359%
29	14.368	1864	1867	1870	rBV4	4334	6682	0.12%	0.011%
30	14.427	1870	1877	1886	rVV2	2718871	3803617	65.89%	6.289%
31	14.610	1905	1908	1914	rVB5	6457	7789	0.13%	0.013%
32	14.733	1921	1929	1938	rBV	1997551	2908876	50.39%	4.810%
33	14.910	1953	1959	1971	rBV	274948	424889	7.36%	0.703%
34	15.133	1993	1997	2001	rBV5	18953	28446	0.49%	0.047%
35	15.374	2033	2038	2044	rBV9	3418	7528	0.13%	0.012%
36	15.557	2067	2069	2072	rVB4	6141	6911	0.12%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112822\
 Data File : BM037773.D
 Acq On : 29 Nov 2022 00:01
 Operator : CG/JU
 Sample : N5684-02
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH1H2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
 Title : SVOA CALIBRATION

37	15.715	2087	2096	2105	rBV	3299589	4694305	81.32%	7.762%
38	15.827	2109	2115	2124	rBV	1051460	1427365	24.73%	2.360%
39	15.951	2132	2136	2143	rVB2	16978	26812	0.46%	0.044%
40	16.074	2153	2157	2161	rBV6	7079	11499	0.20%	0.019%
41	16.504	2224	2230	2233	rBV7	6084	10666	0.18%	0.018%
42	16.927	2296	2302	2305	rBV5	9140	13582	0.24%	0.022%
43	17.139	2335	2338	2339	rBV3	5790	5957	0.10%	0.010%
44	17.198	2347	2348	2353	rBV5	5188	6478	0.11%	0.011%
45	17.256	2355	2358	2361	rVB4	6760	8667	0.15%	0.014%
46	17.468	2387	2394	2402	rBV	2457694	3359238	58.20%	5.555%
47	17.568	2404	2411	2419	rVV	3866221	5357998	92.82%	8.860%
48	17.645	2420	2424	2428	rVB3	34148	50121	0.87%	0.083%
49	17.839	2453	2457	2462	rVB7	14590	19772	0.34%	0.033%
50	18.121	2503	2505	2509	rVB3	9721	9286	0.16%	0.015%
51	18.339	2538	2542	2550	rBV	109633	150366	2.60%	0.249%
52	18.421	2553	2556	2559	rVB	9181	11218	0.19%	0.019%
53	18.768	2611	2615	2618	rBV2	62330	70265	1.22%	0.116%
54	19.415	2720	2725	2729	rBV3	49504	68294	1.18%	0.113%
55	19.480	2732	2736	2740	rVV	51148	81908	1.42%	0.135%
56	19.515	2740	2742	2745	rVV3	23504	29863	0.52%	0.049%
57	19.545	2745	2747	2751	rVB	61968	62581	1.08%	0.103%
58	19.609	2754	2758	2763	rBV4	60275	78976	1.37%	0.131%
59	19.756	2780	2783	2788	rVB3	40006	41904	0.73%	0.069%
60	19.845	2792	2798	2806	rBV	4287019	5772290	100.00%	9.545%
61	20.815	2961	2963	2967	rVB3	58398	63881	1.11%	0.106%
62	21.321	3045	3049	3055	rBV2	184936	276556	4.79%	0.457%
63	21.633	3096	3102	3109	rBV	2563489	3413507	59.14%	5.644%
64	23.956	3490	3497	3508	rVB2	2242585	4966489	86.04%	8.212%
65	24.121	3518	3525	3534	rVB2	1387247	2748932	47.62%	4.545%




Sum of corrected areas: 60477336

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112822\
Data File : BM037773.D
Acq On : 29 Nov 2022 00:01
Operator : CG/JU
Sample : N5684-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH1H2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

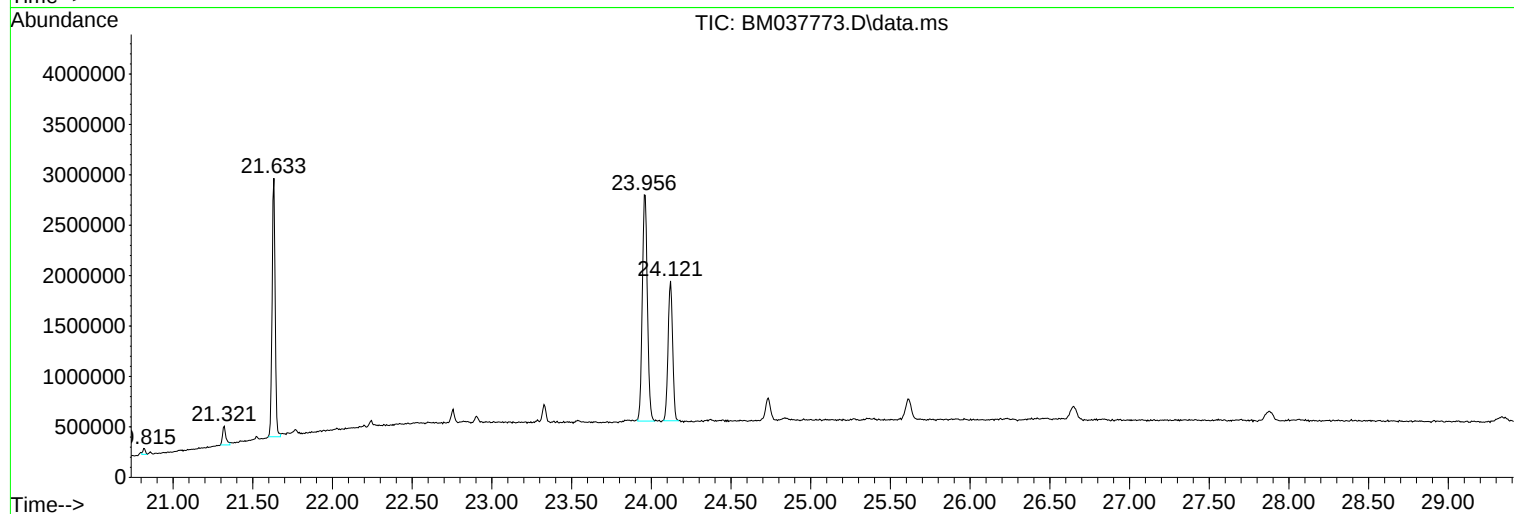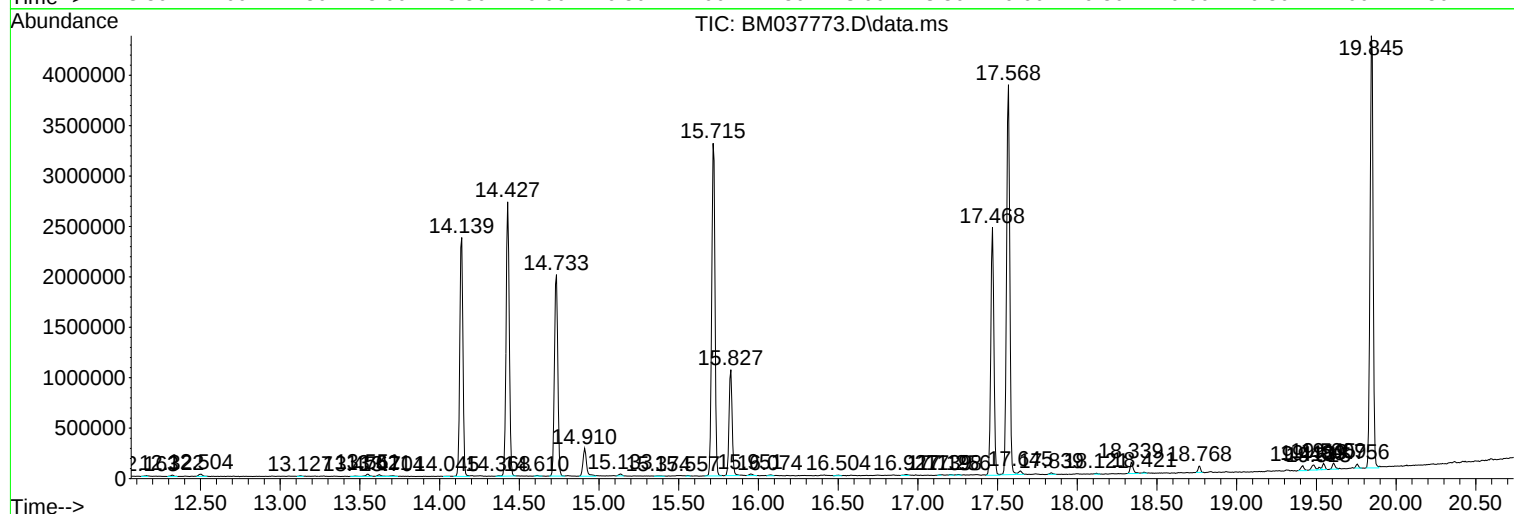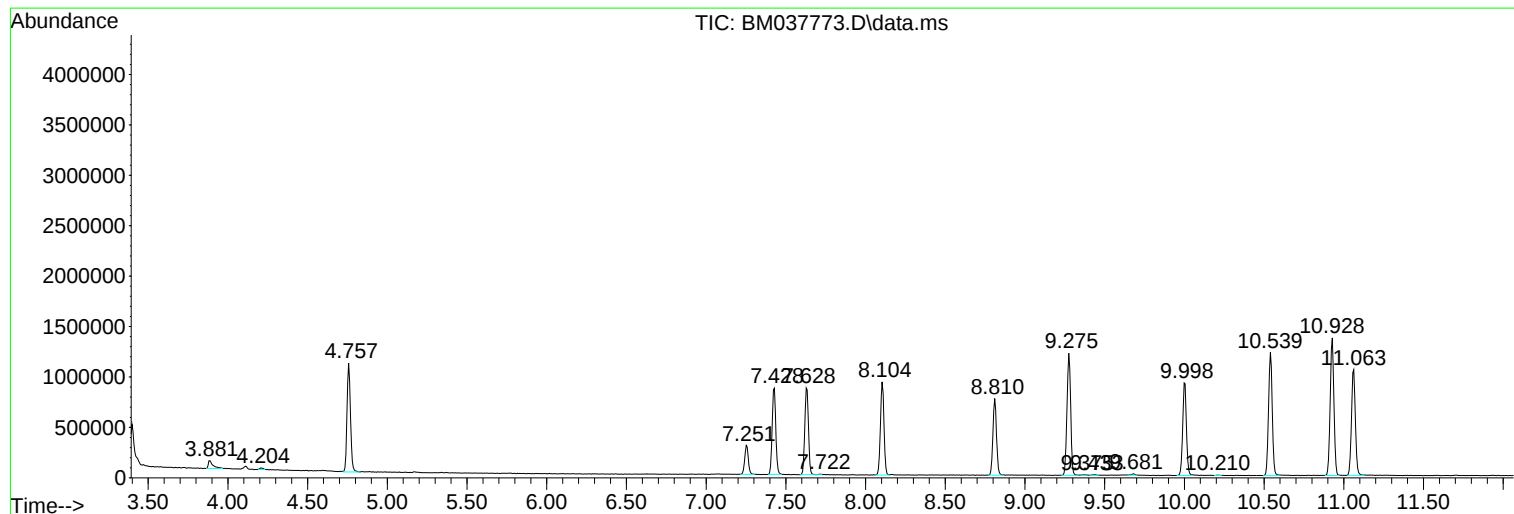

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112822\
Data File : BM037773.D
Acq On : 29 Nov 2022 00:01
Operator : CG/JU
Sample : N5684-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH1H2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112822\
Data File : BM037773.D
Acq On : 29 Nov 2022 00:01
Operator : CG/JU
Sample : N5684-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH1H2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc