

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112822\
 Data File : BM037776.D
 Acq On : 29 Nov 2022 01:51
 Operator : CG/JU
 Sample : N5710-01
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COKY0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037776.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.469	10	14	20	rVB	290732	373710	5.46%	0.543%
2	3.769	62	65	74	rVB	51556	77034	1.13%	0.112%
3	3.875	80	83	96	rVB	223922	368543	5.39%	0.535%
4	4.757	227	233	243	rBV	483230	705599	10.32%	1.025%
5	5.504	356	360	366	rVB	56085	86177	1.26%	0.125%
6	6.298	490	495	500	rBV2	24286	48895	0.71%	0.071%
7	6.357	503	505	509	rVB	18204	22002	0.32%	0.032%
8	6.498	526	529	534	rVB3	13195	20298	0.30%	0.029%
9	6.910	594	599	603	rBV4	25009	40271	0.59%	0.059%
10	6.963	603	608	613	rVV	69068	100653	1.47%	0.146%
11	7.092	624	630	634	rBV	23211	41272	0.60%	0.060%
12	7.145	636	639	644	rVB2	19632	26289	0.38%	0.038%
13	7.251	651	657	664	rVB	315759	480173	7.02%	0.698%
14	7.334	666	671	679	rVB9	14975	25305	0.37%	0.037%
15	7.428	679	687	691	rBV	857707	1379124	20.17%	2.004%
16	7.587	706	714	715	rBV6	19665	32077	0.47%	0.047%
17	7.628	715	721	731	rVV	922139	1437455	21.02%	2.089%
18	7.710	731	735	741	rVB8	11933	24722	0.36%	0.036%
19	7.792	744	749	754	rVB7	14473	26061	0.38%	0.038%
20	7.892	762	766	772	rVB9	9562	20193	0.30%	0.029%
21	8.104	796	802	809	rBV	879120	1337653	19.56%	1.944%
22	8.645	889	894	898	rBV7	13252	21678	0.32%	0.031%
23	8.810	915	922	932	rVV	829020	1308132	19.13%	1.901%
24	8.904	934	938	942	rVV7	8614	12305	0.18%	0.018%
25	9.145	976	979	985	rBV3	17080	29398	0.43%	0.043%
26	9.275	994	1001	1009	rBV	1199464	1933085	28.27%	2.809%
27	9.492	1034	1038	1042	rBV7	8935	16604	0.24%	0.024%
28	9.675	1063	1069	1075	rVV10	25293	54375	0.80%	0.079%
29	9.928	1106	1112	1113	rBV5	11680	17785	0.26%	0.026%
30	9.998	1117	1124	1133	rVV	1007807	1707717	24.97%	2.481%
31	10.151	1145	1150	1156	rVB2	37114	68763	1.01%	0.100%
32	10.228	1161	1163	1171	rVB9	8696	14229	0.21%	0.021%
33	10.469	1202	1204	1208	rVB5	8380	12802	0.19%	0.019%
34	10.539	1208	1216	1228	rBV	1334090	2164816	31.65%	3.145%
35	10.651	1232	1235	1242	rVB9	14458	20822	0.30%	0.030%
36	10.728	1242	1248	1255	rBV10	19287	46627	0.68%	0.068%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112822\
 Data File : BM037776.D
 Acq On : 29 Nov 2022 01:51
 Operator : CG/JU
 Sample : N5710-01
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COKY0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
 Title : SVOA CALIBRATION

37	10.928	1275	1282	1290	rVV	1292958	2172148	31.76%	3.156%
38	11.010	1290	1296	1299	rVV	30029	59857	0.88%	0.087%
39	11.063	1299	1305	1321	rVB	1153871	2008951	29.38%	2.919%
40	11.386	1355	1360	1363	rVB7	14001	24490	0.36%	0.036%
41	11.586	1390	1394	1397	rBV6	7469	11386	0.17%	0.017%
42	11.733	1414	1419	1425	rVB8	23399	39487	0.58%	0.057%
43	11.886	1441	1445	1450	rVB8	6392	12480	0.18%	0.018%
44	11.957	1452	1457	1462	rBV9	9806	18046	0.26%	0.026%
45	12.122	1480	1485	1487	rVB4	10130	12241	0.18%	0.018%
46	12.251	1501	1507	1514	rVB4	22005	38101	0.56%	0.055%
47	12.322	1514	1519	1522	rBV7	8513	14385	0.21%	0.021%
48	12.498	1544	1549	1557	rVB2	26674	49198	0.72%	0.071%
49	12.592	1561	1565	1571	rBV8	11964	24859	0.36%	0.036%
50	12.739	1587	1590	1593	rVB3	14668	14957	0.22%	0.022%
51	12.951	1620	1626	1627	rBV6	7639	12172	0.18%	0.018%
52	13.098	1646	1651	1654	rBV6	12387	18925	0.28%	0.027%
53	13.269	1675	1680	1687	rBV	85971	132771	1.94%	0.193%
54	13.339	1690	1692	1698	rVB6	20442	23747	0.35%	0.035%
55	13.551	1724	1728	1731	rBV6	12453	13834	0.20%	0.020%
56	13.621	1731	1740	1747	rVB3	49978	99031	1.45%	0.144%
57	13.680	1747	1750	1753	rBV5	10743	17061	0.25%	0.025%
58	13.857	1777	1780	1786	rVB7	12178	22574	0.33%	0.033%
59	14.045	1807	1812	1819	rVB9	9379	19294	0.28%	0.028%
60	14.133	1821	1827	1834	rBV	2569225	3537056	51.72%	5.139%
61	14.339	1856	1862	1870	rBV	245293	396326	5.80%	0.576%
62	14.427	1870	1877	1889	rVB	2950783	4200073	61.41%	6.103%
63	14.604	1905	1907	1912	rVB6	8408	12876	0.19%	0.019%
64	14.727	1922	1928	1937	rBV	1953772	2936805	42.94%	4.267%
65	14.798	1938	1940	1945	rVB6	7892	11926	0.17%	0.017%
66	14.910	1953	1959	1966	rBV	389779	553129	8.09%	0.804%
67	15.051	1979	1983	1985	rBV4	10862	13401	0.20%	0.019%
68	15.127	1992	1996	2001	rVB7	40390	61958	0.91%	0.090%
69	15.210	2006	2010	2013	rBV6	20683	31652	0.46%	0.046%
70	15.298	2018	2025	2036	rBV	90748	211366	3.09%	0.307%
71	15.515	2055	2062	2063	rBV7	8082	14217	0.21%	0.021%
72	15.715	2087	2096	2101	rBV	3689066	5253557	76.82%	7.633%
73	15.751	2101	2102	2108	rVV	136884	148838	2.18%	0.216%
74	15.827	2109	2115	2127	rVV	1295364	1843719	26.96%	2.679%
75	15.957	2133	2137	2141	rVB5	18190	29842	0.44%	0.043%
76	16.033	2146	2150	2153	rVV6	12751	12763	0.19%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112822\
 Data File : BM037776.D
 Acq On : 29 Nov 2022 01:51
 Operator : CG/JU
 Sample : N5710-01
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COKY0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
 Title : SVOA CALIBRATION

77	16.074	2154	2157	2161	rVB6	10685	12337	0.18%	0.018%
78	16.251	2182	2187	2192	rBV9	17532	37258	0.54%	0.054%
79	16.362	2201	2206	2215	rBV	73136	143389	2.10%	0.208%
80	16.580	2239	2243	2251	rVB9	17019	31759	0.46%	0.046%
81	16.845	2285	2288	2295	rVB9	15468	24185	0.35%	0.035%
82	16.980	2307	2311	2319	rVB3	89180	135401	1.98%	0.197%
83	17.221	2346	2352	2357	rBV7	42826	87599	1.28%	0.127%
84	17.333	2367	2371	2376	rBV7	14989	27472	0.40%	0.040%
85	17.468	2387	2394	2401	rBV	2563361	3509423	51.32%	5.099%
86	17.568	2404	2411	2420	rVV2	4201218	6093045	89.09%	8.853%
87	17.645	2421	2424	2429	rVB7	23572	34424	0.50%	0.050%
88	17.833	2454	2456	2461	rVB6	14923	14057	0.21%	0.020%
89	18.339	2538	2542	2551	rBV2	181240	255364	3.73%	0.371%
90	18.762	2611	2614	2618	rBV	75589	87124	1.27%	0.127%
91	19.415	2721	2725	2730	rBV	63692	75435	1.10%	0.110%
92	19.486	2734	2737	2740	rVB2	53215	69494	1.02%	0.101%
93	19.603	2753	2757	2764	rBV2	127710	199595	2.92%	0.290%
94	19.756	2780	2783	2786	rVB3	40435	42821	0.63%	0.062%
95	19.845	2792	2798	2806	rBV	5318537	6838847	100.00%	9.937%
96	20.815	2961	2963	2967	rVB	74285	78469	1.15%	0.114%
97	21.321	3045	3049	3054	rBV3	127885	194909	2.85%	0.283%
98	21.633	3096	3102	3110	rBV	2760153	3722796	54.44%	5.409%
99	23.956	3490	3497	3508	rVB2	2769188	5852614	85.58%	8.504%
100	24.121	3518	3525	3535	rVB2	1470333	3023961	44.22%	4.394%




Sum of corrected areas: 68823921

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112822\
Data File : BM037776.D
Acq On : 29 Nov 2022 01:51
Operator : CG/JU
Sample : N5710-01
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COKY0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

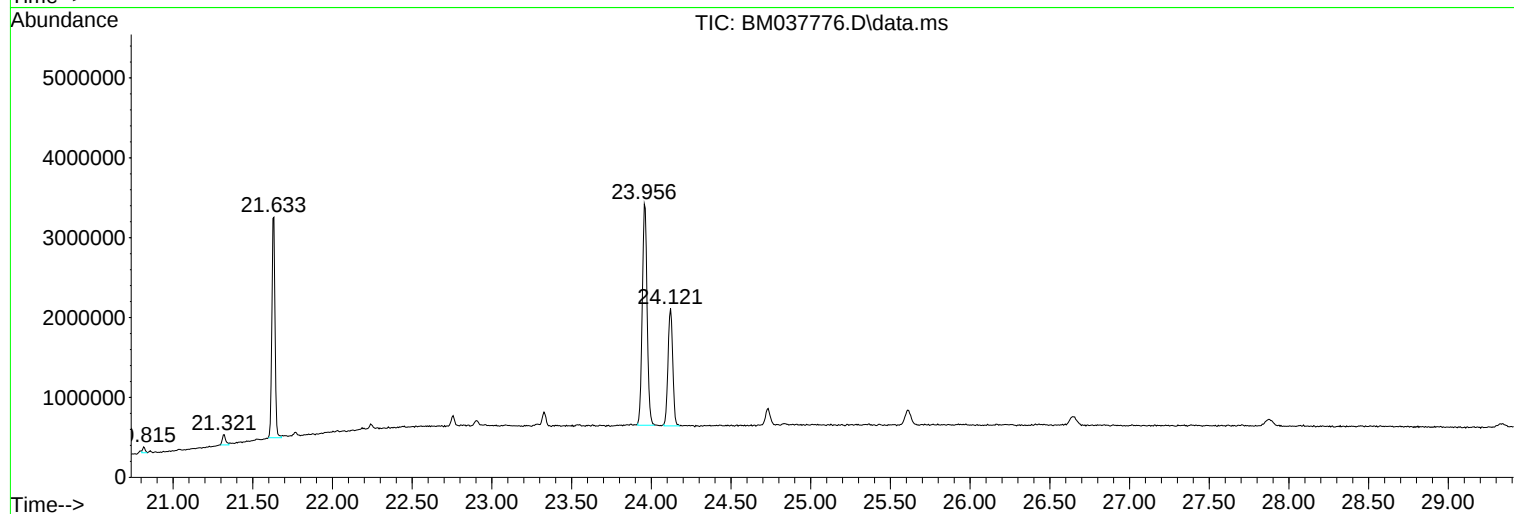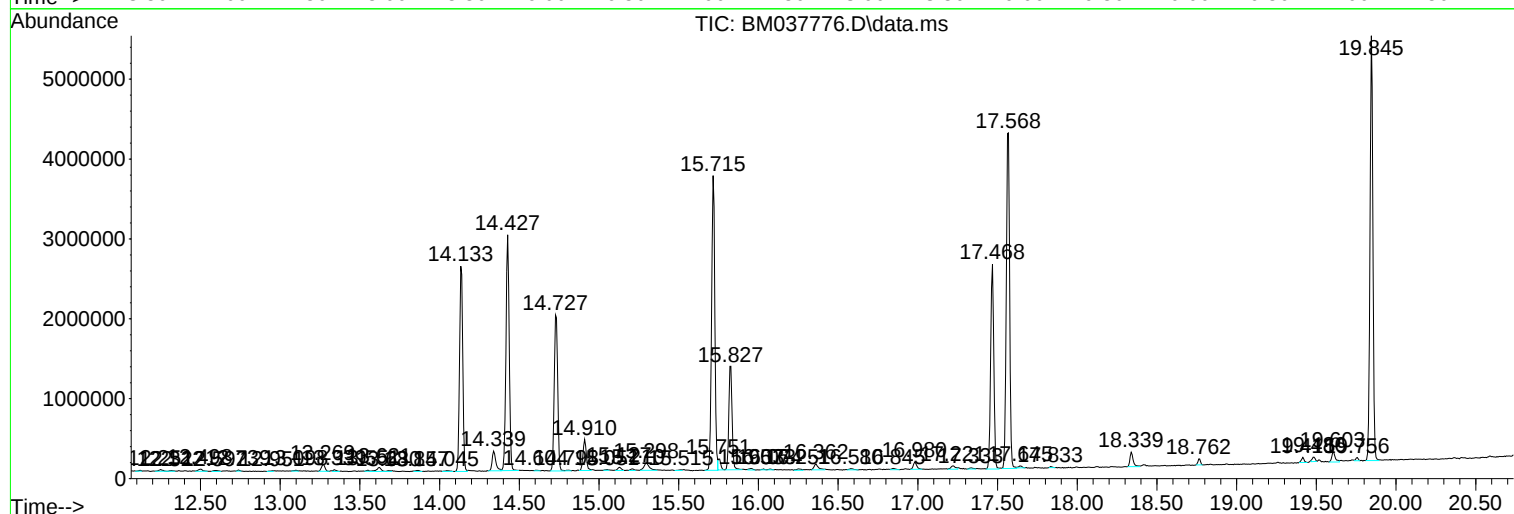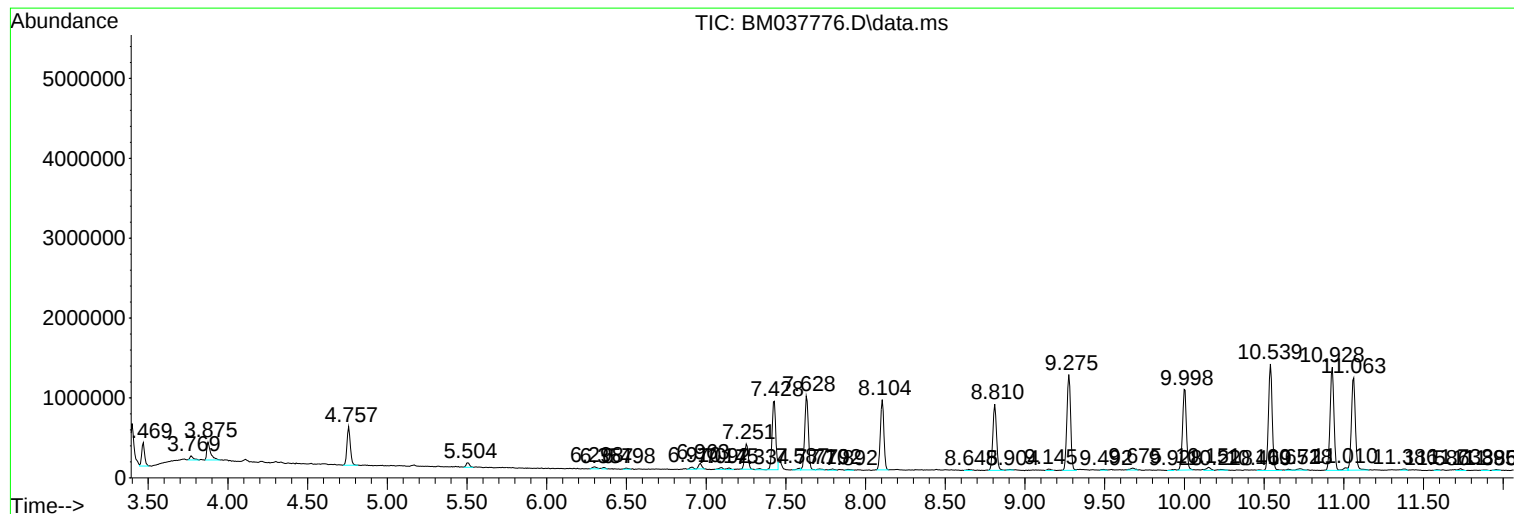

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112822\
Data File : BM037776.D
Acq On : 29 Nov 2022 01:51
Operator : CG/JU
Sample : N5710-01
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COKY0










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 1H-Benzotriazole Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.339	2.70 ng/ul	396326	Acenaphthene-d10	14.727

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	1H-Benzotriazole			119	C6H5N3	000095-14-7	98
2	1H-Benzotriazole			119	C6H5N3	000095-14-7	97
3	1H-Benzotriazole			119	C6H5N3	000095-14-7	96
4	1H-Benzotriazole			119	C6H5N3	000095-14-7	96
5	Benzoxazole			119	C7H5NO	000273-53-0	89

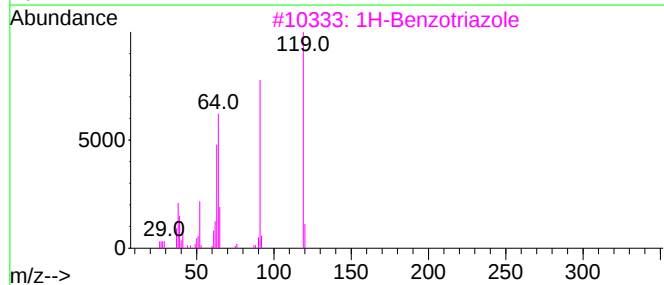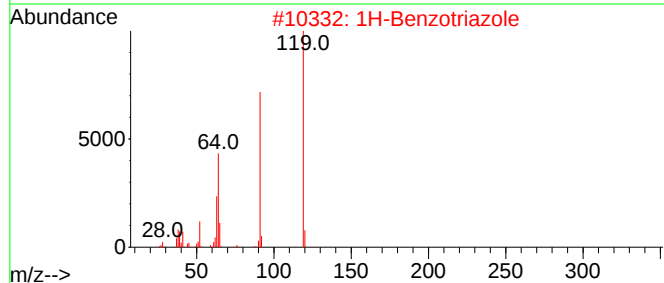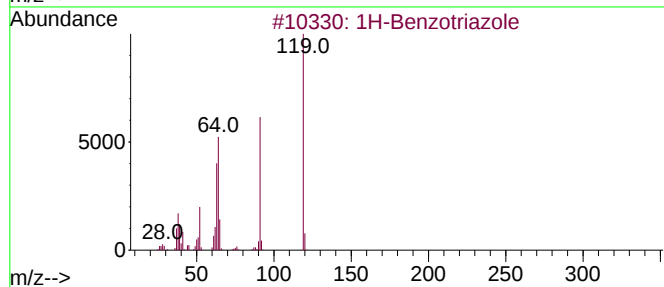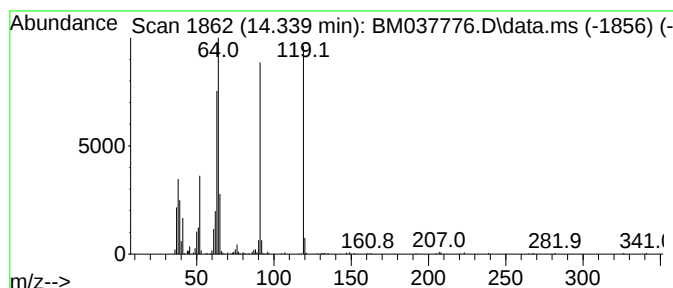

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112822\
Data File : BM037776.D
Acq On : 29 Nov 2022 01:51
Operator : CG/JU
Sample : N5710-01
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0KY0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1H-Benzotriazole	14.339	2.7	ng/u1	396326	3	14.727	2936810	20.0