

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112822\
 Data File : BM037777.D
 Acq On : 29 Nov 2022 02:27
 Operator : CG/JU
 Sample : N5710-02
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COKY1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037777.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.469	10	14	22	rVB	318389	455254	6.85%	0.637%
2	3.769	62	65	73	rBV2	51776	91442	1.38%	0.128%
3	3.875	80	83	95	rBV	284329	487379	7.34%	0.682%
4	4.757	228	233	243	rVB	534690	808516	12.17%	1.132%
5	5.504	356	360	366	rVB	59688	83046	1.25%	0.116%
6	6.299	491	495	501	rBV3	23952	43107	0.65%	0.060%
7	6.357	501	505	510	rVB	24164	36432	0.55%	0.051%
8	6.499	525	529	534	rBV	14002	23586	0.36%	0.033%
9	6.904	595	598	603	rBV2	29013	41505	0.62%	0.058%
10	6.963	603	608	615	rVB	85242	132660	2.00%	0.186%
11	7.093	627	630	635	rVV	22894	31235	0.47%	0.044%
12	7.146	636	639	643	rVB	22134	29670	0.45%	0.042%
13	7.251	651	657	664	rVB	367105	562973	8.47%	0.788%
14	7.334	667	671	675	rVB6	14494	24357	0.37%	0.034%
15	7.428	678	687	692	rBV	1002280	1665557	25.07%	2.332%
16	7.587	709	714	715	rBV3	17964	26806	0.40%	0.038%
17	7.628	715	721	728	rVB	1064580	1655610	24.92%	2.318%
18	7.793	746	749	754	rVB6	10396	15103	0.23%	0.021%
19	7.893	762	766	771	rBV7	9113	14520	0.22%	0.020%
20	8.104	795	802	809	rBV	980590	1518846	22.86%	2.127%
21	8.193	815	817	825	rVB8	9101	16681	0.25%	0.023%
22	8.645	890	894	902	rVB7	9164	19081	0.29%	0.027%
23	8.810	910	922	931	rBV	929962	1458873	21.96%	2.043%
24	8.904	934	938	942	rBV7	8627	15747	0.24%	0.022%
25	9.151	975	980	985	rBV2	18581	33403	0.50%	0.047%
26	9.275	993	1001	1008	rBV	1414356	2227674	33.53%	3.119%
27	9.375	1014	1018	1025	rVB4	25629	45835	0.69%	0.064%
28	9.498	1035	1039	1042	rVB7	8270	12105	0.18%	0.017%
29	9.540	1042	1046	1050	rBV4	5930	9761	0.15%	0.014%
30	9.675	1062	1069	1078	rVB9	26254	65952	0.99%	0.092%
31	9.845	1095	1098	1106	rVB10	5475	10127	0.15%	0.014%
32	9.928	1108	1112	1116	rBV4	11093	22898	0.34%	0.032%
33	9.998	1116	1124	1135	rVV	1170607	1948368	29.33%	2.728%
34	10.151	1146	1150	1156	rVB	36790	57787	0.87%	0.081%
35	10.216	1156	1161	1162	rBV5	6169	8766	0.13%	0.012%
36	10.228	1162	1163	1169	rVB6	7025	10255	0.15%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112822\
 Data File : BM037777.D
 Acq On : 29 Nov 2022 02:27
 Operator : CG/JU
 Sample : N5710-02
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COKY1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
 Title : SVOA CALIBRATION

37	10.328	1176	1180	1182	rBV4	6247	8429	0.13%	0.012%
38	10.416	1190	1195	1199	rBV8	4187	9650	0.15%	0.014%
39	10.469	1202	1204	1208	rVB5	7347	10477	0.16%	0.015%
40	10.539	1208	1216	1224	rBV	1493597	2364024	35.58%	3.310%
41	10.657	1232	1236	1241	rVV6	11443	16714	0.25%	0.023%
42	10.722	1241	1247	1255	rVB10	18108	40222	0.61%	0.056%
43	10.928	1273	1282	1289	rBV	1401786	2326518	35.02%	3.258%
44	11.016	1289	1297	1298	rBV	35901	52355	0.79%	0.073%
45	11.063	1298	1305	1318	rVB	1345581	2330125	35.07%	3.263%
46	11.381	1354	1359	1363	rVB7	13604	23499	0.35%	0.033%
47	11.592	1386	1395	1400	rBV9	10613	22834	0.34%	0.032%
48	11.733	1415	1419	1424	rVB4	18209	30613	0.46%	0.043%
49	11.886	1442	1445	1451	rVB8	6480	9582	0.14%	0.013%
50	11.963	1451	1458	1461	rBV9	8479	17563	0.26%	0.025%
51	12.122	1481	1485	1490	rBV3	8900	17409	0.26%	0.024%
52	12.251	1503	1507	1513	rVB3	18730	28681	0.43%	0.040%
53	12.369	1520	1527	1528	rBV5	5490	9518	0.14%	0.013%
54	12.498	1542	1549	1557	rVB	31815	62291	0.94%	0.087%
55	12.598	1562	1566	1569	rVB6	10134	15591	0.23%	0.022%
56	12.733	1586	1589	1594	rVB4	11970	17620	0.27%	0.025%
57	12.898	1611	1617	1619	rBV8	4397	9954	0.15%	0.014%
58	13.098	1647	1651	1656	rBV8	8828	15868	0.24%	0.022%
59	13.269	1674	1680	1686	rBV	103369	166487	2.51%	0.233%
60	13.339	1686	1692	1696	rVV5	15783	24987	0.38%	0.035%
61	13.598	1730	1736	1737	rBV6	14221	22327	0.34%	0.031%
62	13.622	1737	1740	1746	rVB3	30071	44902	0.68%	0.063%
63	13.857	1775	1780	1784	rVV3	9643	17672	0.27%	0.025%
64	13.922	1787	1791	1794	rBV6	4959	8409	0.13%	0.012%
65	14.133	1821	1827	1837	rBV	2632422	3673504	55.30%	5.144%
66	14.339	1853	1862	1870	rBV	236660	409400	6.16%	0.573%
67	14.427	1870	1877	1887	rVB2	3074783	4404912	66.31%	6.168%
68	14.733	1920	1929	1938	rBV	2032597	3002401	45.19%	4.204%
69	14.910	1950	1959	1970	rBV	370430	563778	8.49%	0.789%
70	15.045	1978	1982	1985	rBV2	8073	10243	0.15%	0.014%
71	15.127	1991	1996	2003	rVB9	33308	52550	0.79%	0.074%
72	15.210	2005	2010	2016	rBV6	21128	35453	0.53%	0.050%
73	15.298	2017	2025	2035	rBV	72977	178948	2.69%	0.251%
74	15.533	2057	2065	2069	rBV4	10484	23904	0.36%	0.033%
75	15.639	2079	2083	2086	rVB6	7734	10626	0.16%	0.015%
76	15.716	2086	2096	2101	rBV	3729255	5365377	80.76%	7.513%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112822\
 Data File : BM037777.D
 Acq On : 29 Nov 2022 02:27
 Operator : CG/JU
 Sample : N5710-02
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COKY1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
 Title : SVOA CALIBRATION

77	15.757	2101	2103	2109	rVV	129214	150453	2.26%	0.211%
78	15.827	2109	2115	2128	rVV	1295653	1800017	27.09%	2.521%
79	15.957	2132	2137	2142	rVB5	23611	35861	0.54%	0.050%
80	16.069	2153	2156	2161	rVB7	8857	12733	0.19%	0.018%
81	16.257	2183	2188	2197	rBV7	10475	28804	0.43%	0.040%
82	16.363	2199	2206	2212	rBV	84848	159187	2.40%	0.223%
83	16.580	2240	2243	2250	rVB7	11670	17691	0.27%	0.025%
84	16.757	2268	2273	2275	rBV6	10524	16489	0.25%	0.023%
85	16.921	2295	2301	2306	rBV7	10482	24063	0.36%	0.034%
86	16.980	2306	2311	2317	rBV3	88718	143064	2.15%	0.200%
87	17.221	2346	2352	2356	rBV6	37272	72102	1.09%	0.101%
88	17.327	2368	2370	2374	rBV5	9077	9843	0.15%	0.014%
89	17.468	2387	2394	2400	rBV	2501252	3445999	51.87%	4.825%
90	17.568	2404	2411	2420	rBV	4249040	6021329	90.64%	8.432%
91	18.339	2537	2542	2552	rBV2	127018	191391	2.88%	0.268%
92	19.415	2721	2725	2729	rBV3	57922	73960	1.11%	0.104%
93	19.480	2733	2736	2740	rVV	50535	63366	0.95%	0.089%
94	19.604	2754	2757	2765	rBV	130433	166089	2.50%	0.233%
95	19.845	2792	2798	2805	rBV	5163551	6643372	100.00%	9.303%
96	20.815	2961	2963	2967	rVB2	65034	64200	0.97%	0.090%
97	21.627	3096	3101	3108	rBV2	2758565	3652344	54.98%	5.114%
98	23.956	3490	3497	3509	rVB2	2749453	5934591	89.33%	8.310%
99	24.121	3518	3525	3535	rVB2	1541152	3093503	46.57%	4.332%
100	24.727	3625	3628	3635	rVB	240400	426684	6.42%	0.597%




Sum of corrected areas: 71413469

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112822\
Data File : BM037777.D
Acq On : 29 Nov 2022 02:27
Operator : CG/JU
Sample : N5710-02
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0KY1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

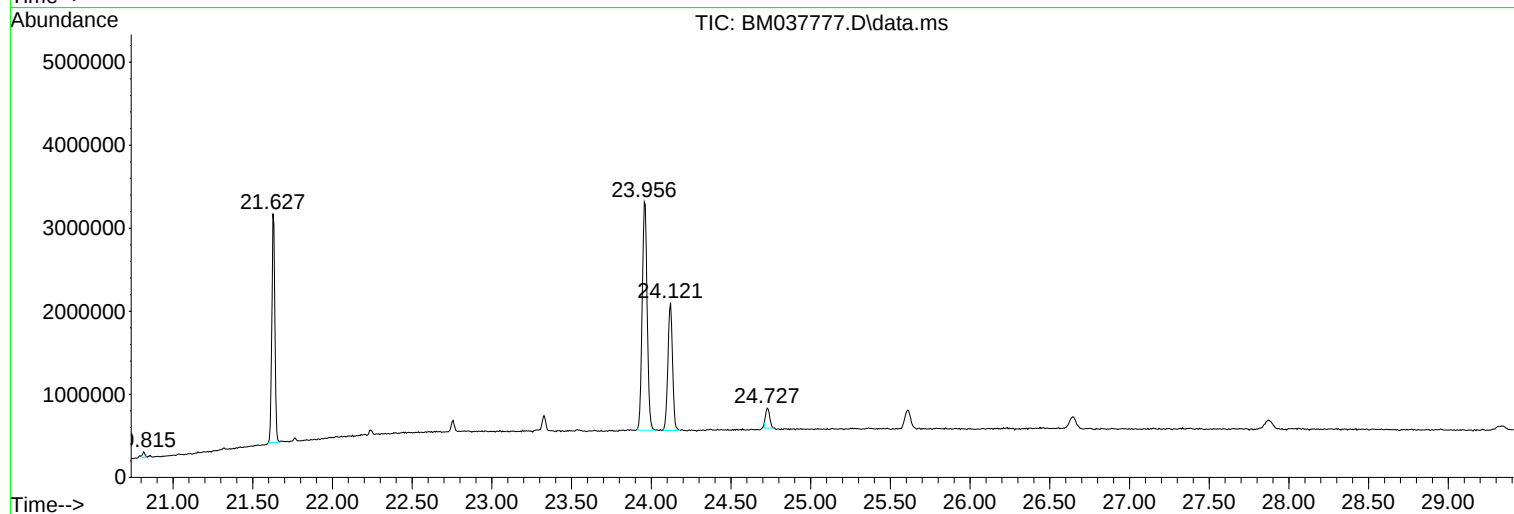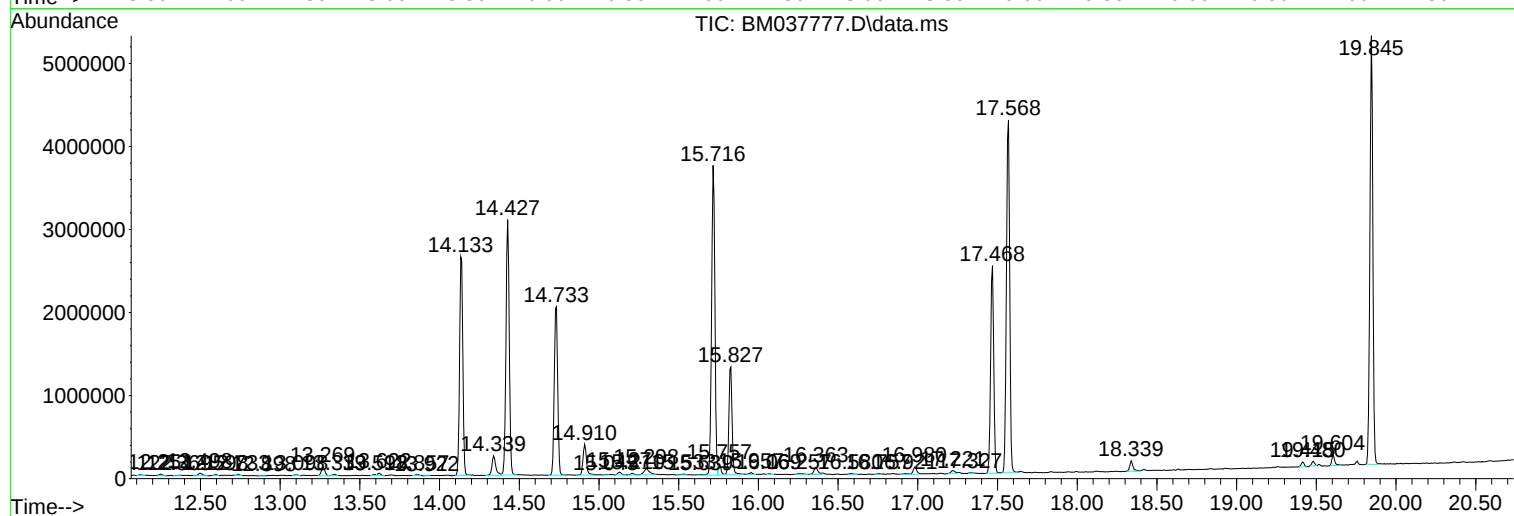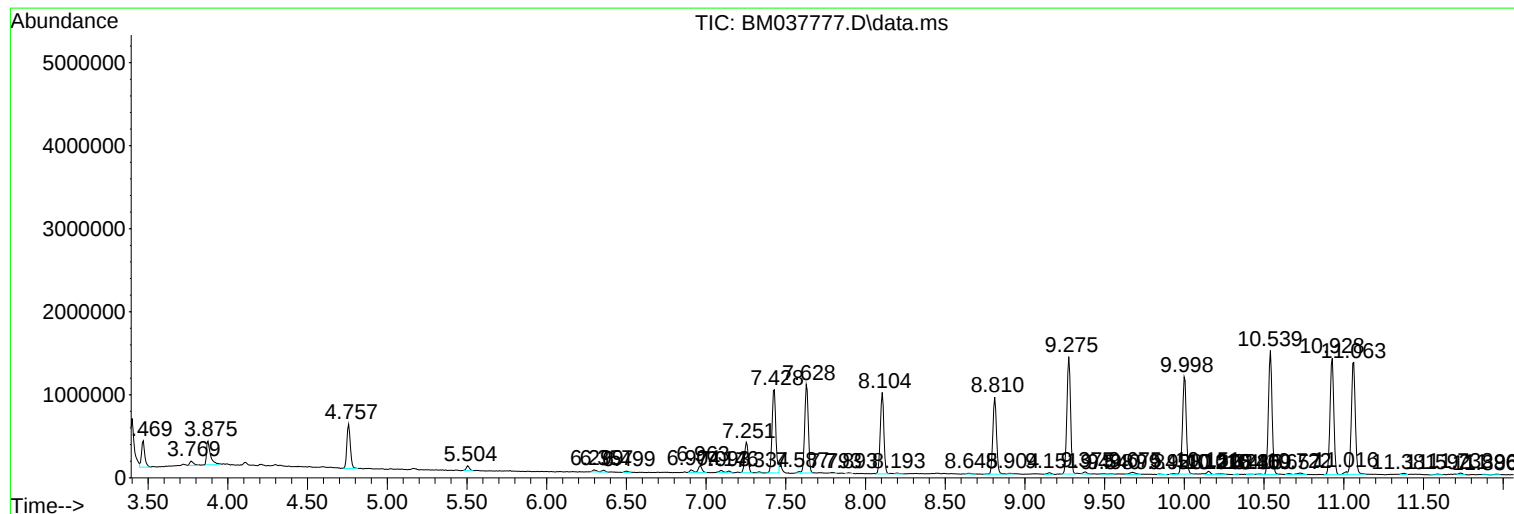

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112822\
Data File : BM037777.D
Acq On : 29 Nov 2022 02:27
Operator : CG/JU
Sample : N5710-02
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0KY1










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 1H-Benzotriazole Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.339	2.73 ng/ul	409400	Acenaphthene-d10	14.733

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	1H-Benzotriazole			119	C6H5N3	000095-14-7	98
2	1H-Benzotriazole			119	C6H5N3	000095-14-7	98
3	1H-Benzotriazole			119	C6H5N3	000095-14-7	96
4	1H-Benzotriazole			119	C6H5N3	000095-14-7	96
5	Ethane-1,2-diol, 1,2-bis(1-benzo...			296	C14H12N6O2	111507-88-1	91

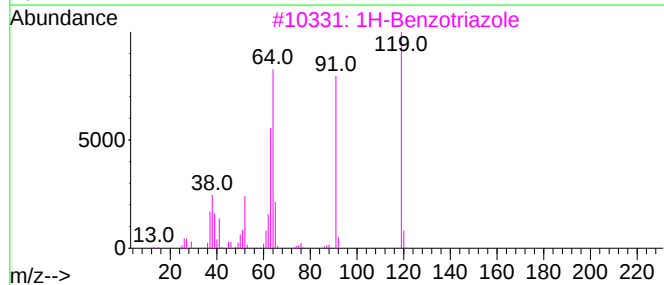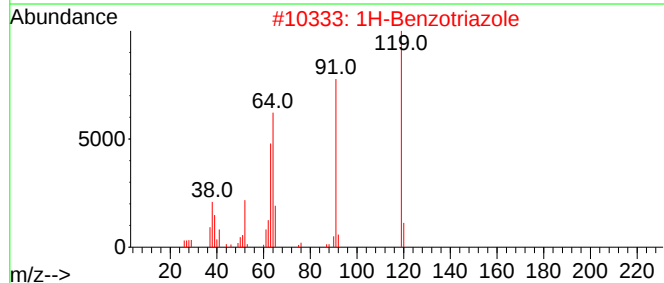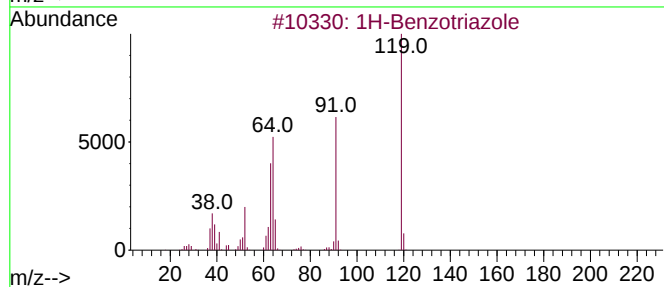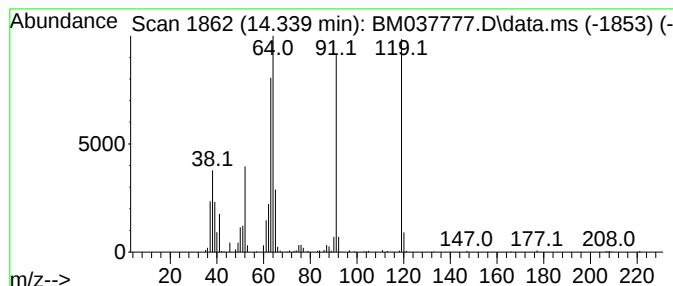

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112822\
Data File : BM037777.D
Acq On : 29 Nov 2022 02:27
Operator : CG/JU
Sample : N5710-02
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0KY1










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 (DEL) Alkane: Straight-Chai... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
24.727	2.76 ng/ul	426684	Perylene-d12	24.121

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Eicosane	282	C20H42	000112-95-8	90
2			Eicosane	282	C20H42	000112-95-8	89
3			Tetracosane	338	C24H50	000646-31-1	83
4			Heneicosane	296	C21H44	000629-94-7	83
5			Octacosane, 2-methyl-	408	C29H60	001560-98-1	83

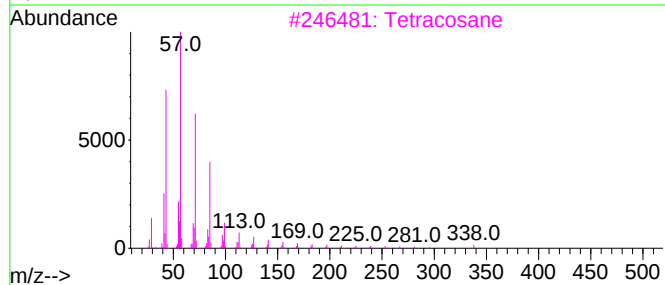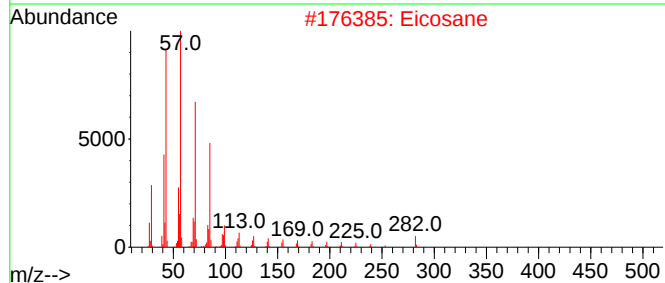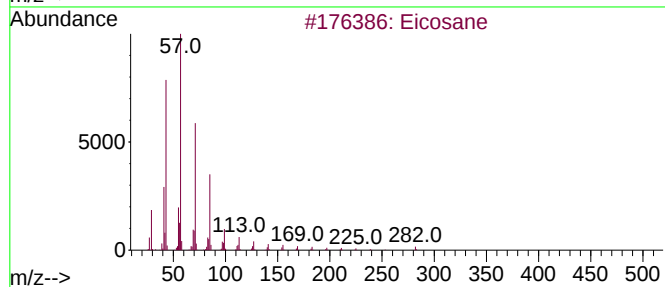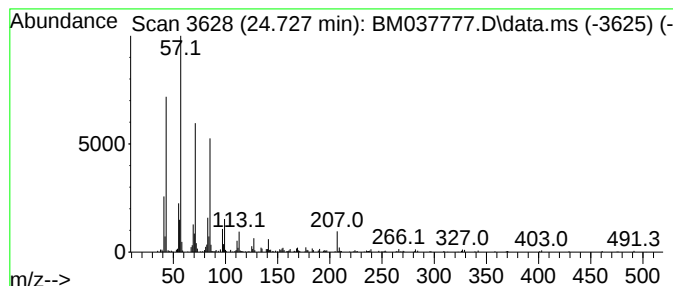

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112822\
Data File : BM037777.D
Acq On : 29 Nov 2022 02:27
Operator : CG/JU
Sample : N5710-02
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0KY1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1H-Benzotriazole	14.339	2.7	ng/u1	409400	3	14.733	3002400	20.0
(DEL) Alkane: S...	24.727	2.8	ng/u1	426684	6	24.121	3093500	20.0