

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112822\
 Data File : BM037778.D
 Acq On : 29 Nov 2022 03:04
 Operator : CG/JU
 Sample : N5710-03
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COKY2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037778.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.769	62	65	75	rVB	54650	89088	1.56%	0.148%
2	3.875	80	83	97	rBV	216492	367117	6.44%	0.610%
3	4.757	227	233	244	rVB	776403	1203404	21.10%	2.000%
4	5.345	329	333	344	rVB4	36563	78096	1.37%	0.130%
5	5.604	375	377	383	rVB4	9897	12650	0.22%	0.021%
6	6.498	525	529	536	rVB	28654	45636	0.80%	0.076%
7	7.251	652	657	668	rVB	342259	530163	9.29%	0.881%
8	7.428	679	687	696	rBV	911949	1437706	25.21%	2.389%
9	7.628	714	721	730	rBV	946758	1502702	26.34%	2.497%
10	7.716	733	736	741	rVB6	6220	9739	0.17%	0.016%
11	8.051	790	793	795	rBV4	7136	8918	0.16%	0.015%
12	8.104	795	802	809	rVB	904206	1370756	24.03%	2.278%
13	8.810	915	922	931	rBV	802200	1252688	21.96%	2.082%
14	9.275	992	1001	1008	rBV	1263178	1997114	35.01%	3.319%
15	9.380	1012	1019	1029	rVV2	38535	71703	1.26%	0.119%
16	9.680	1066	1070	1077	rVB3	17044	31659	0.56%	0.053%
17	9.845	1093	1098	1105	rVB8	8936	16982	0.30%	0.028%
18	9.998	1117	1124	1133	rBV	965381	1587513	27.83%	2.638%
19	10.128	1142	1146	1156	rVB4	15498	31630	0.55%	0.053%
20	10.286	1167	1173	1178	rVB5	13882	24090	0.42%	0.040%
21	10.539	1209	1216	1228	rBV	1236867	2018143	35.38%	3.354%
22	10.657	1233	1236	1241	rVB6	4010	6135	0.11%	0.010%
23	10.786	1254	1258	1264	rVB7	7773	15656	0.27%	0.026%
24	10.927	1274	1282	1291	rBV	1257525	2081853	36.50%	3.460%
25	10.998	1291	1294	1297	rVB4	4001	6195	0.11%	0.010%
26	11.057	1297	1304	1318	rBV	992721	1679924	29.45%	2.792%
27	11.427	1360	1367	1370	rBV8	3803	7818	0.14%	0.013%
28	11.692	1409	1412	1416	rBV6	9109	15987	0.28%	0.027%
29	11.739	1416	1420	1426	rVB8	12908	20110	0.35%	0.033%
30	11.798	1426	1430	1436	rBV5	9929	15323	0.27%	0.025%
31	12.045	1466	1472	1478	rBV9	13574	31160	0.55%	0.052%
32	12.169	1488	1493	1499	rVB5	10651	21014	0.37%	0.035%
33	12.321	1513	1519	1522	rBV6	11483	18870	0.33%	0.031%
34	12.498	1545	1549	1555	rVB2	25091	38938	0.68%	0.065%
35	12.780	1592	1597	1600	rVB7	5388	8222	0.14%	0.014%
36	12.951	1621	1626	1628	rVB5	4768	6055	0.11%	0.010%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112822\
 Data File : BM037778.D
 Acq On : 29 Nov 2022 03:04
 Operator : CG/JU
 Sample : N5710-03
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COKY2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
 Title : SVOA CALIBRATION

37	13.127	1652	1656	1659	rVB5	5122	7128	0.12%	0.012%
38	13.339	1687	1692	1694	rBV6	5861	7606	0.13%	0.013%
39	13.468	1710	1714	1718	rVB7	5252	7967	0.14%	0.013%
40	13.551	1718	1728	1733	rBV4	20855	37454	0.66%	0.062%

41	13.621	1735	1740	1745	rBV4	16937	29999	0.53%	0.050%
42	13.710	1750	1755	1757	rVB5	5494	8699	0.15%	0.014%
43	14.133	1821	1827	1838	rBV	2359017	3223496	56.51%	5.357%
44	14.427	1870	1877	1884	rBV	2609825	3738150	65.54%	6.212%
45	14.510	1887	1891	1894	rBV	22536	30333	0.53%	0.050%

46	14.610	1902	1908	1913	rBV8	7960	12442	0.22%	0.021%
47	14.727	1919	1928	1938	rBV	1735754	2628143	46.08%	4.368%
48	14.810	1938	1942	1946	rVB6	5755	8198	0.14%	0.014%
49	14.910	1953	1959	1973	rBV	331051	506853	8.89%	0.842%
50	15.133	1992	1997	2002	rVB8	16858	27871	0.49%	0.046%

51	15.292	2020	2024	2027	rBV6	5532	8663	0.15%	0.014%
52	15.492	2054	2058	2061	rBV5	5710	9380	0.16%	0.016%
53	15.557	2064	2069	2072	rVB7	6584	10958	0.19%	0.018%
54	15.715	2088	2096	2103	rBV	3390219	4603509	80.71%	7.650%
55	15.827	2108	2115	2126	rVV	1150413	1609223	28.21%	2.674%

56	15.957	2132	2137	2142	rVB4	16956	25296	0.44%	0.042%
57	16.074	2153	2157	2161	rBV7	5994	8047	0.14%	0.013%
58	16.404	2207	2213	2219	rVB7	8766	16555	0.29%	0.028%
59	16.845	2286	2288	2291	rBV4	7658	8693	0.15%	0.014%
60	16.927	2298	2302	2307	rVB7	6301	10499	0.18%	0.017%

61	16.992	2310	2313	2316	rVB4	6503	6823	0.12%	0.011%
62	17.204	2343	2349	2353	rBV8	6823	13146	0.23%	0.022%
63	17.256	2355	2358	2362	rVB5	6664	10019	0.18%	0.017%
64	17.339	2369	2372	2376	rBV5	9753	13177	0.23%	0.022%
65	17.468	2387	2394	2404	rBV	2162692	3018395	52.92%	5.016%

66	17.568	2404	2411	2421	rVV	3552982	5089696	89.23%	8.458%
67	17.639	2421	2423	2433	rVB9	26030	44500	0.78%	0.074%
68	17.739	2438	2440	2444	rVV4	5152	7092	0.12%	0.012%
69	17.839	2453	2457	2462	rVB7	15654	20109	0.35%	0.033%
70	17.945	2472	2475	2480	rVB7	8965	14465	0.25%	0.024%

71	17.992	2480	2483	2490	rBV9	9037	19244	0.34%	0.032%
72	18.121	2501	2505	2509	rVB6	12583	18166	0.32%	0.030%
73	18.339	2538	2542	2549	rBV	173718	233550	4.09%	0.388%
74	18.633	2589	2592	2596	rBV5	9695	13942	0.24%	0.023%
75	18.762	2610	2614	2618	rBV	78908	89957	1.58%	0.149%

76	18.839	2623	2627	2631	rVB3	32196	42676	0.75%	0.071%
----	--------	------	------	------	------	-------	-------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112822\
 Data File : BM037778.D
 Acq On : 29 Nov 2022 03:04
 Operator : CG/JU
 Sample : N5710-03
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COKY2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
 Title : SVOA CALIBRATION

77	19.415	2721	2725	2729	rVB2	44816	57860	1.01%	0.096%
78	19.480	2731	2736	2740	rVV2	53849	87244	1.53%	0.145%
79	19.515	2740	2742	2746	rVB4	17047	19552	0.34%	0.032%
80	19.609	2753	2758	2764	rBV	116715	173628	3.04%	0.289%
81	19.750	2780	2782	2789	rVB3	30039	37492	0.66%	0.062%
82	19.845	2792	2798	2807	rBV	4404506	5703977	100.00%	9.479%
83	20.815	2961	2963	2967	rVB	53605	55024	0.96%	0.091%
84	21.315	3045	3048	3056	rBV	145572	215428	3.78%	0.358%
85	21.633	3096	3102	3107	rBV	2384820	3157650	55.36%	5.248%
86	23.956	3490	3497	3510	rVB2	2308188	5008520	87.81%	8.323%
87	24.121	3518	3525	3534	rVB2	1357676	2756244	48.32%	4.580%




Sum of corrected areas: 60173495

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112822\
Data File : BM037778.D
Acq On : 29 Nov 2022 03:04
Operator : CG/JU
Sample : N5710-03
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0KY2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

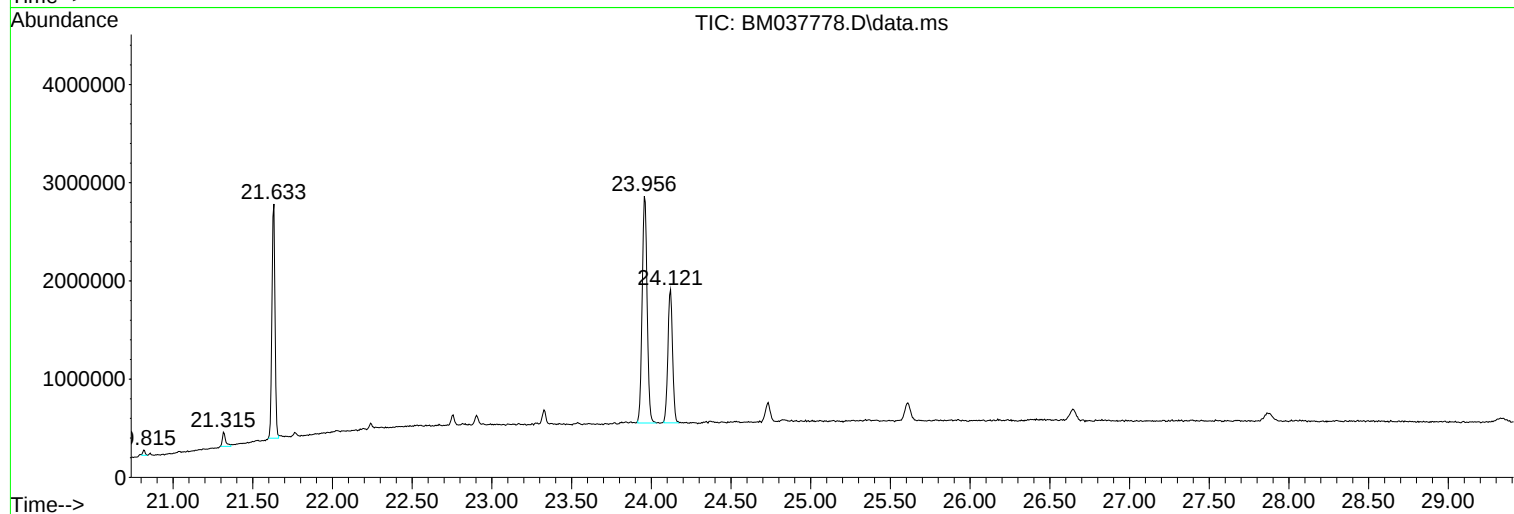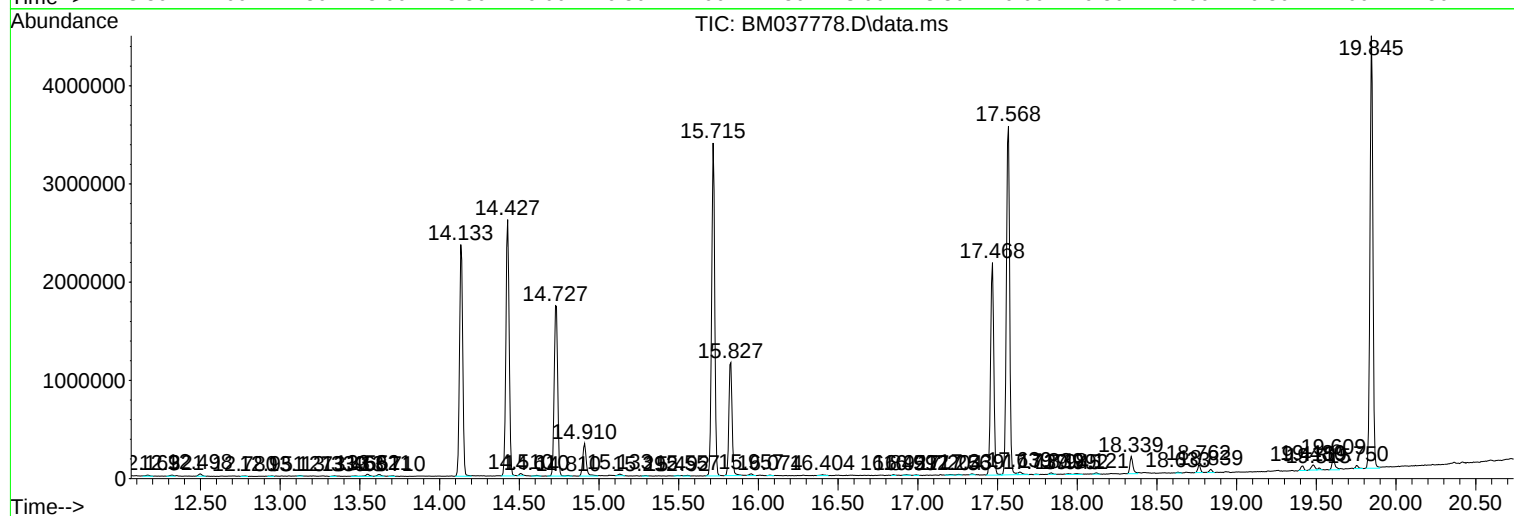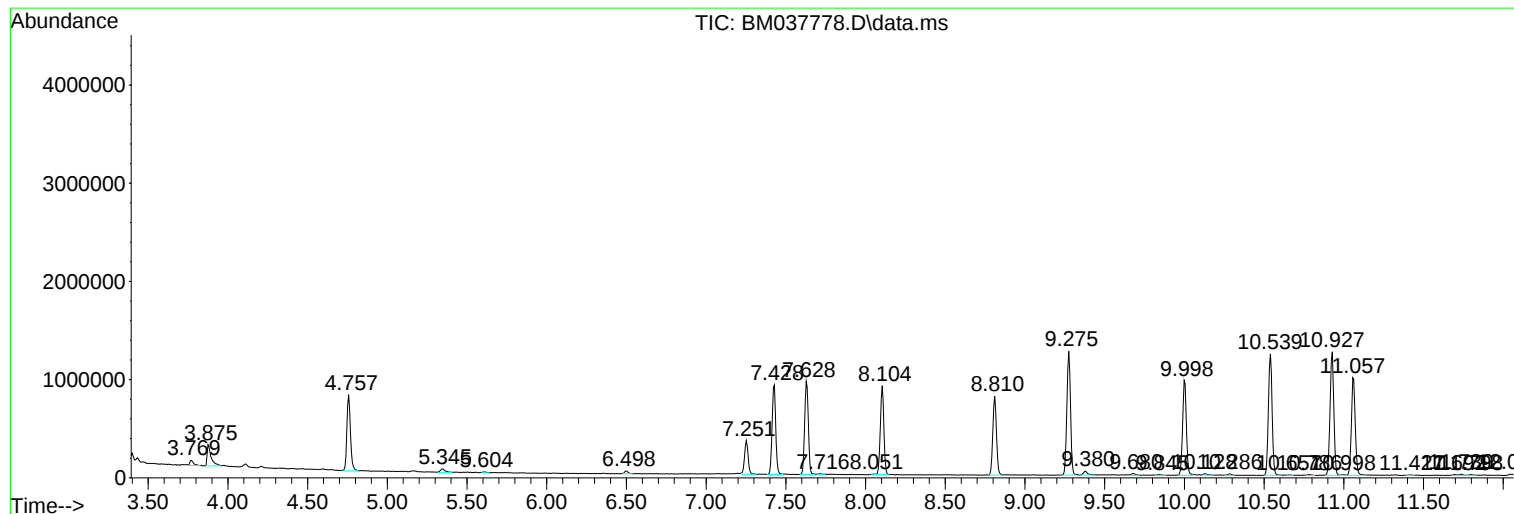

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112822\
Data File : BM037778.D
Acq On : 29 Nov 2022 03:04
Operator : CG/JU
Sample : N5710-03
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0KY2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112822\
Data File : BM037778.D
Acq On : 29 Nov 2022 03:04
Operator : CG/JU
Sample : N5710-03
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0KY2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc