

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM112918\
 Data File : BM017805.D
 Acq On : 29 Nov 2018 20:46
 Operator : JU/SJ
 Sample : J6038-13
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB4J7

Quant Time: Nov 30 00:35:54 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Nov 29 00:55:29 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	250453	20.00	ng/ul	0.00
18) Naphthalene-d8	10.36	136	1055446	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.23	164	624679	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.99	188	1339673	20.00	ng/ul	0.00
77) Chrysene-d12	21.19	240	1102841	20.00	ng/ul	0.00
85) Perylene-d12	23.37	264	931194	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	0.00	96	0	0.00	ng/uL	
5) Phenol-d5	6.80	99	394	0.02	ng/ul	0.02
7) Bis-(2-Chloroethyl)ether-d	6.91	67	4132	0.30	ng/ul	-0.03
9) 2-Chlorophenol-d4	0.00	132	0	0.00	ng/ul	
13) 4-Methylphenol-d8	8.23	113	1676	0.09	ng/ul	-0.06
19) Nitrobenzene-d5	8.75	128	176	0.02	ng/ul	0.00
22) 2-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
26) 2,4-Dichlorophenol-d3	10.07	165	379	0.02	ng/ul	0.09
29) 4-Chloroaniline-d4	10.47	131	23558	1.55	ng/ul	-0.04
43) Dimethylphthalate-d6	13.63	166	627	0.01	ng/ul	-0.03
46) Acenaphthylene-d8	13.93	160	365	0.01	ng/ul	0.00
51) 4-Nitrophenol-d4	14.46	143	2428	0.25	ng/ul	0.00
57) Fluorene-d10	15.24	176	4744	0.10	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.37	200	99	0.01	ng/ul	0.00
70) Anthracene-d10	16.99	188	1339673	20.09	ng/ul	-0.11
78) Pyrene-d10	19.39	212	296	0.01	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.37	264	926045	18.34	ng/ul	0.13

Target Compounds


					Qvalue	
58) Fluorene	15.29	166	62286	1.195	ng/ul#	96
69) Phenanthrene	17.03	178	557403	7.276	ng/ul	100
76) Fluoranthene	19.06	202	1132597	12.569	ng/ul	99
79) Pyrene	19.42	202	743240	11.102	ng/ul	99
82) Benzo(a)anthracene	21.17	228	383011	5.599	ng/ul	99
84) Chrysene	21.23	228	364627	5.700	ng/ul	99
87) Benzo(b)fluoranthene	22.73	252	241463	4.172	ng/ul#	92
88) Benzo(k)fluoranthene	22.77	252	86399	1.536	ng/ul#	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM112918\
Data File : BM017805.D
Acq On : 29 Nov 2018 20:46
Operator : JU/SJ
Sample : J6038-13
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB4J7

Quant Time: Nov 30 00:35:54 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Nov 29 00:55:29 2018
Response via : Initial Calibration




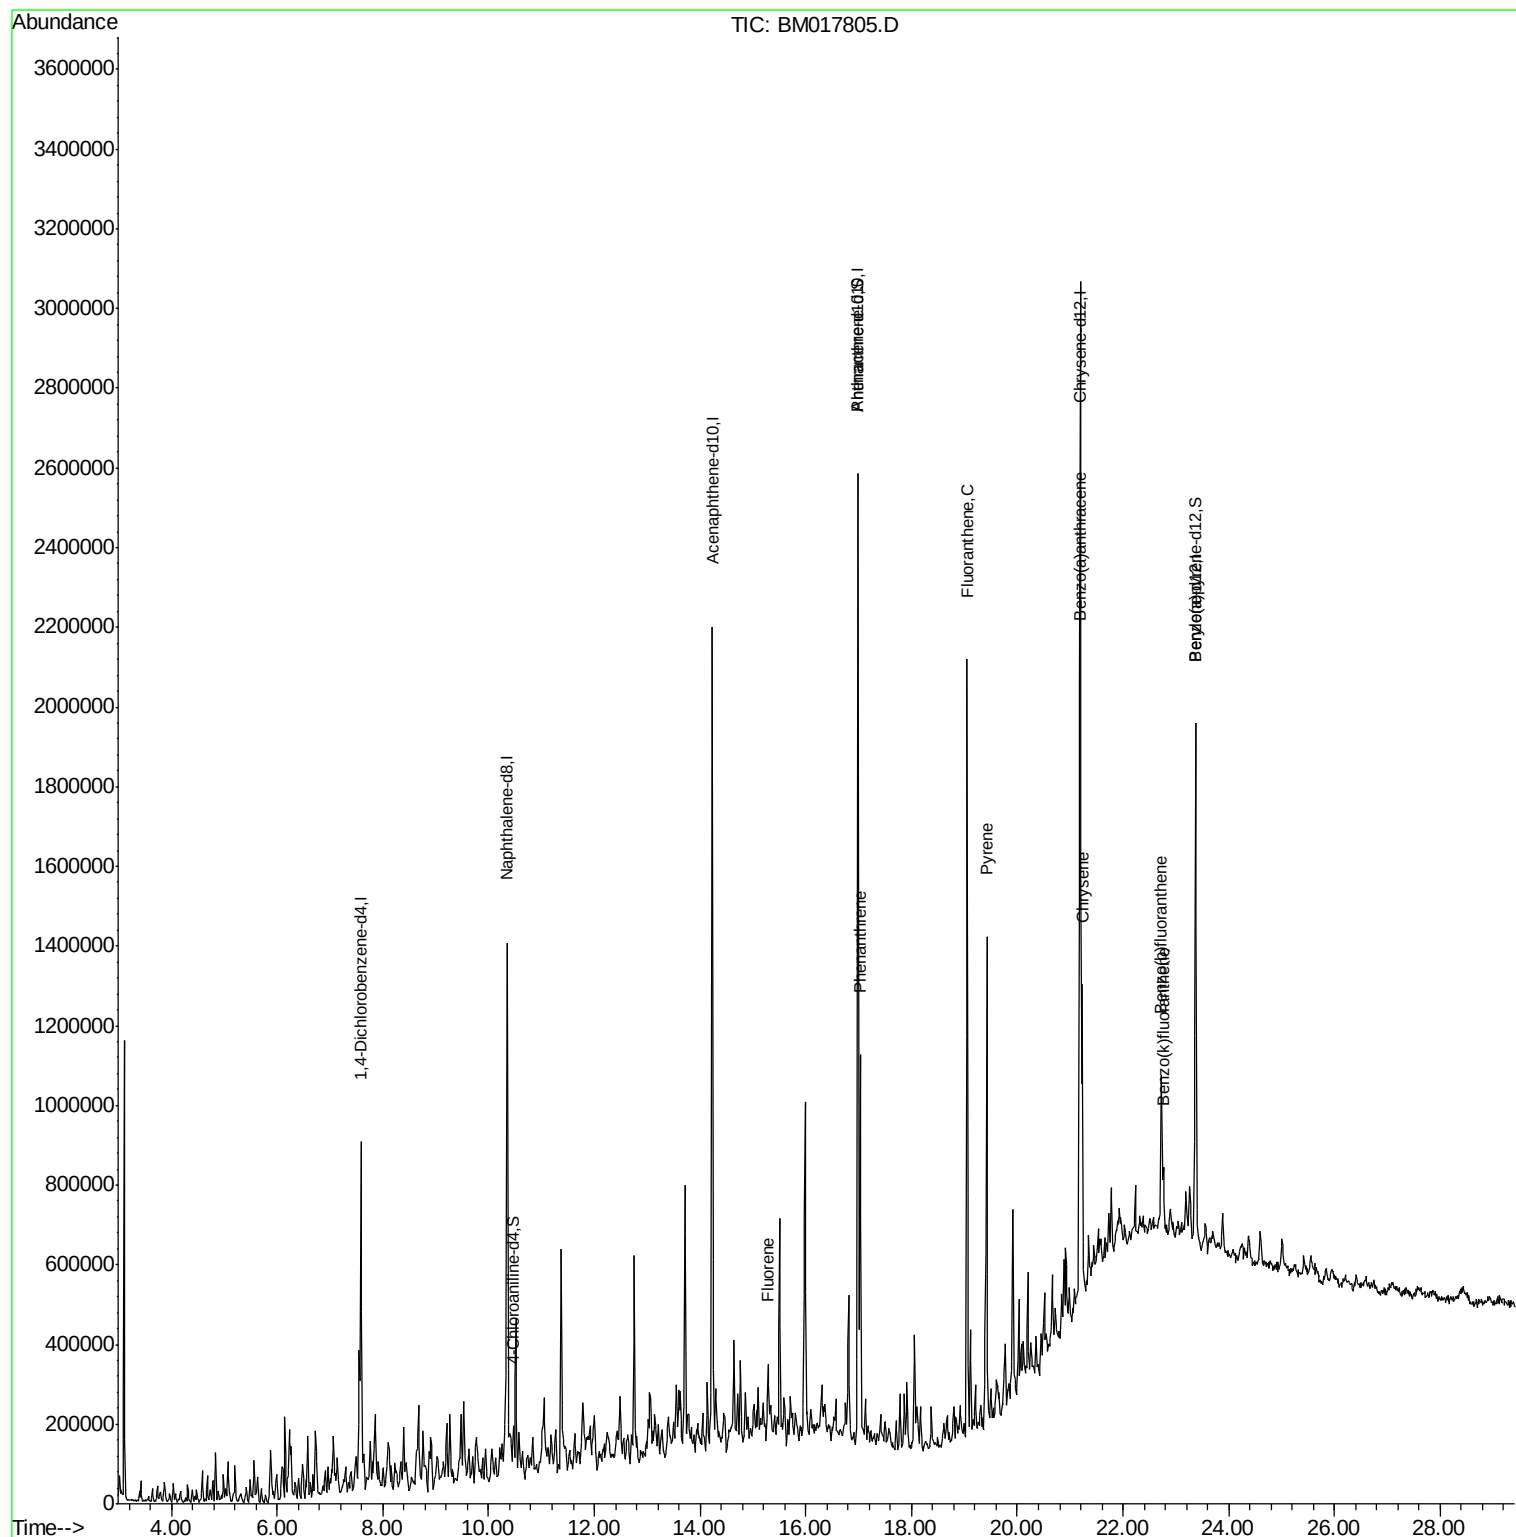


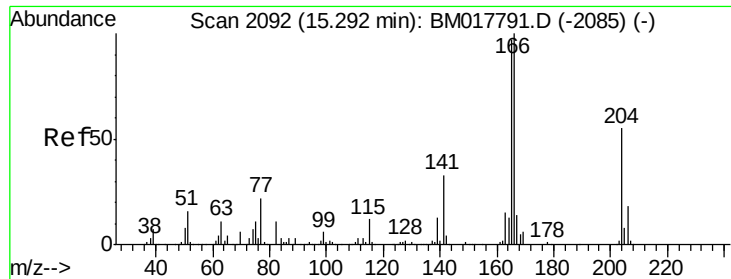

#58
 Fluorene
 Concen: 1.195 ng/ul
 RT: 15.29 min Scan# 2092
 Delta R.T. -0.00 min
 Lab File: BM017805.D
 Acq: 29 Nov 2018 20:46




Instrument :
 BNA_M
 ClientSampleId :
 CB4J7


Tgt Ion:166 Resp: 62286
 Ion Ratio Lower Upper
 166 100
 165 100.5 78.0 117.0
 167 16.8 10.8 16.2#

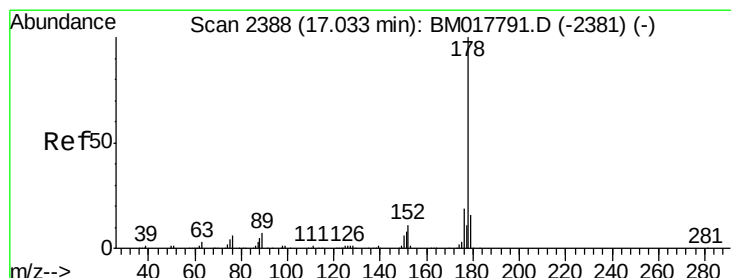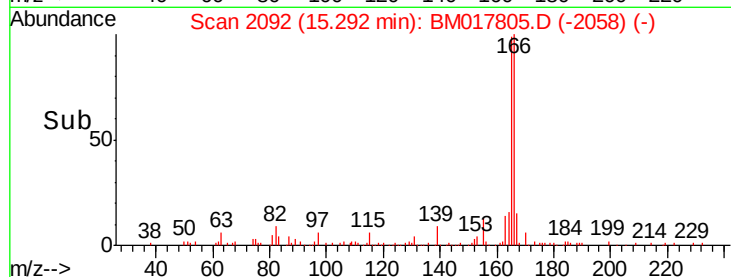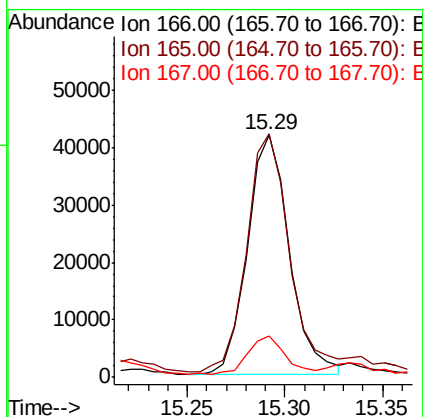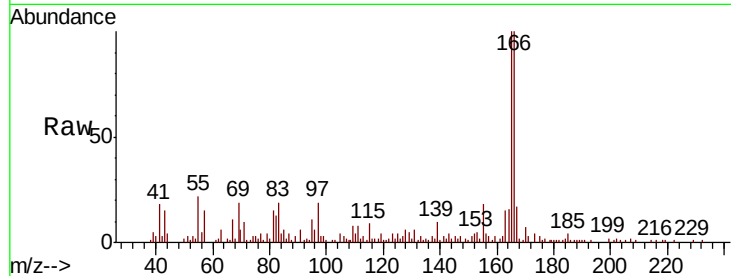

#69
 Phenanthrene
 Concen: 7.276 ng/ul
 RT: 17.03 min Scan# 2387
 Delta R.T. -0.01 min
 Lab File: BM017805.D
 Acq: 29 Nov 2018 20:46

Tgt Ion:178 Resp: 557403
 Ion Ratio Lower Upper
 178 100
 179 15.0 11.8 17.8
 176 19.1 15.0 22.6

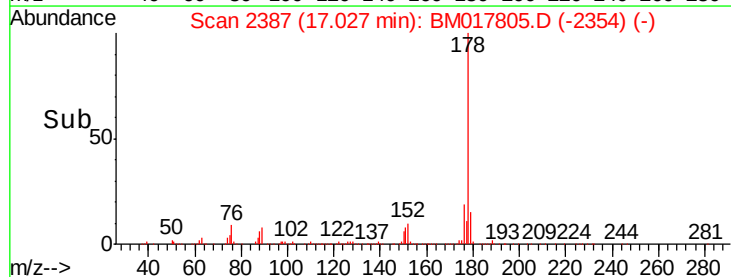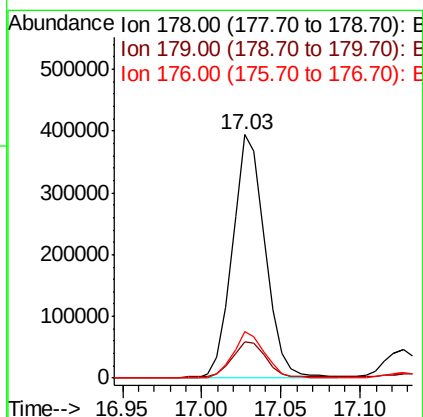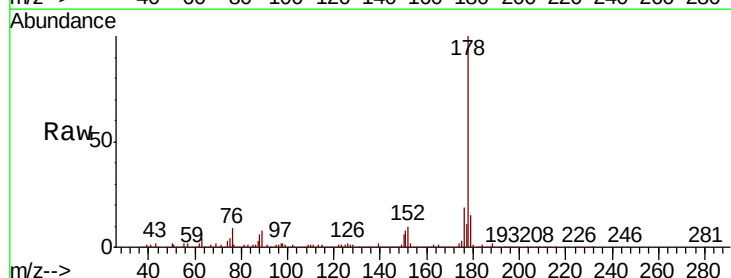

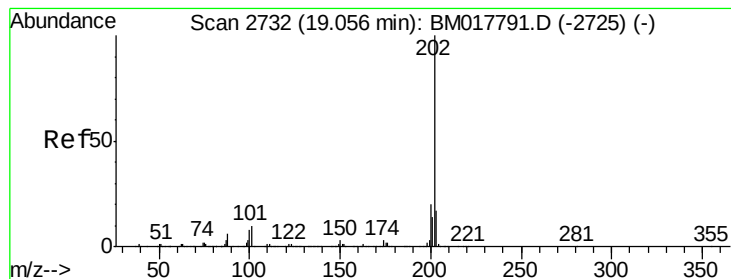

#76

Fluoranthene

Concen: 12.569 ng/ul

RT: 19.06 min Scan# 2732

Delta R.T. -0.01 min

Lab File: BM017805.D

Acq: 29 Nov 2018 20:46

Instrument :

BNA_M

ClientSampleId :

CB4J7


Tgt Ion:202 Resp: 1132597

Ion Ratio Lower Upper

202 100

101 10.7 8.4 12.6




100 8.4 6.6 9.8

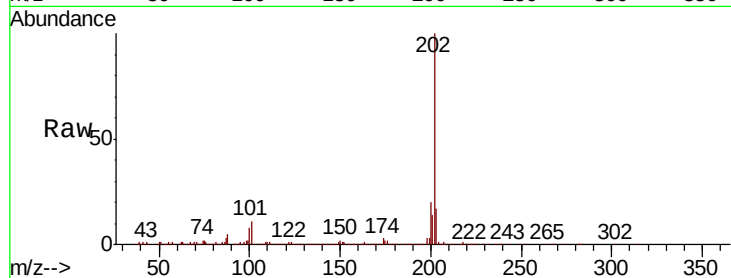

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

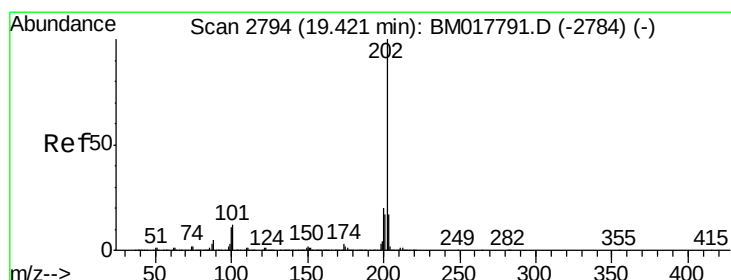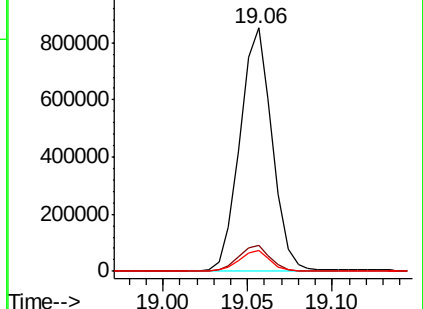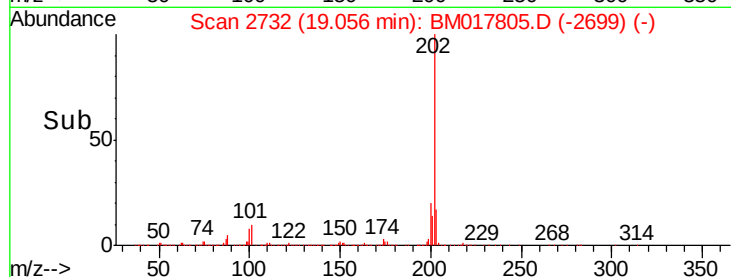

#79

Pyrene

Concen: 11.102 ng/ul

RT: 19.42 min Scan# 2794

Delta R.T. -0.01 min

Lab File: BM017805.D

Acq: 29 Nov 2018 20:46


Tgt Ion:202 Resp: 743240

Ion Ratio Lower Upper

202 100

101 11.6 9.6 14.4



100 10.3 7.9 11.9

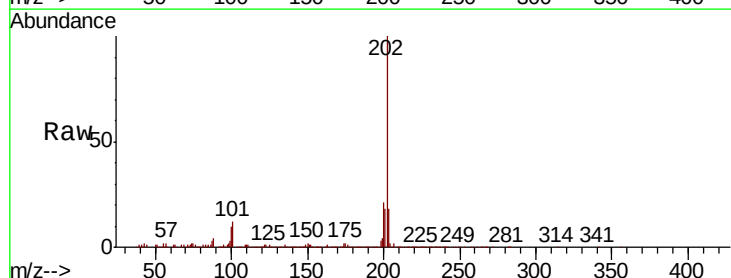


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B



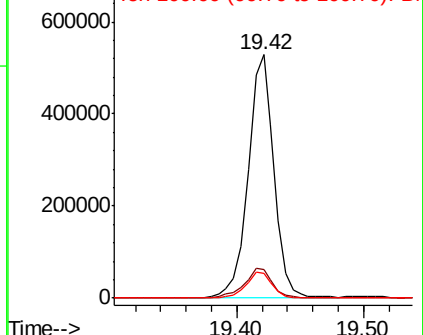
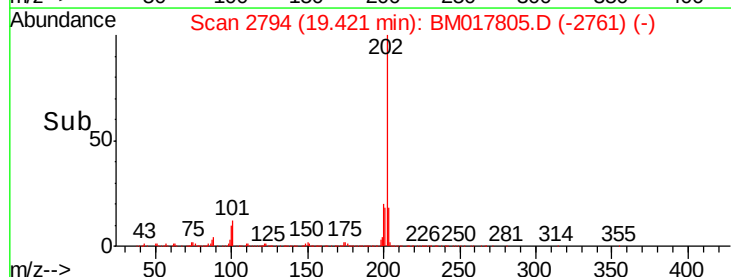


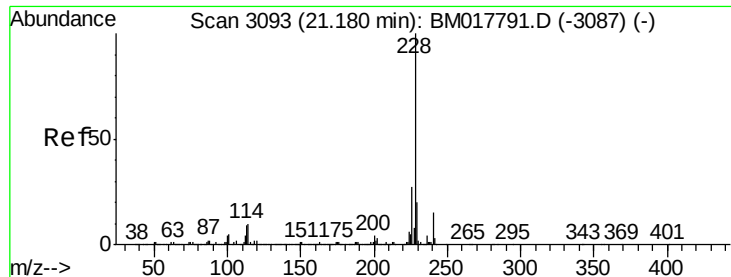

#82
Benzo(a)anthracene
Concen: 5.599 ng/ul
RT: 21.17 min Scan# 3092
Delta R.T. -0.01 min
Lab File: BM017805.D
Acq: 29 Nov 2018 20:46




Instrument :
BNA_M
ClientSampleId :
CB4J7


Tgt Ion:228 Resp: 383011
Ion Ratio Lower Upper
228 100
229 20.5 16.0 24.0
226 26.1 21.0 31.6

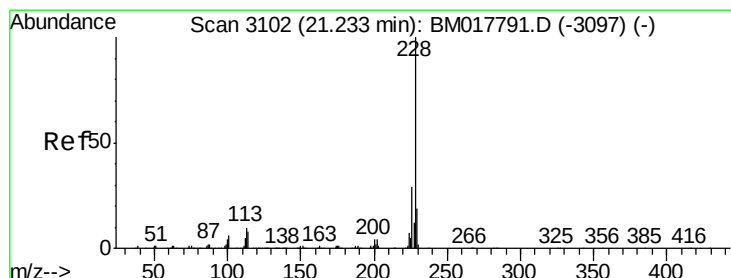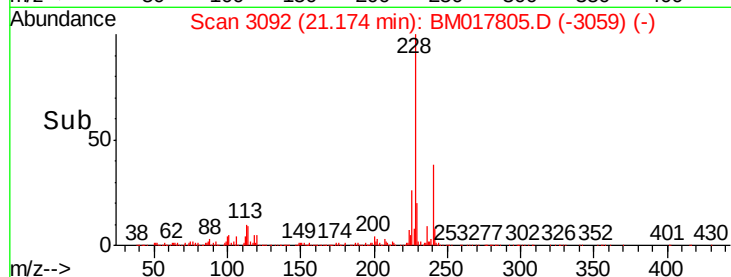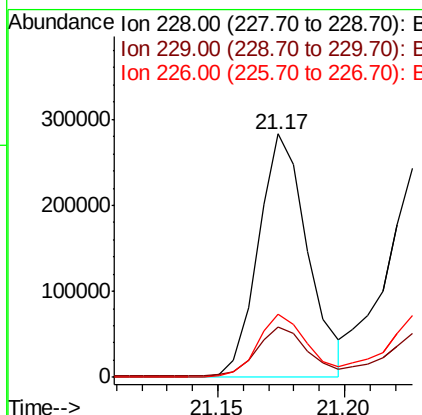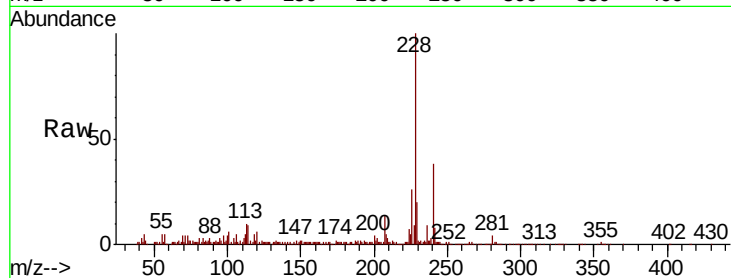

#84
Chrysene
Concen: 5.700 ng/ul
RT: 21.23 min Scan# 3101
Delta R.T. -0.01 min
Lab File: BM017805.D
Acq: 29 Nov 2018 20:46

Tgt Ion:228 Resp: 364627
Ion Ratio Lower Upper
228 100
226 29.6 23.7 35.5
229 21.1 15.8 23.8

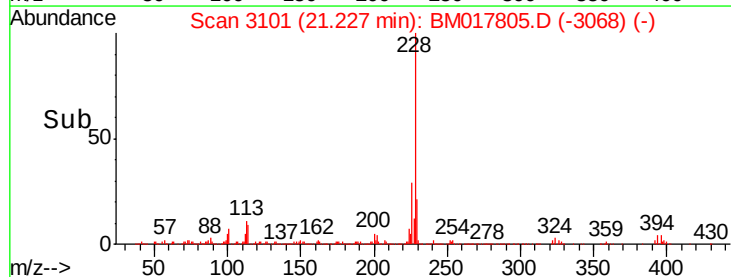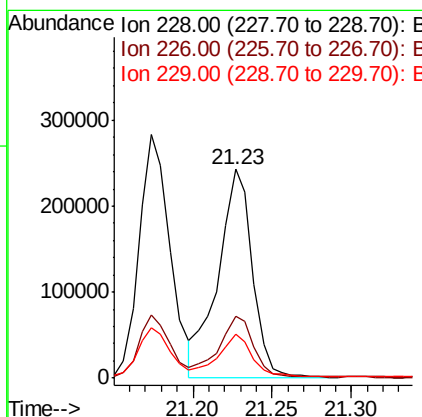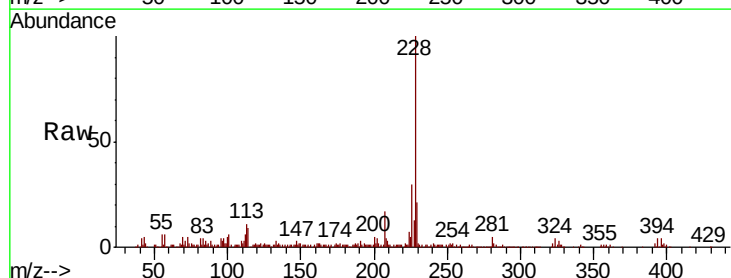

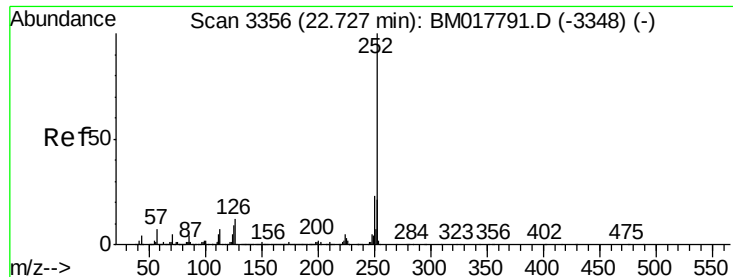

#87

Benzo(b)fluoranthene

Concen: 4.172 ng/ul

RT: 22.73 min Scan# 3356

Delta R.T. -0.00 min

Lab File: BM017805.D

Acq: 29 Nov 2018 20:46


Instrument :

BNA_M




ClientSampleId :

CB4J7

Tgt Ion:	252	Resp:	241463
Ion Ratio	Lower	Upper	
252	100		
253	23.9	17.0	25.4
125	14.2	7.3	10.9#

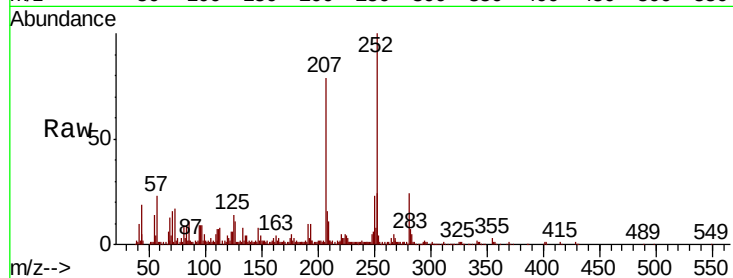

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

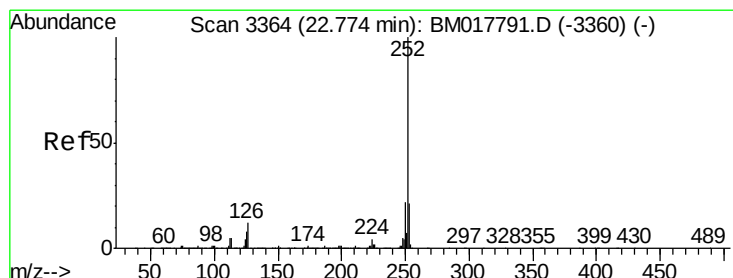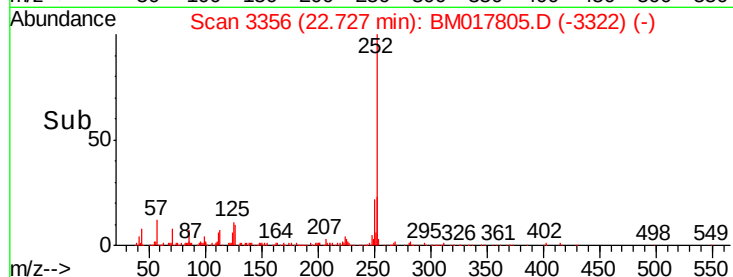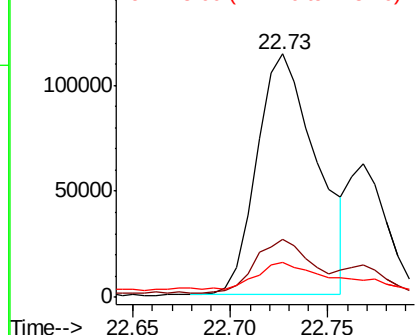

#88

Benzo(k)fluoranthene

Concen: 1.536 ng/ul


RT: 22.77 min Scan# 3363

Delta R.T. -0.01 min

Lab File: BM017805.D

Acq: 29 Nov 2018 20:46

Tgt Ion:	252	Resp:	86399
Ion Ratio	Lower	Upper	
252	100		
253	24.7	17.4	26.0
125	13.0	7.1	10.7#

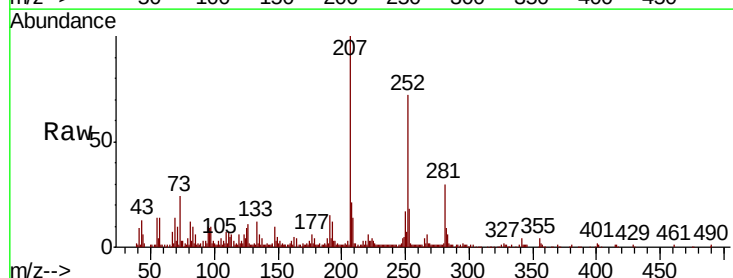

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

