

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM113022\
 Data File : BM037807.D
 Acq On : 30 Nov 2022 17:47
 Operator : CG/JU
 Sample : N5811-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGCE1

Quant Time: Dec 01 00:20:28 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM113022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 01 00:14:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.104	152	4052	0.400	ng/ul	0.00
4) Naphthalene-d8	10.926	136	13845	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.730	164	8141	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.463	188	16080	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.631	240	11808	0.400	ng/ul	# 0.00
23) Perylene-d12	24.116	264	12235	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.434	96	24499	4.540	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.499	152	6371	0.319	ng/ul	0.00
18) Fluoranthene-d10	19.482	212	12615	0.314	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.472	88	1058	0.188	ng/ul#	75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM113022\
Data File : BM037807.D
Acq On : 30 Nov 2022 17:47
Operator : CG/JU
Sample : N5811-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGCE1


Quant Time: Dec 01 00:20:28 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM113022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 01 00:14:21 2022
Response via : Initial Calibration

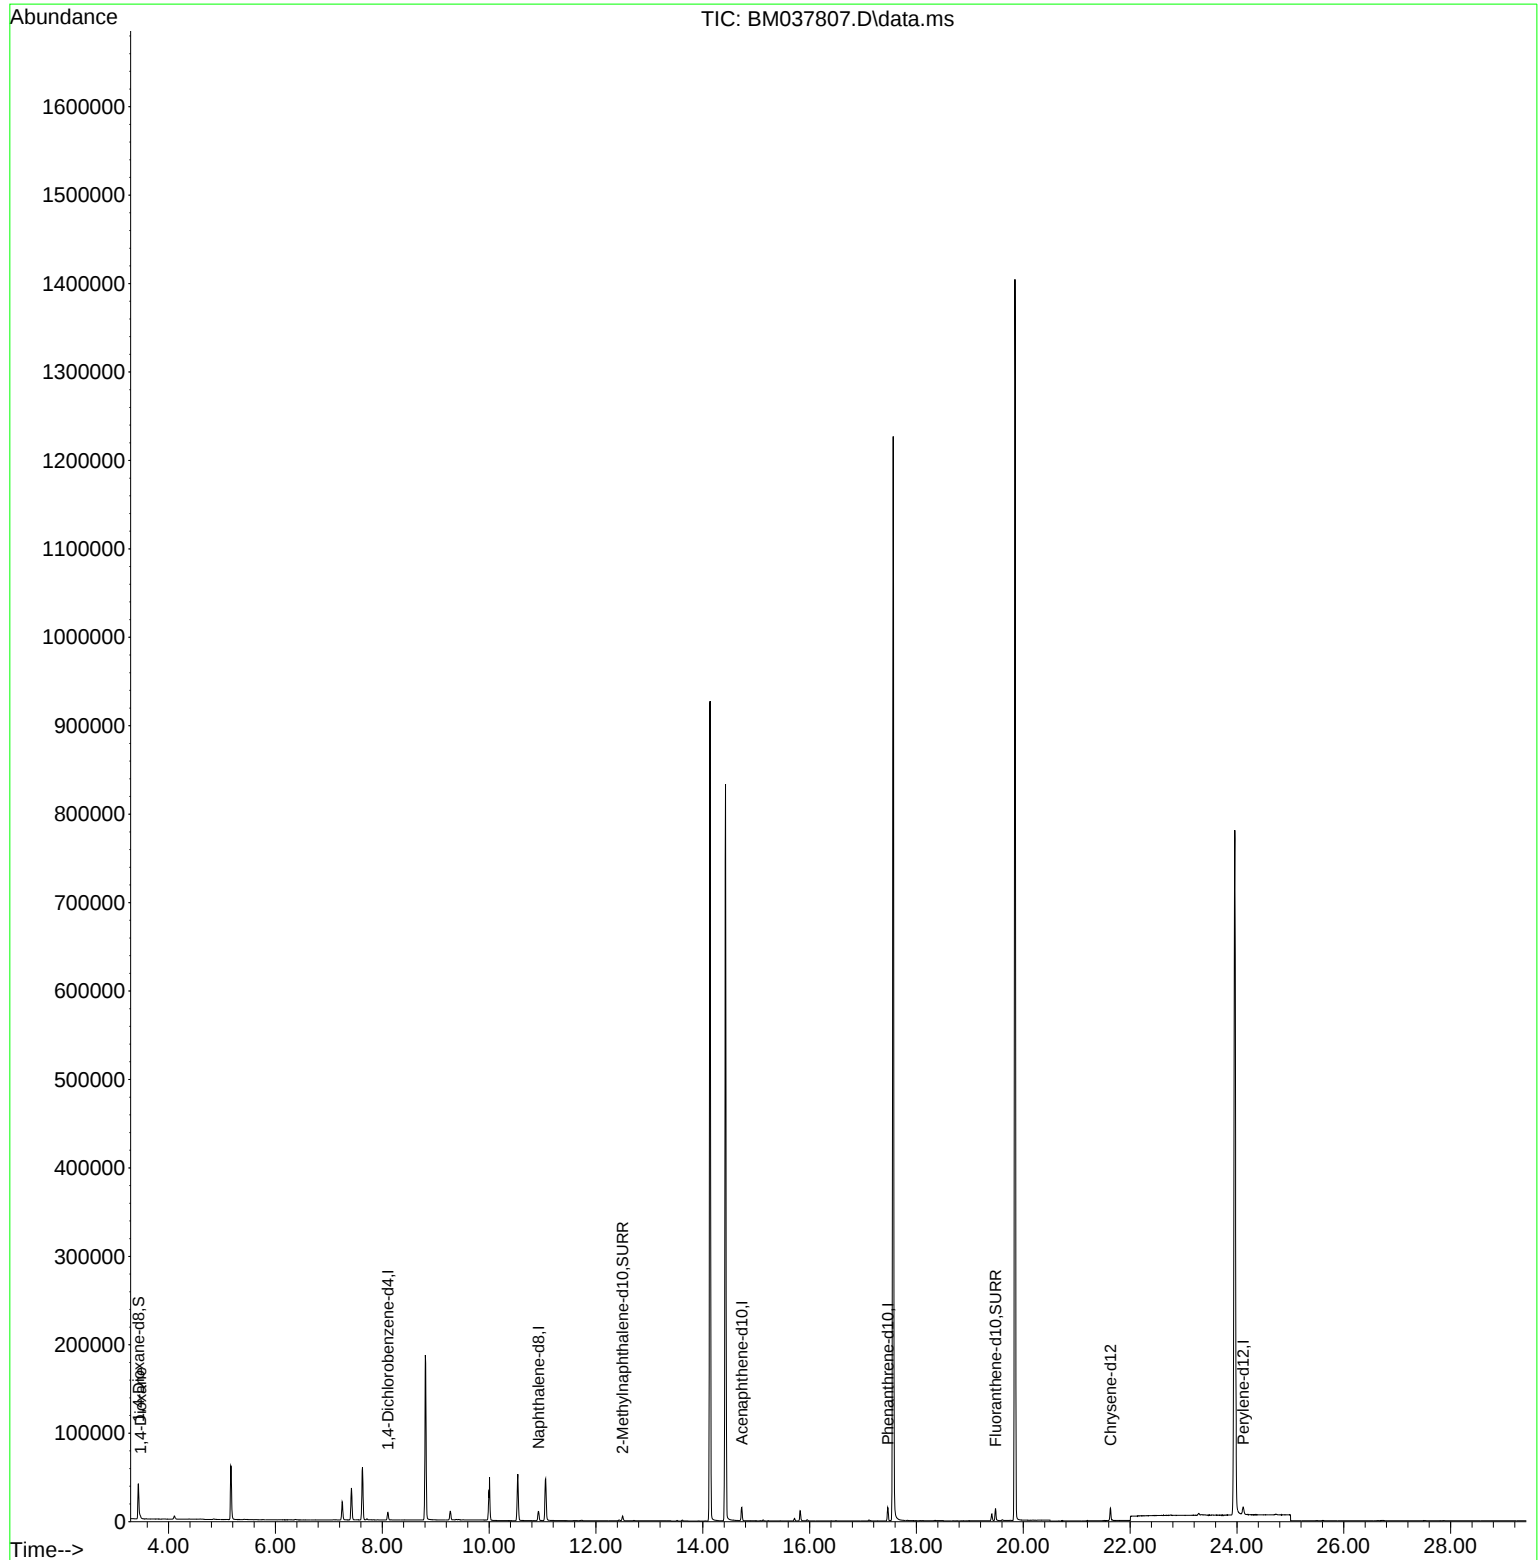

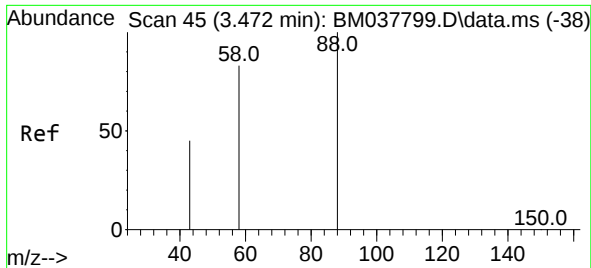

#2
 1,4-Dioxane
 Concen: 0.188 ng/ul
 RT: 3.472 min Scan# 45
 Delta R.T. 0.000 min
 Lab File: BM037807.D
 Acq: 30 Nov 2022 17:47

Instrument :
 BNA_M
 ClientSampleId :
 BGCE1

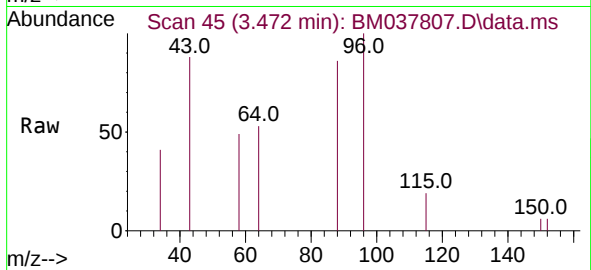

Tgt Ion:	88	Resp:	1058
Ion	Ratio	Lower	Upper
88	100		
43	103.1	102.8	154.2
58	56.6	67.3	100.9

