

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM113022\
 Data File : BM037809.D
 Acq On : 30 Nov 2022 19:02
 Operator : CG/JU
 Sample : N5811-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGCG9

Quant Time: Dec 01 00:20:40 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM113022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 01 00:14:21 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.104	152	4665	0.400	ng/ul	0.00
4) Naphthalene-d8	10.921	136	15448	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.730	164	8868	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.463	188	17485	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.631	240	12616	0.400	ng/ul	# 0.00
23) Perylene-d12	24.116	264	12964	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.434	96	23237	3.740	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.499	152	6445	0.289	ng/ul	0.00
18) Fluoranthene-d10	19.482	212	12588	0.293	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.472	88	628	0.097	ng/ul#	86

(#) = qualifier out of range (m) = manual integration (+) = signals summed

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM113022\  
Data File : BM037809.D  
Acq On    : 30 Nov 2022  19:02  
Operator  : CG/JU  
Sample    : N5811-04  
Misc      :  
ALS Vial  : 14    Sample Multiplier: 1
```


Quant Time: Dec 01 00:20:40 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM113022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 01 00:14:21 2022
Response via : Initial Calibration

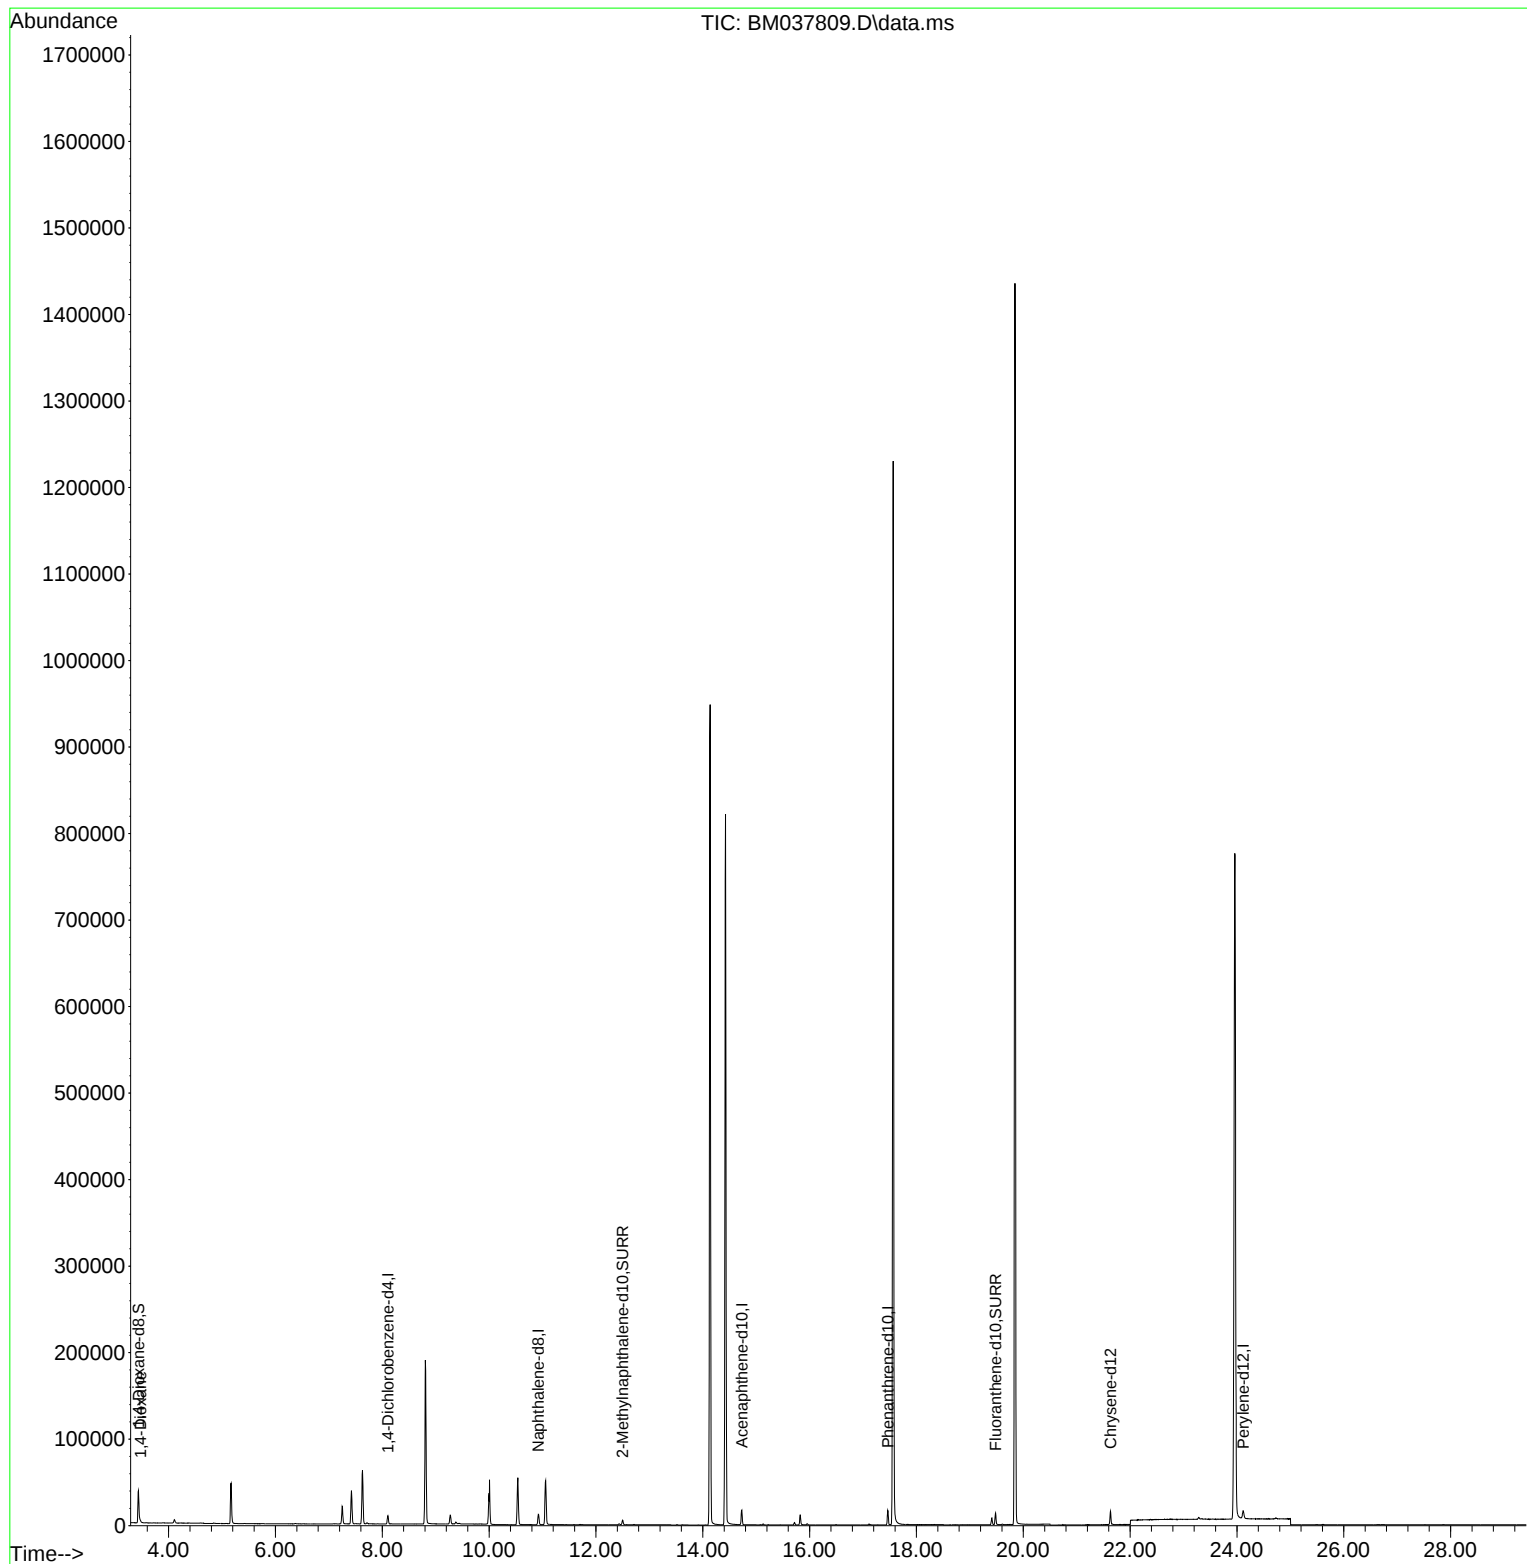

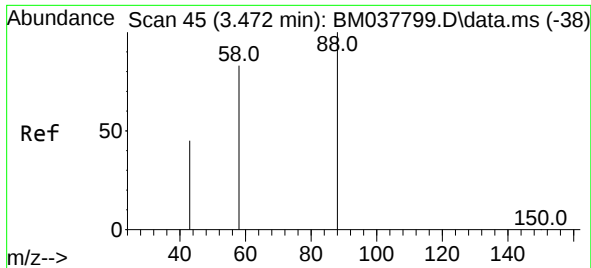

#2
 1,4-Dioxane
 Concen: 0.097 ng/ul
 RT: 3.472 min Scan# 41
 Delta R.T. 0.000 min
 Lab File: BM037809.D
 Acq: 30 Nov 2022 19:02

Instrument :
 BNA_M
 ClientSampleId :
 BGCG9

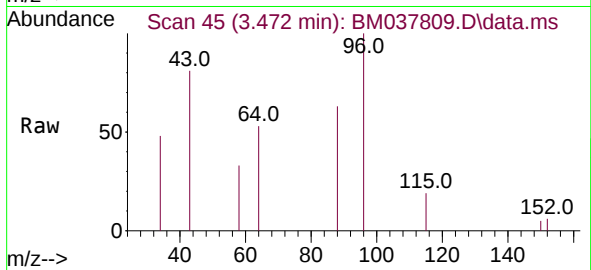

Tgt Ion:	88	Resp:	628
Ion	Ratio	Lower	Upper
88	100		
43	128.4	102.8	154.2
58	51.7	67.3	100.9

