

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM120118\
 Data File : BM017825.D
 Acq On : 30 Nov 2018 15:57
 Operator : JU/SJ
 Sample : PB115224BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK24

Quant Time: Nov 30 16:46:58 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 30 15:55:15 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	174904	20.00	ng/ul	0.00
18) Naphthalene-d8	10.35	136	765031	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.23	164	434855	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.99	188	925579	20.00	ng/ul	0.00
77) Chrysene-d12	21.19	240	734101	20.00	ng/ul	0.00
85) Perylene-d12	23.38	264	652135	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.18	96	26143	6.84	ng/uL	0.00
5) Phenol-d5	6.77	99	539195	33.75	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.93	67	344811	35.80	ng/ul	0.00
9) 2-Chlorophenol-d4	7.12	132	464311	37.15	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	450252	34.50	ng/ul	0.00
19) Nitrobenzene-d5	8.74	128	231383	39.38	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	263317	39.11	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.99	165	439309	34.27	ng/ul	0.00
29) 4-Chloroaniline-d4	10.50	131	640278	58.21	ng/ul	0.00
43) Dimethylphthalate-d6	13.65	166	1517813	40.23	ng/ul	0.00
46) Acenaphthylene-d8	13.92	160	1872904	41.02	ng/ul	0.00
51) 4-Nitrophenol-d4	14.46	143	199952	29.15	ng/ul	0.00
57) Fluorene-d10	15.23	176	1287704	39.52	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.37	200	214070	32.35	ng/ul	0.00
70) Anthracene-d10	17.09	188	1963529	42.61	ng/ul	0.00
78) Pyrene-d10	19.39	212	1927976	54.28	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.24	264	1532854	43.34	ng/ul	0.00


Target Compounds				Ovalue
45) 2,6-Dinitrotoluene	13.65	165	10394	1.447 ng/ul#




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM120118\
Data File : BM017825.D
Acq On : 30 Nov 2018 15:57
Operator : JU/SJ
Sample : PB115224BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK24

Quant Time: Nov 30 16:46:58 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM11918MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 30 15:55:15 2018
Response via : Initial Calibration

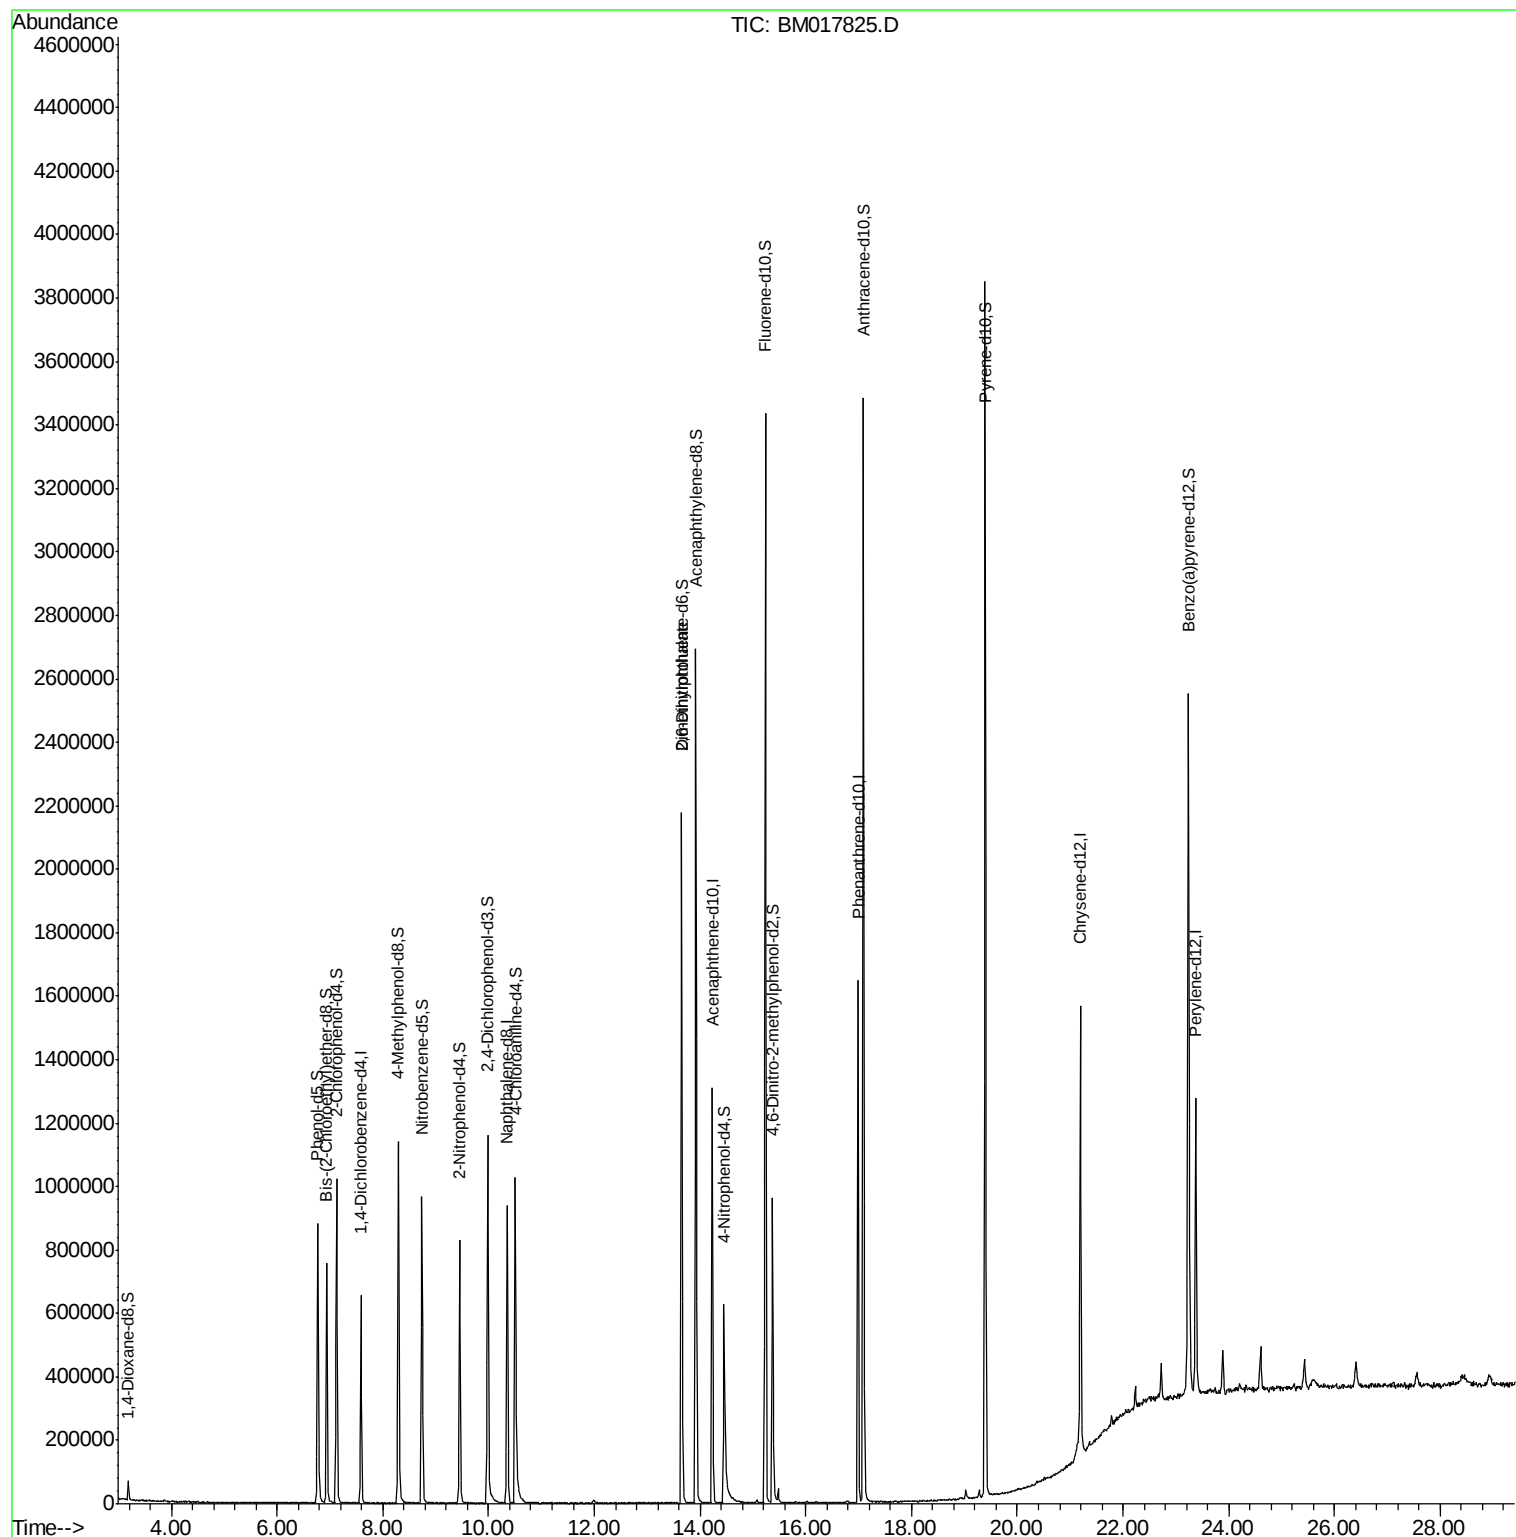

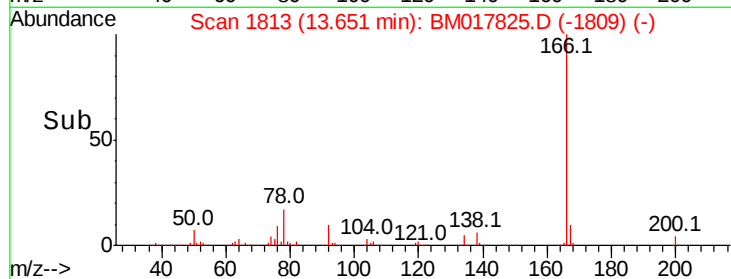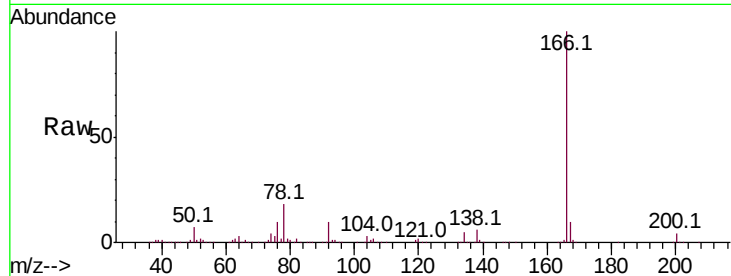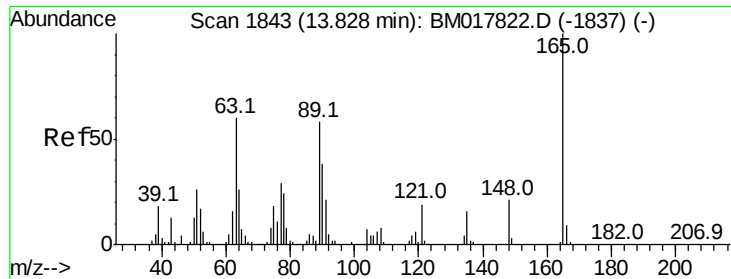

#45

2,6-Dinitrotoluene

Concen: 1.447 ng/ul

RT: 13.65 min Scan# 1813

Delta R.T. -0.18 min

Lab File: BM017825.D

Acq: 30 Nov 2018 15:57

Instrument :

BNA_M

ClientSampleId :

SBLK24

Tot Ion:165 Resp: 10394

Ion Ratio Lower Upper

165 100

89 0.0 48.0 72.0#

121 41.9 17.0 25.6#

