

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM120118\
 Data File : BM017823.D
 Acq On : 30 Nov 2018 14:36
 Operator : JU/SJ
 Sample : J5945-19
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ETOB2

Quant Time: Nov 30 15:13:49 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Nov 29 00:55:29 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	209442	20.00	ng/ul	0.00
18) Naphthalene-d8	10.36	136	917559	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.23	164	513788	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.99	188	1080032	20.00	ng/ul	0.00
77) Chrysene-d12	21.20	240	830994	20.00	ng/ul	0.00
85) Perylene-d12	23.38	264	777246	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.19	96	21952	4.80	ng/uL	0.00
5) Phenol-d5	6.78	99	519657	27.17	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.94	67	342064	29.66	ng/ul	0.00
9) 2-Chlorophenol-d4	7.13	132	435210	29.08	ng/ul	0.00
13) 4-Methylphenol-d8	8.30	113	459459	29.40	ng/ul	0.00
19) Nitrobenzene-d5	8.75	128	234383	33.26	ng/ul	0.00
22) 2-Nitrophenol-d4	9.46	143	274355	33.97	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.99	165	461615	30.03	ng/ul	0.00
29) 4-Chloroaniline-d4	10.51	131	656948	49.80	ng/ul	0.00
43) Dimethylphthalate-d6	13.66	166	1574736	35.32	ng/ul	0.00
46) Acenaphthylene-d8	13.93	160	2074778	38.46	ng/ul	0.00
51) 4-Nitrophenol-d4	14.46	143	219182	27.04	ng/ul	0.00
57) Fluorene-d10	15.23	176	1378242	35.80	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.37	200	235282	30.47	ng/ul	0.00
70) Anthracene-d10	17.09	188	2010427	37.39	ng/ul	0.00
78) Pyrene-d10	19.39	212	2024076	50.34	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.24	264	1870269	44.37	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.70	163	92013	2.130	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM120118\
Data File : BM017823.D
Acq On : 30 Nov 2018 14:36
Operator : JU/SJ
Sample : J5945-19
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ETOB2

Quant Time: Nov 30 15:13:49 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM11918MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Nov 29 00:55:29 2018
Response via : Initial Calibration

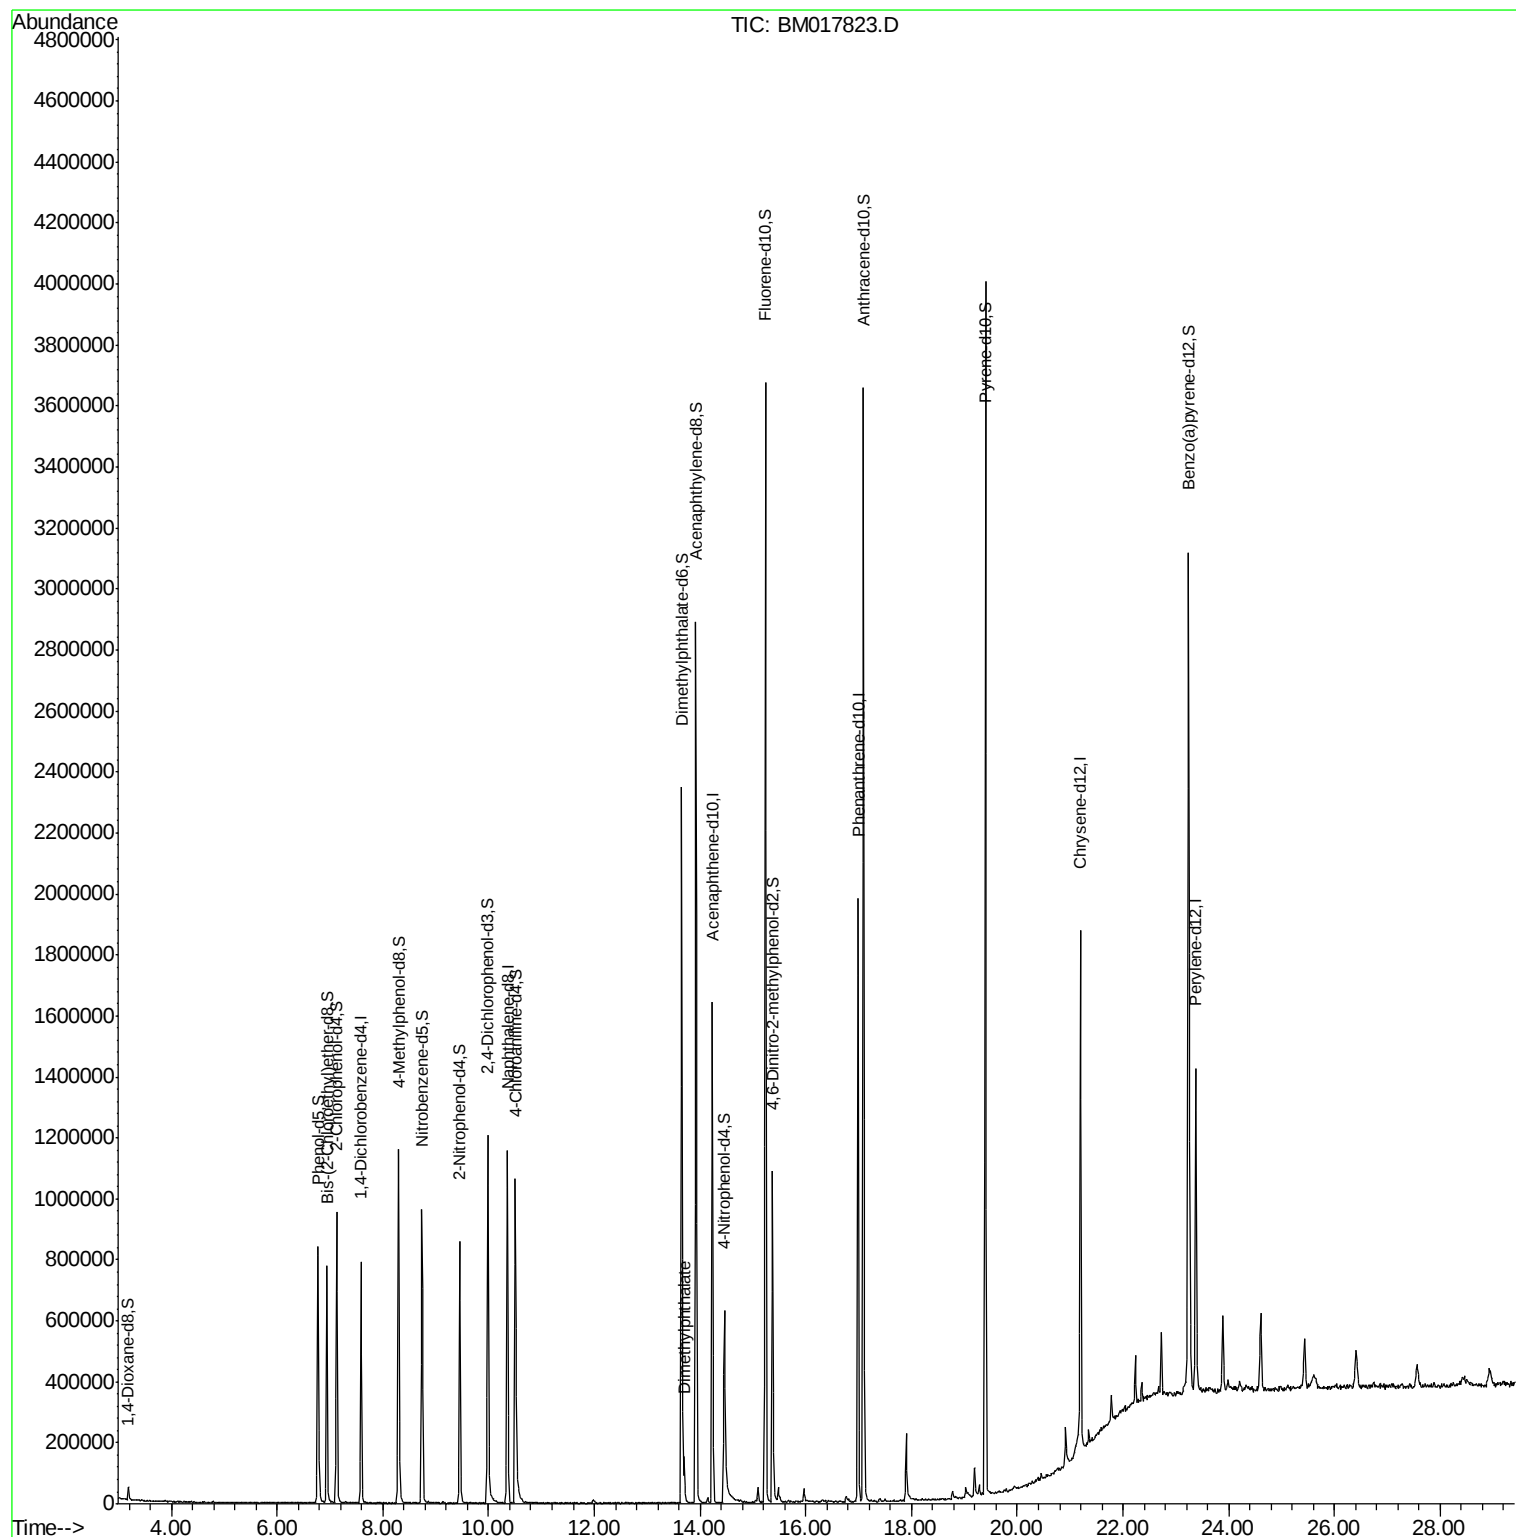

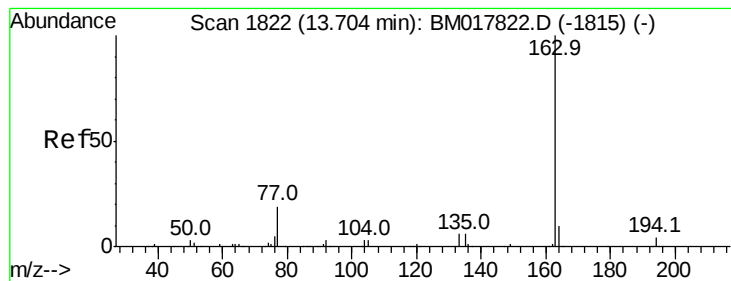

#44

Dimethylphthalate

Concen: 2.130 ng/ul

RT: 13.70 min Scan# 1822

Delta R.T. 0.00 min

Lab File: BM017823.D

Acq: 30 Nov 2018 14:36

Instrument :

BNA_M

ClientSampleId :

ETOB2


Tot Ion:163 Resp: 92013

Ion Ratio Lower Upper

163 100

194 4.5 3.4 5.0

164 9.4 8.1 12.1

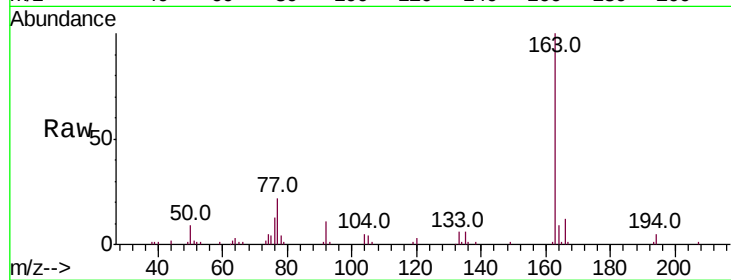

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

