
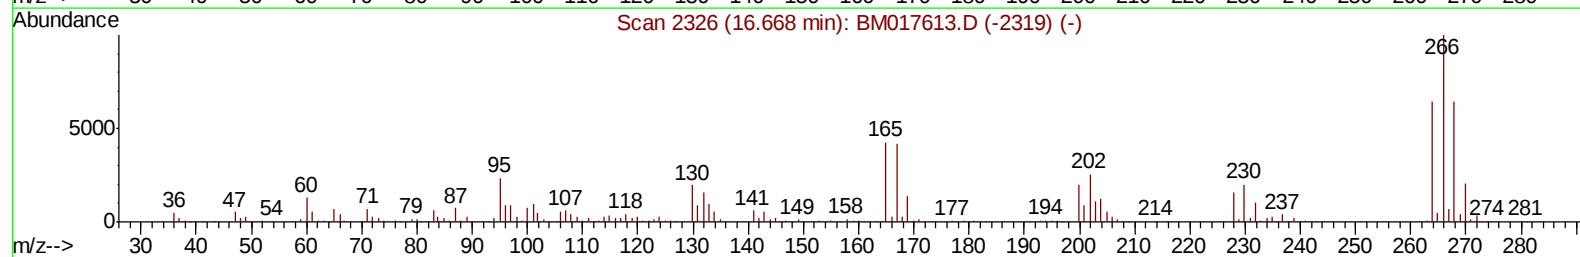
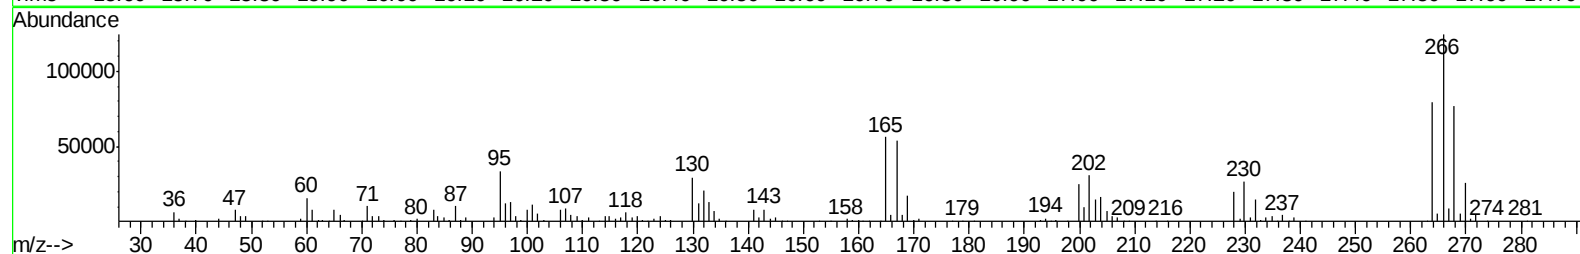


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120218\
Data File : BM017870.D
Acq On : 01 Dec 2018 23:53
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 03 05:53:48 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM111218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 12 18:37:25 2018
Response via : Initial Calibration

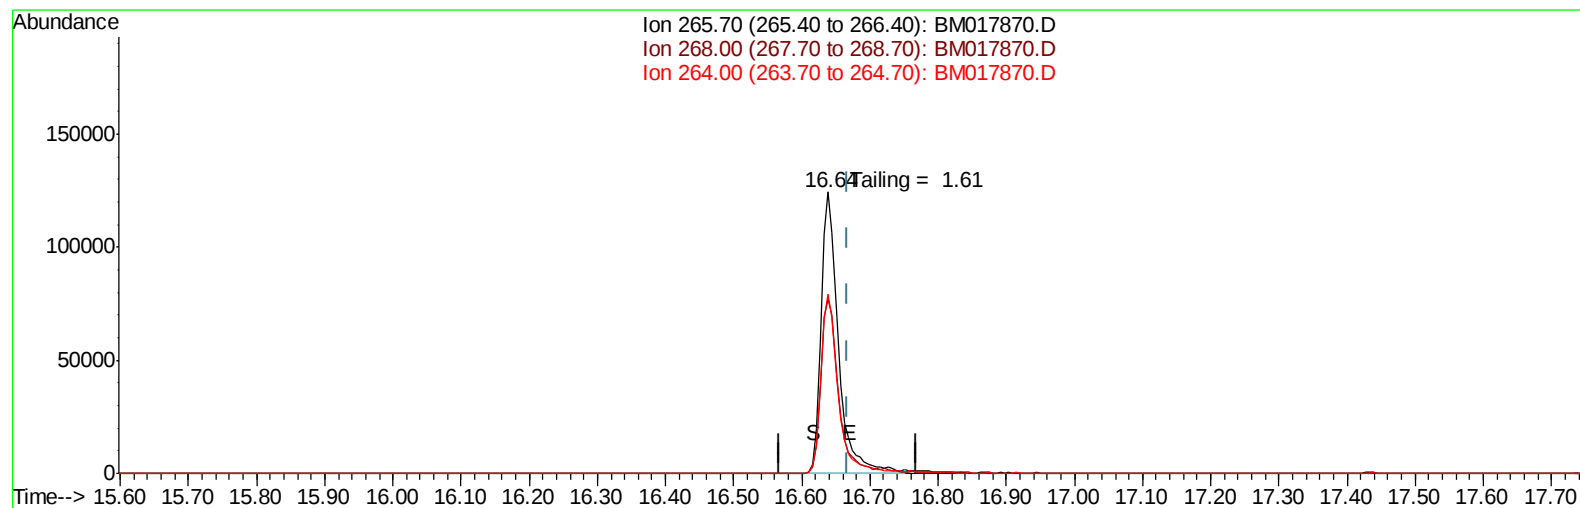

TIC: BM017870.D

(70) Pentachlorophenol (C)




16.639min (-0.030) 0.00ng

response 218220

Ion	Exp%	Act%
265.70	100	100
268.00	64.60	61.96
264.00	64.10	63.71
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120218\
 Data File : BM017870.D
 Acq On : 01 Dec 2018 23:53
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 03 05:53:48 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM111218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 12 18:37:25 2018
 Response via : Initial Calibration

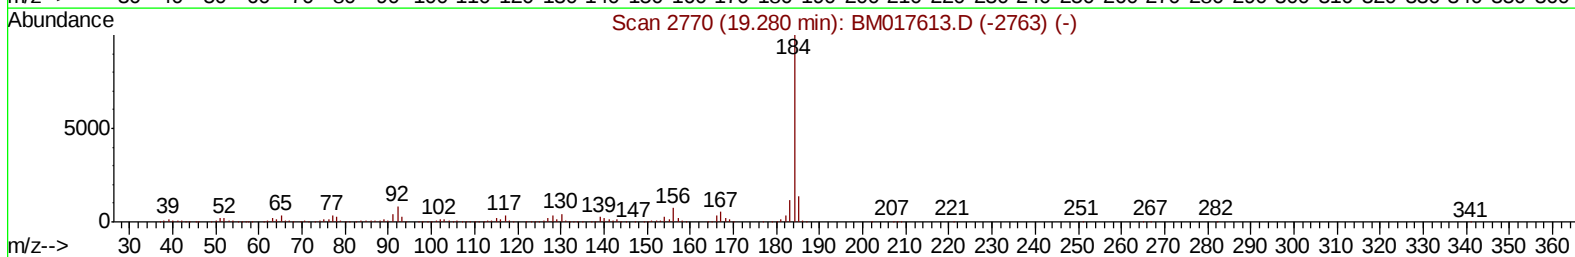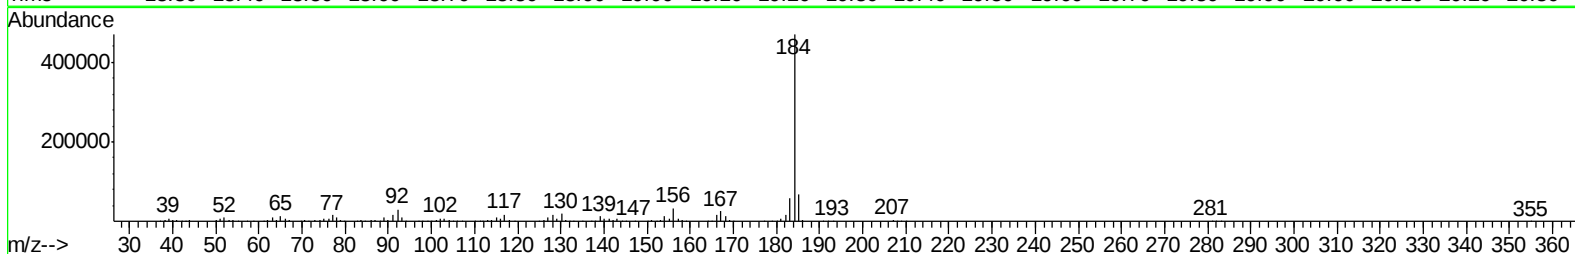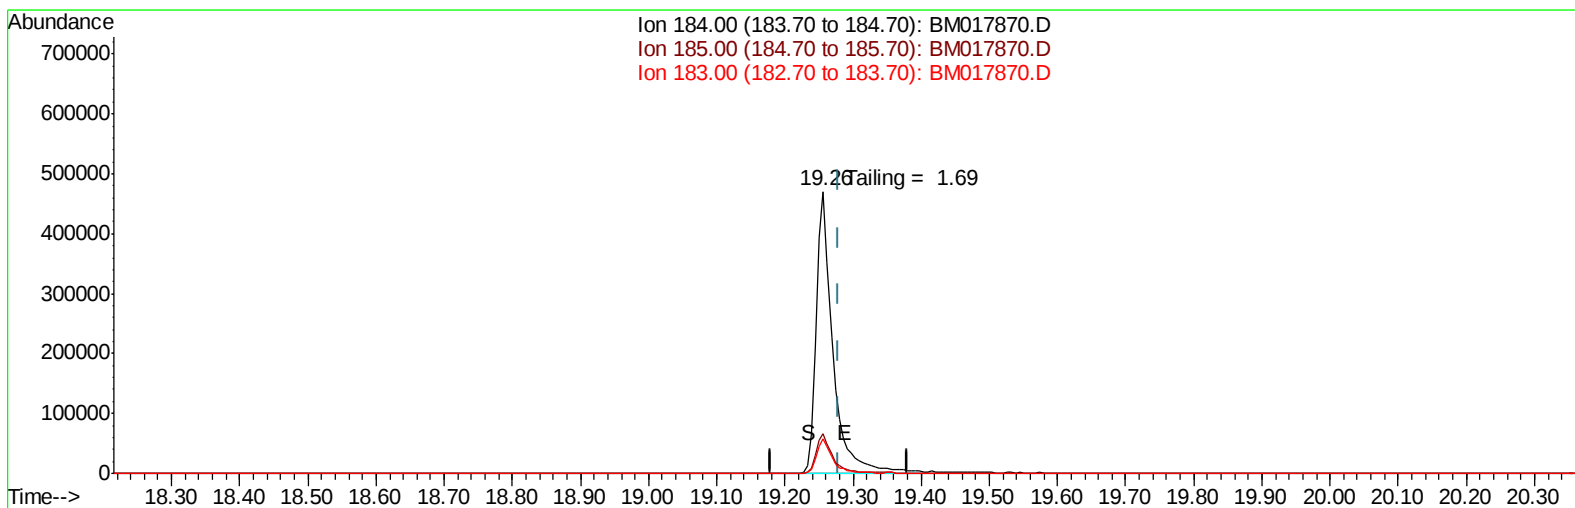

TIC: BM017870.D

(77) Benzidine

19.256min (-0.024) 224241.56ng

response 788636

Ion	Exp%	Act%
184.00	100	100
185.00	14.00	14.18
183.00	11.90	12.21
0.00	0.00	0.00