


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM120218\
 Data File : BM017870.D
 Acq On : 01 Dec 2018 23:53
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM111218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 12 18:37:25 2018

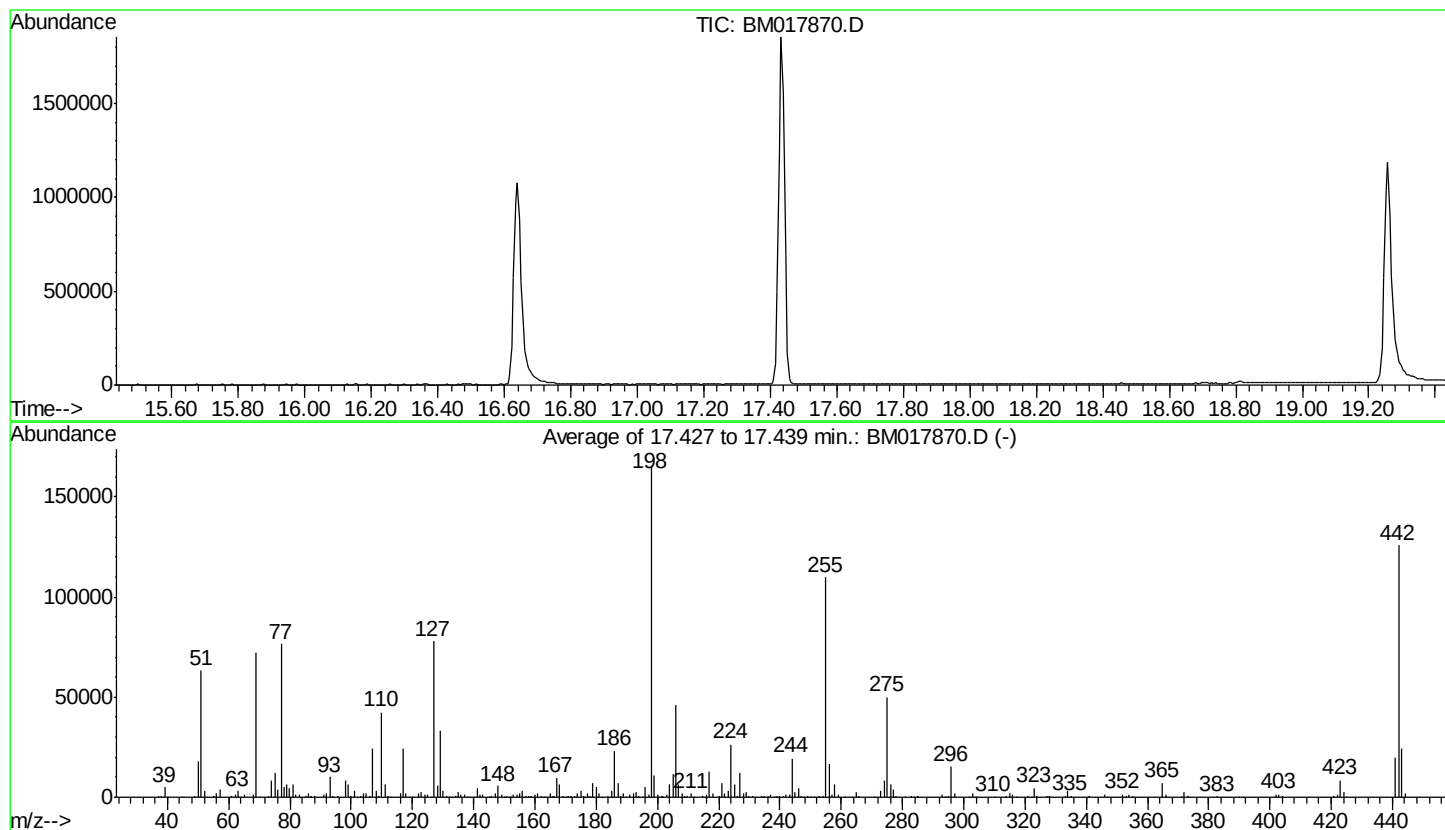

AutoFind: Scans 2455, 2456, 2457; Background Corrected with Scan 2449

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.2	63224	PASS
68	69	0.00	2	2.0	1463	PASS
69	198	0.00	100	43.6	72261	PASS
70	69	0.00	2	0.5	332	PASS
127	198	10	80	47.0	77885	PASS
197	198	0.00	2	0.7	1129	PASS
198	198	100	100	100.0	165589	PASS
199	198	5	9	6.5	10819	PASS
275	198	10	60	30.2	49994	PASS
365	198	1	100	4.4	7337	PASS
441	198	0.01	100	11.9	19680	PASS
442	198	50	100	76.0	125773	PASS
443	442	15	24	19.2	24112	PASS