

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM120319\
 Data File : BM023967.D
 Acq On : 03 Dec 2019 11:42
 Operator : JU
 Sample : K5889-11
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JLLQ8

Quant Time: Dec 03 12:14:26 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM112719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 03 11:33:32 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.49	152	387102	20.00	ng/ul	0.00
18) Naphthalene-d8	10.26	136	1702275	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.14	164	1102833	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.90	188	2339574	20.00	ng/ul	0.00
78) Chrysene-d12	21.11	240	1804184	20.00	ng/ul	0.00
86) Perylene-d12	23.25	264	1778435	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.05	96	5320	0.61	ng/uL	0.01
5) Phenol-d5	6.67	99	725131	21.37	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.83	67	434660	22.03	ng/ul	0.00
9) 2-Chlorophenol-d4	7.02	132	583819	22.26	ng/ul	0.00
13) 4-Methylphenol-d8	8.20	113	607656	22.70	ng/ul	0.00
19) Nitrobenzene-d5	8.64	128	297349	22.51	ng/ul	0.00
22) 2-Nitrophenol-d4	9.36	143	343805	22.89	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.89	165	603730	21.23	ng/ul	0.00
29) 4-Chloroaniline-d4	10.40	131	861705	27.61	ng/ul	0.00
44) Dimethylphthalate-d6	13.57	166	1990449	23.23	ng/ul	0.00
47) Acenaphthylene-d8	13.83	160	2506470	24.96	ng/ul	0.00
52) 4-Nitrophenol-d4	14.37	143	249704	17.33	ng/ul	0.00
58) Fluorene-d10	15.14	176	1717225	23.81	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.29	200	213021	14.50	ng/ul	0.00
71) Anthracene-d10	17.00	188	2657404	23.78	ng/ul	0.00
79) Pyrene-d10	19.30	212	2746071	29.46	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.12	264	2163002	23.01	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.62	163	143662	1.713	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM120319\
Data File : BM023967.D
Acq On : 03 Dec 2019 11:42
Operator : JU
Sample : K5889-11
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JLLQ8

Quant Time: Dec 03 12:14:26 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM112719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 03 11:33:32 2019
Response via : Initial Calibration

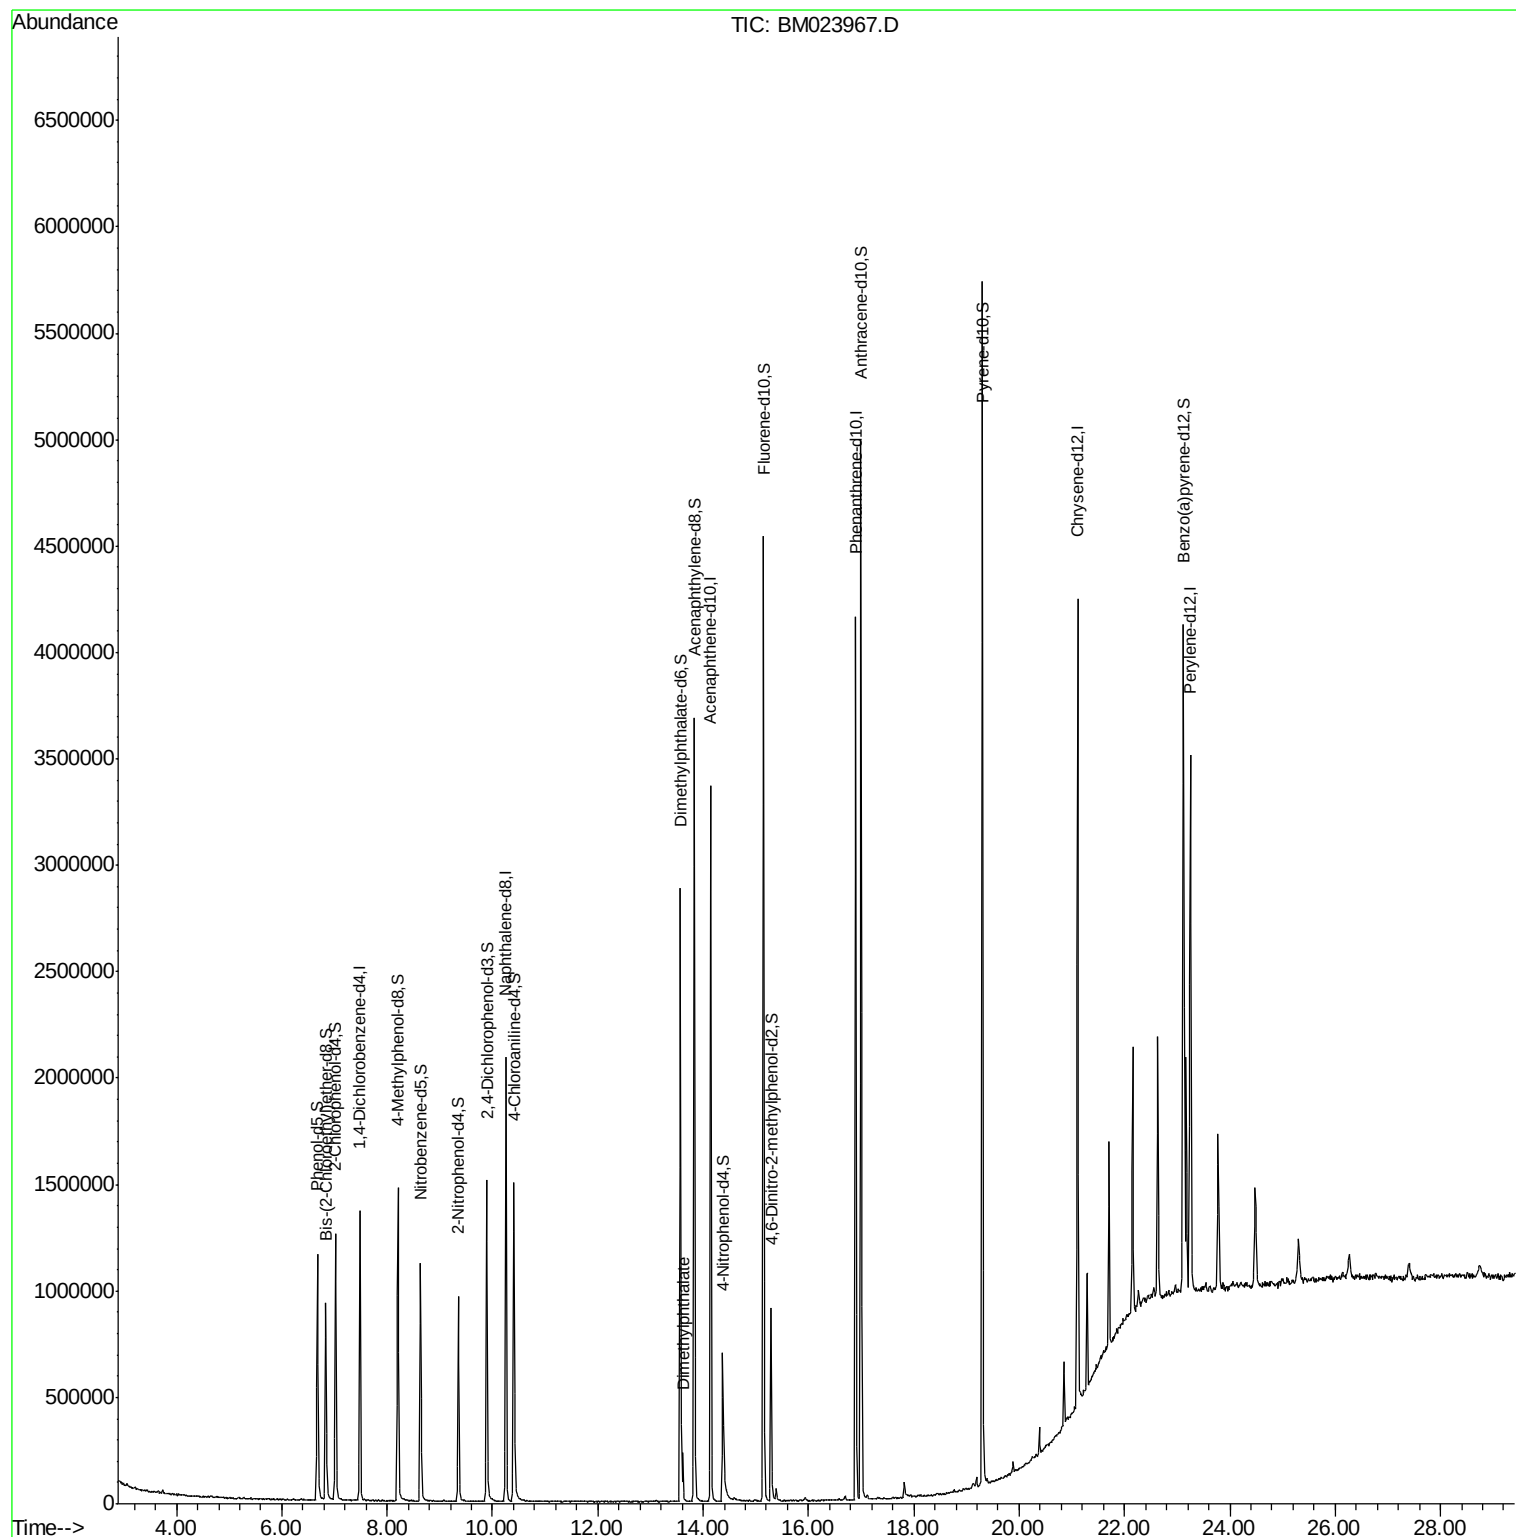

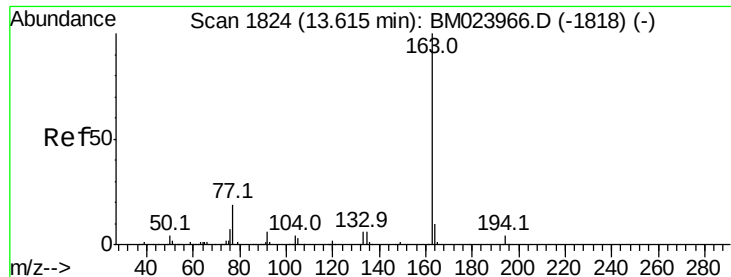

#45

Dimethylphthalate

Concen: 1.713 ng/ul

RT: 13.62 min Scan# 1824

Delta R.T. 0.00 min

Lab File: BM023967.D

Acq: 03 Dec 2019 11:42

Instrument :

BNA_M

ClientSampleId :

JLLQ8


Tot Ion:163 Resp: 143662

Ion Ratio Lower Upper

163 100

194 4.3 3.2 4.8

164 10.7 8.0 12.0

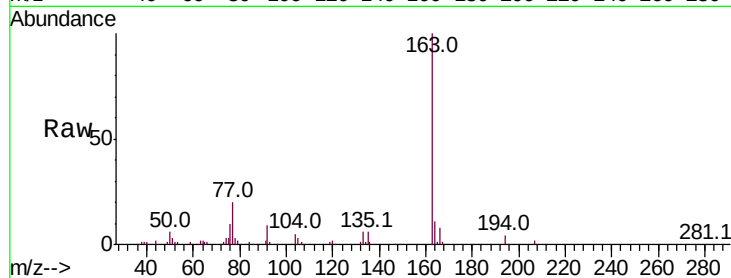

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

